

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
 Data File : BM044167.D
 Acq On : 17 Feb 2024 09:18
 Operator : MA/JU
 Sample : P1402-15
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/19/2024
 Supervised By :mohammad ahmed 02/19/2024

Quant Time: Feb 18 23:55:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.901	152	7960	0.400	ng/u1	0.00
4) Naphthalene-d8	10.699	136	26131	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.543	164	13628	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.292	188	28330m	0.400	ng/u1	0.00
17) Chrysene-d12	21.497	240	17570m	0.400	ng/u1	0.00
23) Perylene-d12	23.888	264	22288	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	46018	4.082	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.294	152	14612	0.399	ng/u1	0.00
18) Fluoranthene-d10	19.326	212	31141	0.594	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.390	88	4143	0.368	ng/u1	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021524\
Data File : BM044167.D
Acq On : 17 Feb 2024 09:18
Operator : MA/JU
Sample : P1402-15
Misc :
ALS Vial : 79 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AD4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/19/2024
Supervised By :mohammad ahmed 02/19/2024


Quant Time: Feb 18 23:55:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

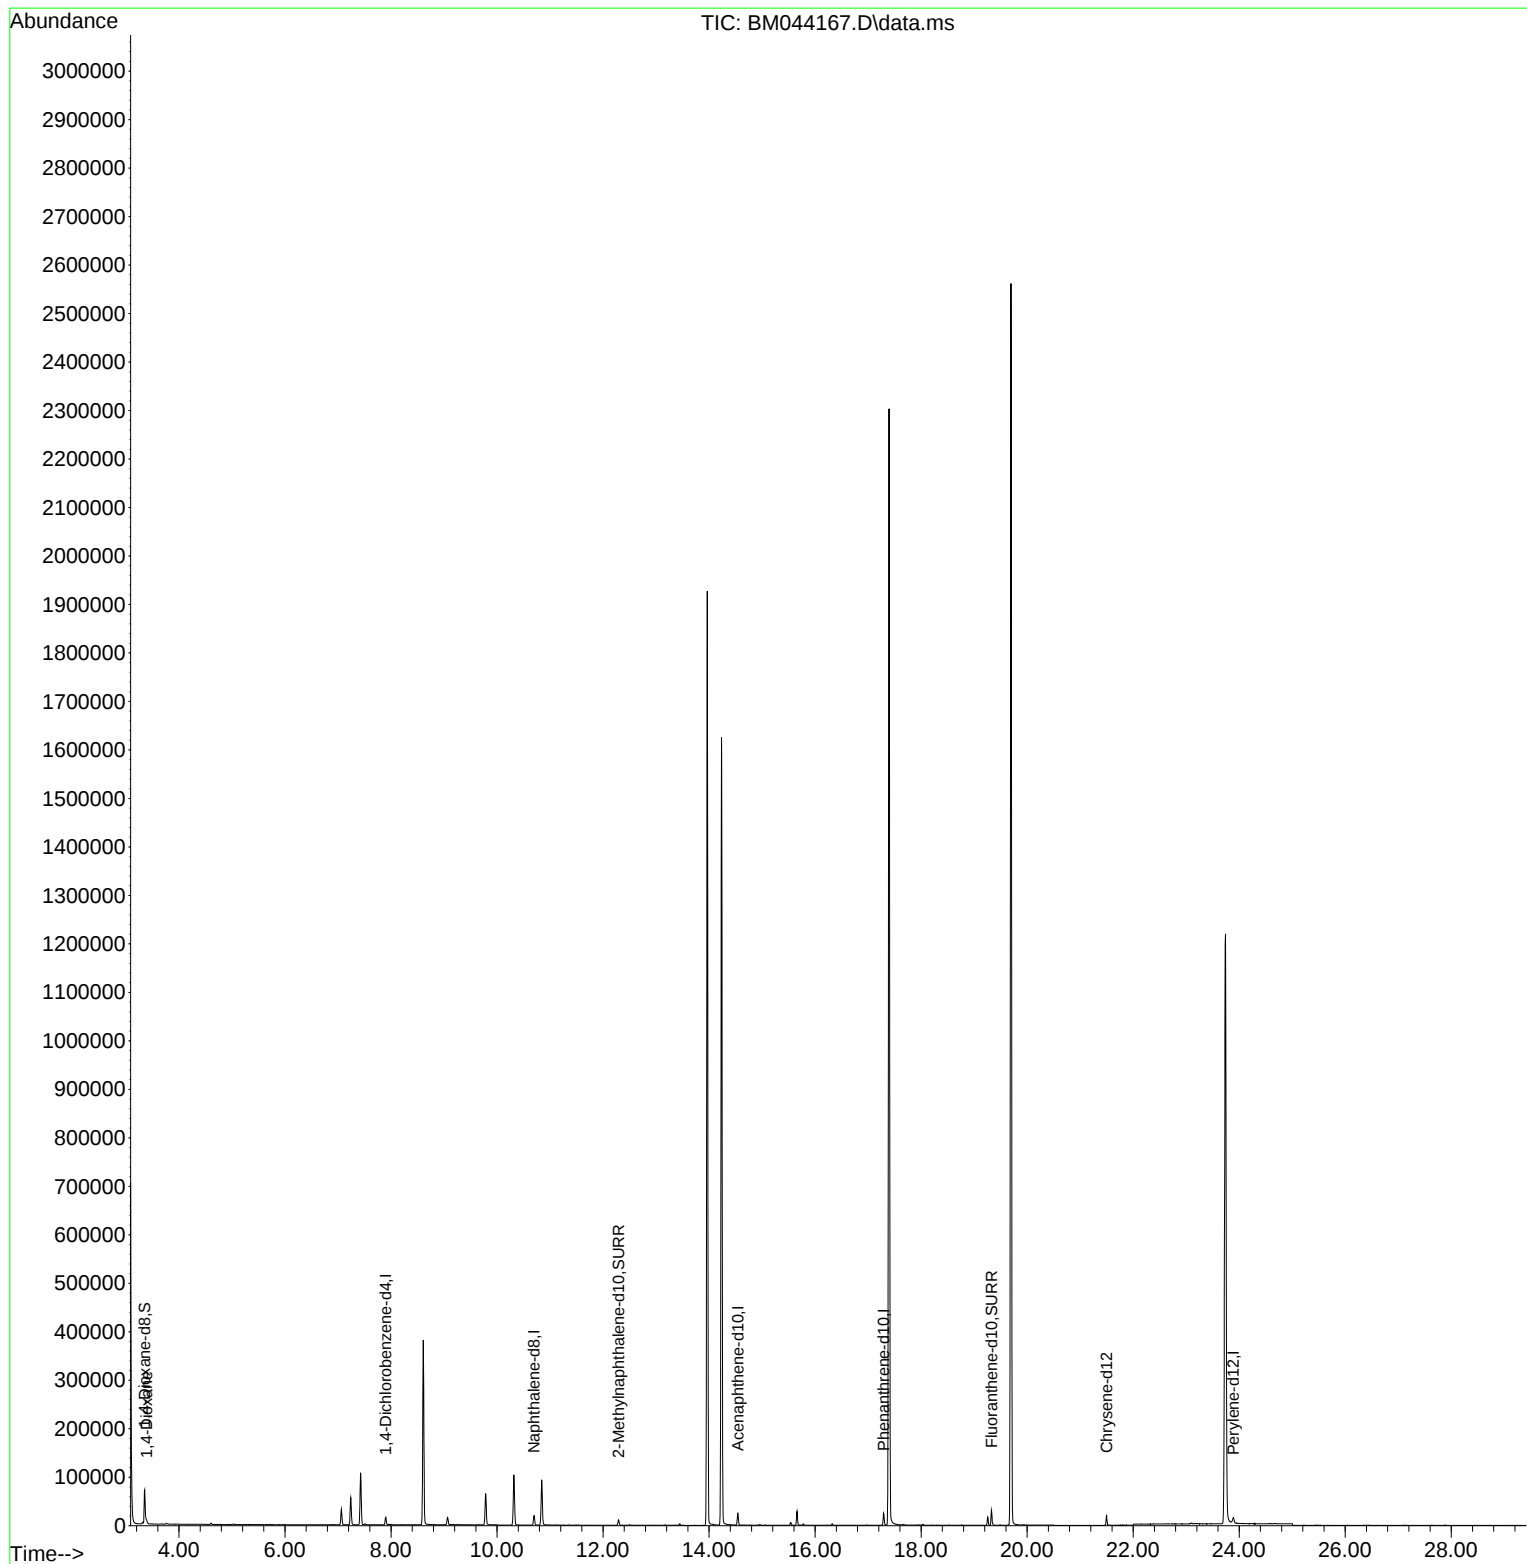

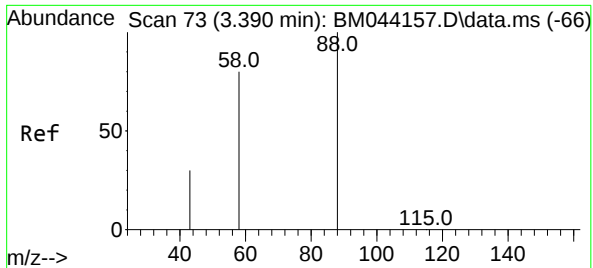

#2
 1,4-Dioxane
 Concen: 0.368 ng/ul
 RT: 3.390 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BM044167.D
 Acq: 17 Feb 2024 09:18

Instrument :
 BNA_M
 ClientSampleId :
 C0AD4

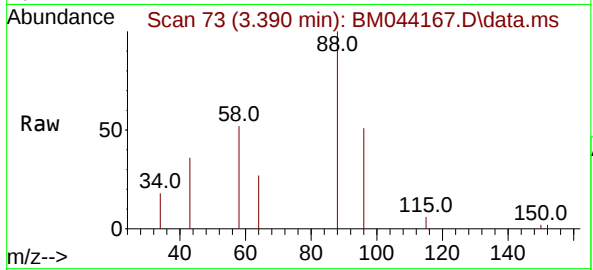

Tgt Ion: 88 Resp: 414

Ion	Ratio	Lower	Upper
88	100		
43	35.8	32.2	48.2
58	51.5	40.6	60.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/19/2024
 Supervised By :mohammad ahmed 02/19/2024

