


Data Path : Z:\HPCHEM1\BNA_M\Data\BM021715\
 Data File : BM000536.D
 Acq On : 16 Feb 2015 18:48
 Operator : TP/IZ
 Sample : DFTPP24
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP24

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-SIM-BM021215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 12 16:45:55 2015

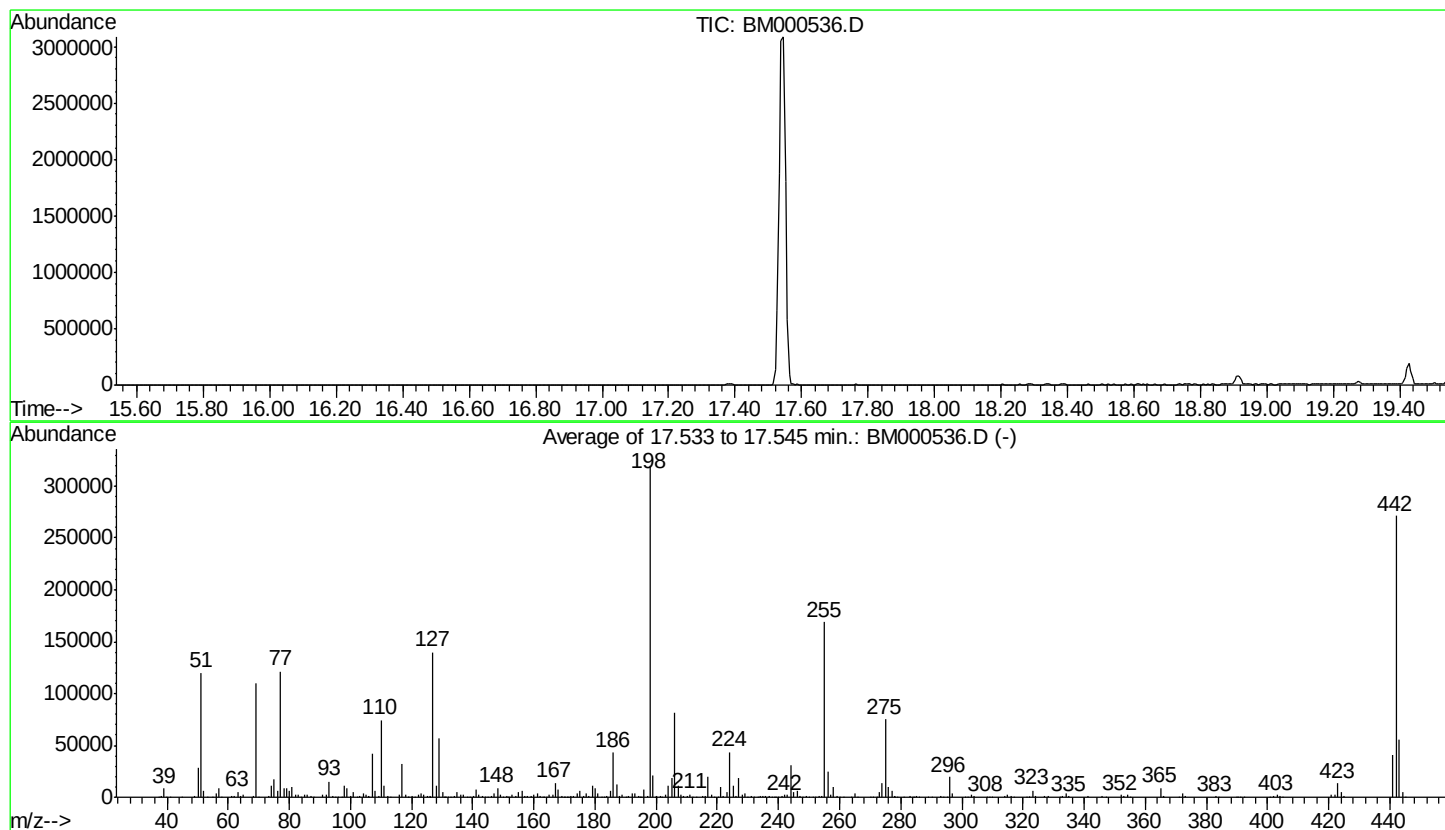

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	120362	PASS
68	69	0.00	2	1.7	1824	PASS
69	198	0.00	100	34.4	109968	PASS
70	69	0.00	2	0.5	536	PASS
127	198	10	80	43.7	139848	PASS
197	198	0.00	2	0.5	1640	PASS
198	198	100	100	100.0	319744	PASS
199	198	5	9	6.8	21599	PASS
275	198	10	60	23.4	74973	PASS
365	198	1	100	2.8	8997	PASS
441	443	0.01	100	72.7	40472	PASS
442	198	50	100	84.9	271466	PASS
443	442	15	24	20.5	55661	PASS