

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021618\
 Data File : BM014260.D
 Acq On : 16 Feb 2018 09:41
 Operator : SJ/JU
 Sample : PB106593BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 16 12:30:49 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 15 01:12:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	81546	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	361669	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.19	164	241976	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.95	188	576350	20.00	ng/ul	0.00
75) Chrysene-d12	21.16	240	578965	20.00	ng/ul	0.00
83) Perylene-d12	23.33	264	491286	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.11	96	8575	4.50	ng/uL	0.00
5) Phenol-d5	6.73	99	177740	25.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	109367	26.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.07	132	144804	27.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	157525	26.12	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	79301	29.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	83512	30.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	135062	23.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	182472	32.32	ng/ul	0.00
43) Dimethylphthalate-d6	13.62	166	644732	32.26	ng/ul	0.00
46) Acenaphthylene-d8	13.88	160	750524	30.46	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	49737	18.03	ng/ul	0.01
57) Fluorene-d10	15.19	176	546587	30.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	77680	22.47	ng/ul	0.00
70) Anthracene-d10	17.05	188	888123	31.94	ng/ul	0.00
76) Pyrene-d10	19.36	212	1027845	34.42	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.19	264	786519	32.89	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.26	70	5576	1.069	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021618\
Data File : BM014260.D
Acq On : 16 Feb 2018 09:41
Operator : SJ/JU
Sample : PB106593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 16 12:30:49 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 15 01:12:03 2018
Response via : Initial Calibration

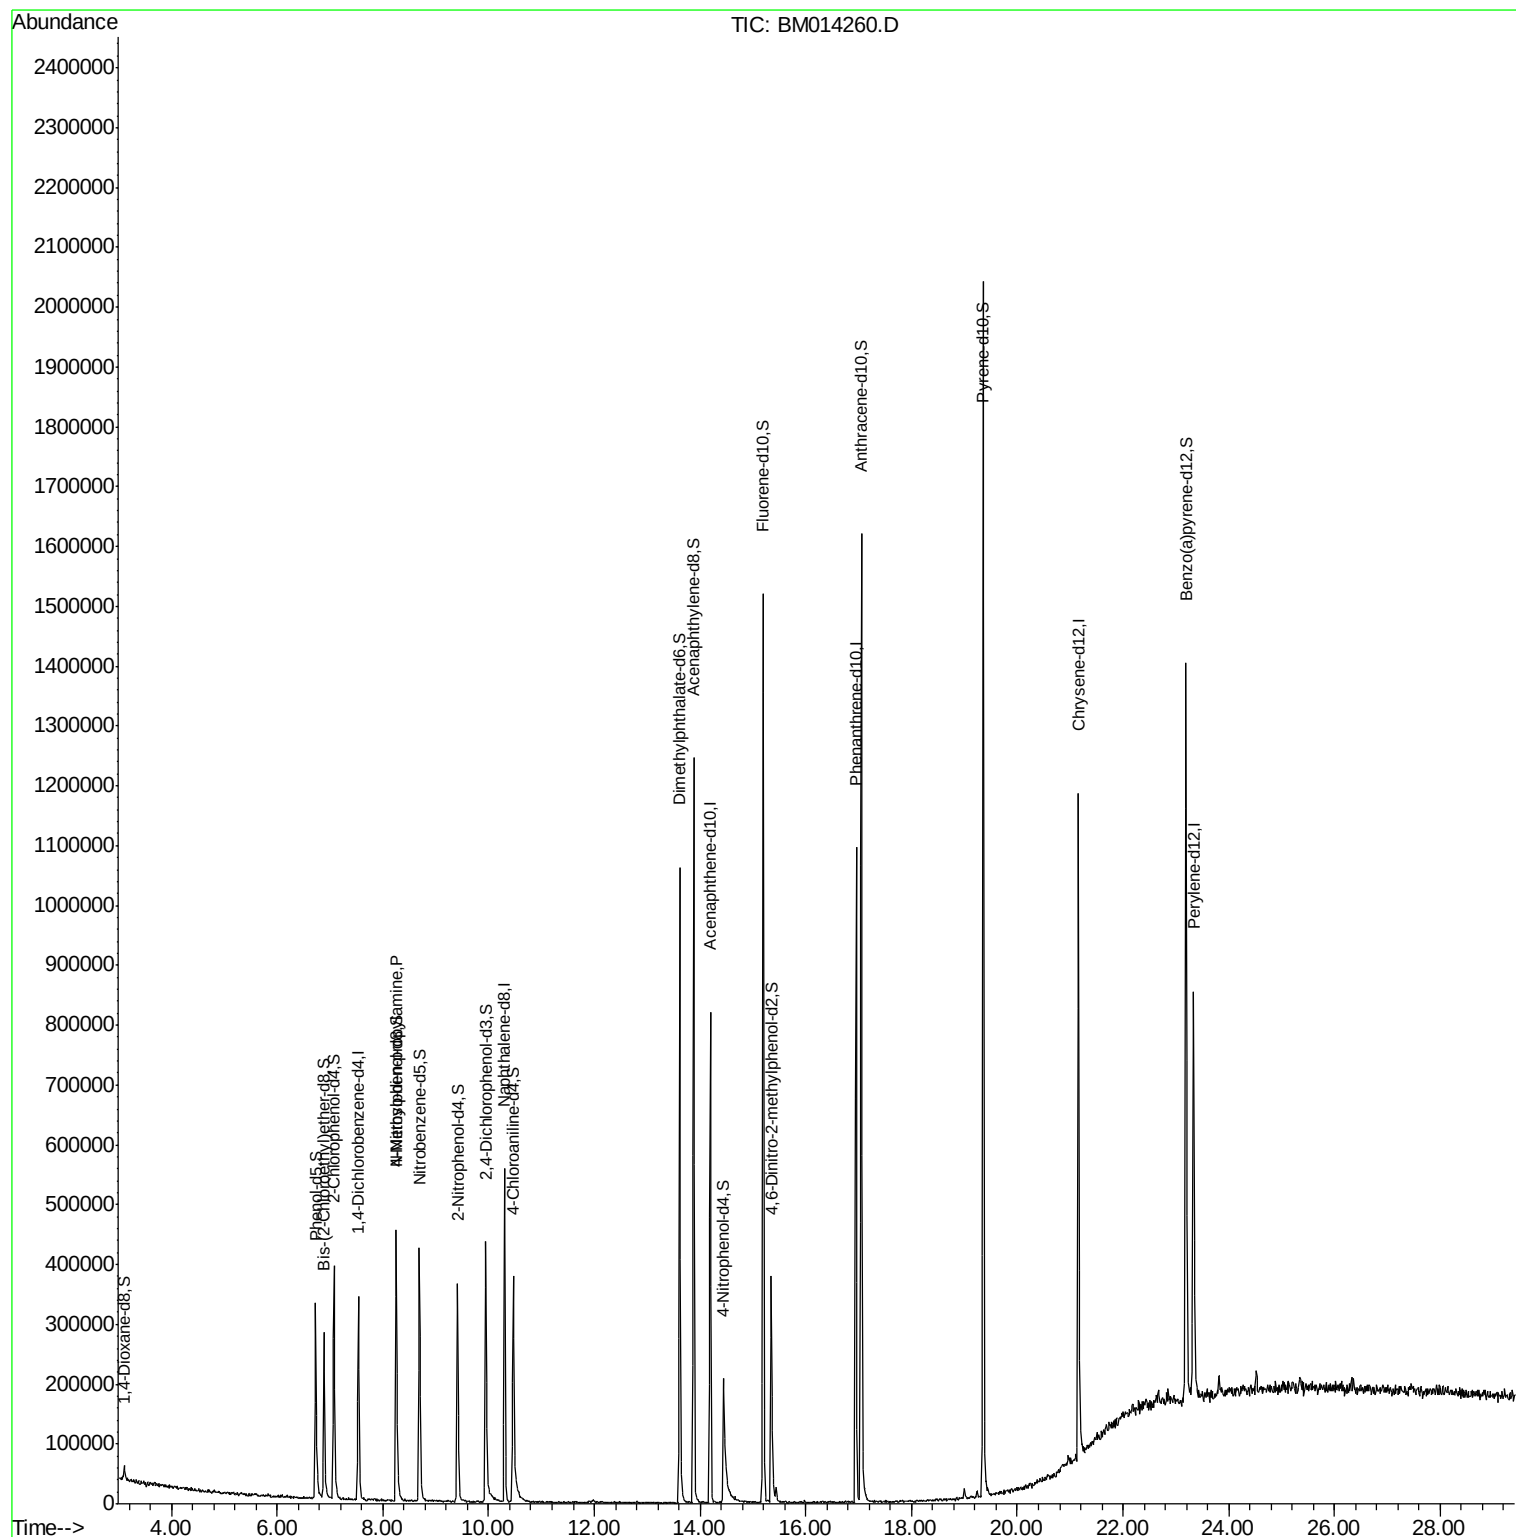

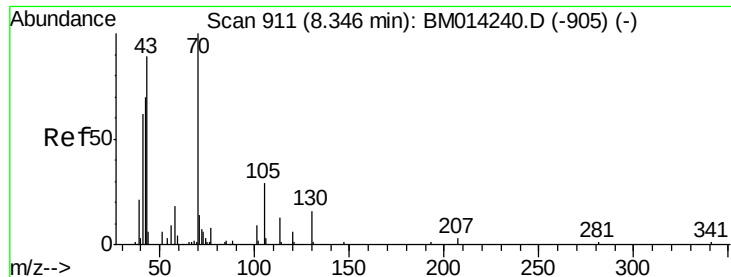

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.069 ng/ul
 RT: 8.26 min Scan# 896
 Delta R.T. -0.09 min
 Lab File: BM014260.D
 Acq: 16 Feb 2018 09:41

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 5576
 Ion Ratio Lower Upper
 70 100
 42 350.6 76.0 114.0#
 101 0.0 6.7 10.1#
 130 0.0 14.6 22.0#

