

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021618\
 Data File : BM014264.D
 Acq On : 16 Feb 2018 12:05
 Operator : SJ/JU
 Sample : J1553-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C02Q1

Quant Time: Feb 16 13:24:12 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 15 01:12:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	66887	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	303790	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.19	164	210395	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.95	188	502512	20.00	ng/ul	0.00
75) Chrysene-d12	21.16	240	496793	20.00	ng/ul	0.00
83) Perylene-d12	23.33	264	435175	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	8934	5.72	ng/uL	0.00
5) Phenol-d5	6.73	99	40609	7.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	123190	36.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.07	132	128028	29.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	83951	16.97	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	87412	38.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	95859	41.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	135639	28.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.32	131	264	0.06	ng/ul	-0.15
43) Dimethylphthalate-d6	13.62	166	677205	38.98	ng/ul	0.00
46) Acenaphthylene-d8	13.88	160	803504	37.50	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	4062	1.69	ng/ul	0.06
57) Fluorene-d10	15.19	176	591567	38.00	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	88862	29.48	ng/ul	0.00
70) Anthracene-d10	17.05	188	967452	39.90	ng/ul	0.00
76) Pyrene-d10	19.36	212	1102144	43.01	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.19	264	824597	38.93	ng/ul	0.00

Target Compounds


				Ovalue	
2) 1,4-Dioxane	3.14	88	23035	13.268	ng/uL# 65
21) Isophorone	9.41	82	14161	1.247	ng/ul# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021618\
Data File : BM014264.D
Acq On : 16 Feb 2018 12:05
Operator : SJ/JU
Sample : J1553-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C02Q1

Quant Time: Feb 16 13:24:12 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 15 01:12:03 2018
Response via : Initial Calibration

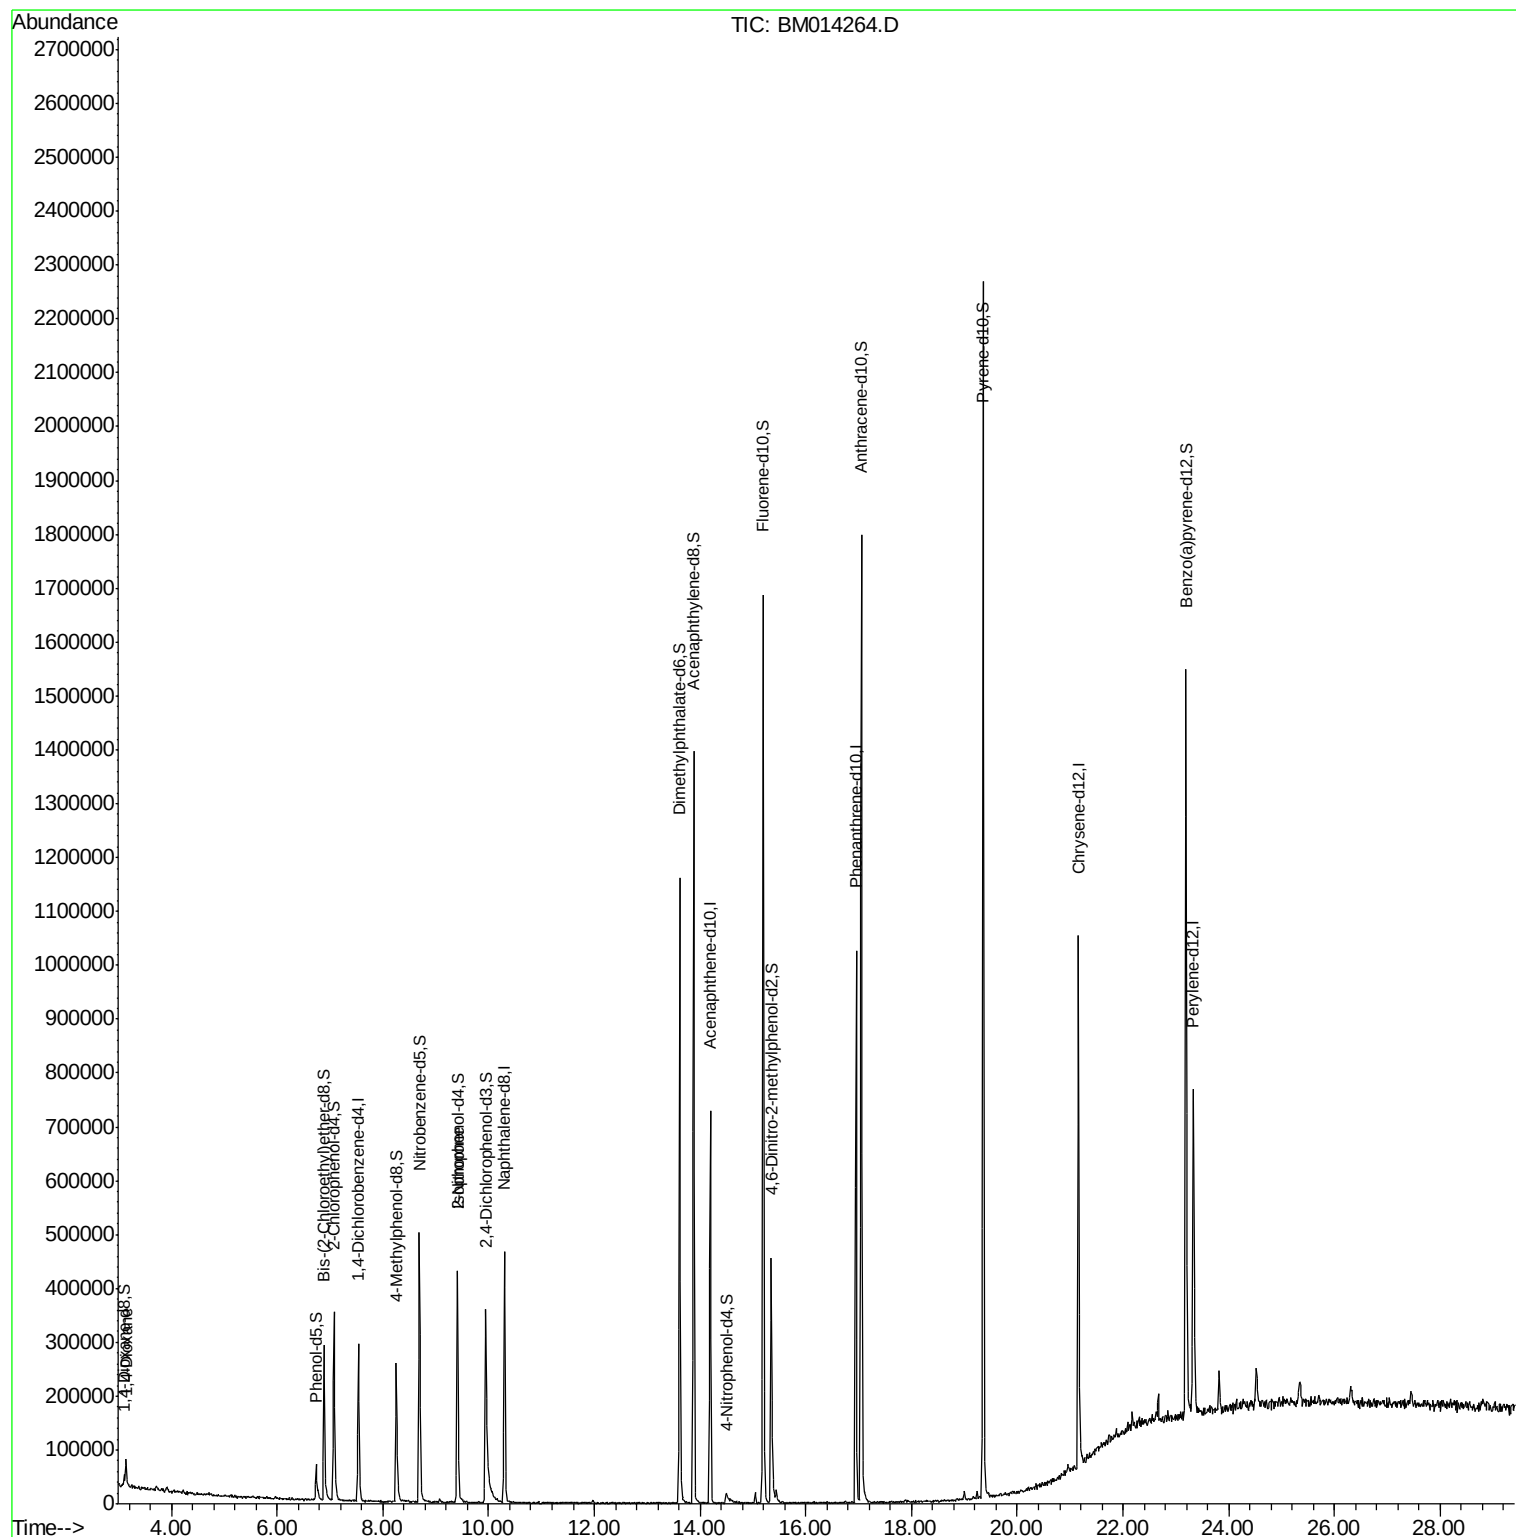

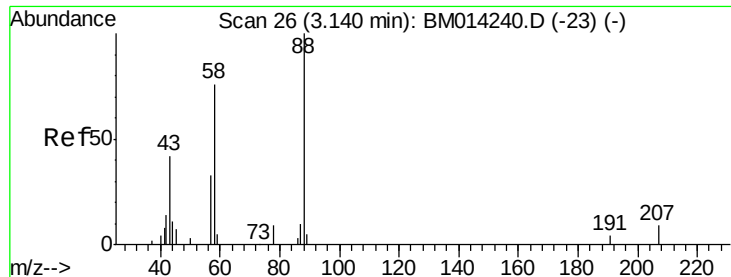

#2

1,4-Dioxane

Concen: 13.268 ng/uL

RT: 3.14 min Scan# 26

Delta R.T. -0.00 min

Lab File: BM014264.D

Acq: 16 Feb 2018 12:05

Instrument :

BNA_M

ClientSampleId :

C02Q1


Tot Ion: 88 Resp: 23035

Ion Ratio Lower Upper

88 100

43 34.3 48.0 72.0#




58 64.6 80.0 120.0#

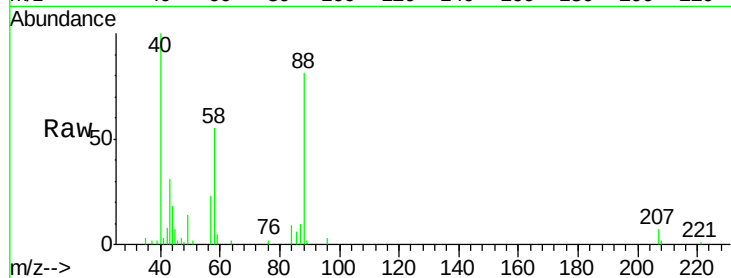

Abundance Ion 88.00 (87.70 to 88.70): BM014264.D (-1) (-)

Ion 43.00 (42.70 to 43.70): BM014264.D (-1) (-)

Ion 58.00 (57.70 to 58.70): BM014264.D (-1) (-)

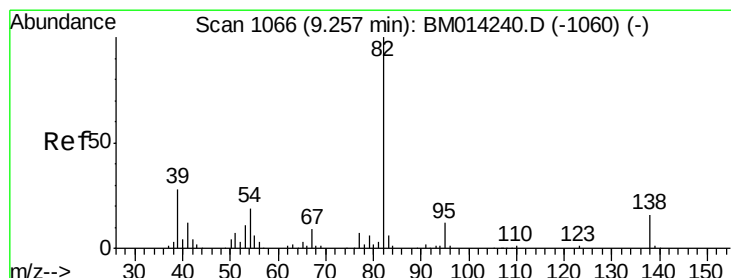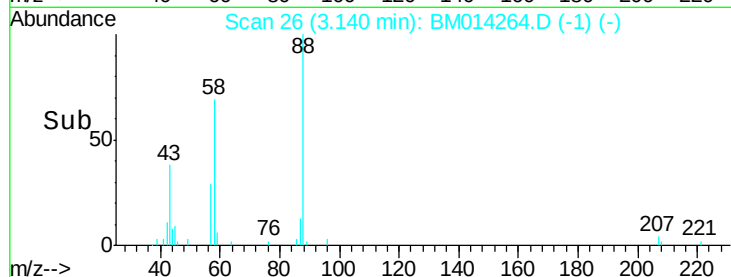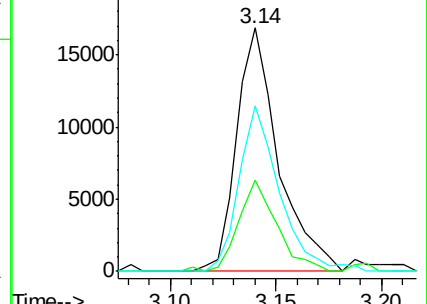

#21

Isophorone

Concen: 1.247 ng/uL

RT: 9.41 min Scan# 1092

Delta R.T. 0.15 min

Lab File: BM014264.D

Acq: 16 Feb 2018 12:05


Tgt Ion: 82 Resp: 14161

Ion Ratio Lower Upper

82 100

95 15.8 7.8 11.8#

138 0.0 11.9 17.9#

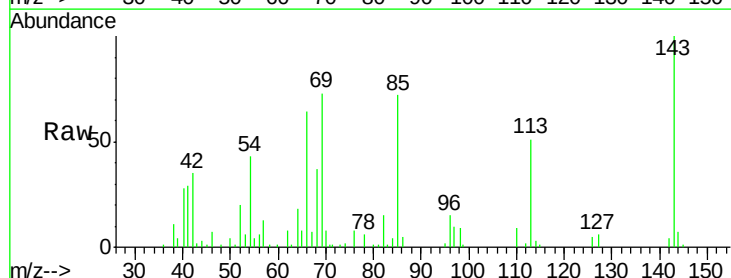

Abundance Ion 82.00 (81.70 to 82.70): BM014264.D (-1032) (-)

Ion 95.00 (94.70 to 95.70): BM014264.D (-1032) (-)

Ion 138.00 (137.70 to 138.70): BM014264.D (-1032) (-)

