

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021618\
 Data File : BM014276.D
 Acq On : 16 Feb 2018 19:19
 Operator : SJ/JU
 Sample : J1569-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C02R0

Manual Integrations
 APPROVED

Quant Time: Feb 17 02:27:15 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 17 00:49:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	73116	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	322968	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.19	164	214999	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.95	188	516510	20.00	ng/ul	0.00
75) Chrysene-d12	21.16	240	534954	20.00	ng/ul	0.00
83) Perylene-d12	23.33	264	456997	20.00	ng/ul	0.00

Sohil

2/19/2018 4:15:59 PM

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.11	96	10079	5.90	ng/uL	0.00
5) Phenol-d5	6.74	99	31360	5.07	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.89	67	107489	28.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	109467m	23.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	63821	11.80	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	70367	29.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	77430	31.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	118733m	23.21	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	13.61	166	534701	30.12	ng/ul	0.00
46) Acenaphthylene-d8	13.88	160	649340	29.66	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	4788m	1.95	ng/ul	0.11
57) Fluorene-d10	15.19	176	485143	30.50	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	67351	21.74	ng/ul	0.00
70) Anthracene-d10	17.05	188	756531	30.36	ng/ul	0.00
76) Pyrene-d10	19.35	212	875620	31.74	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.19	264	684401	30.77	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) 1,4-Dioxane	3.14	88	10950	5.770	ng/uL#	55

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM021618\
Data File : BM014276.D
Acq On : 16 Feb 2018 19:19
Operator : SJ/JU
Sample : J1569-11
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C02R0

Manual Integrations
APPROVED

Quant Time: Feb 17 02:27:15 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 17 00:49:49 2018
Response via : Initial Calibration

Sohil

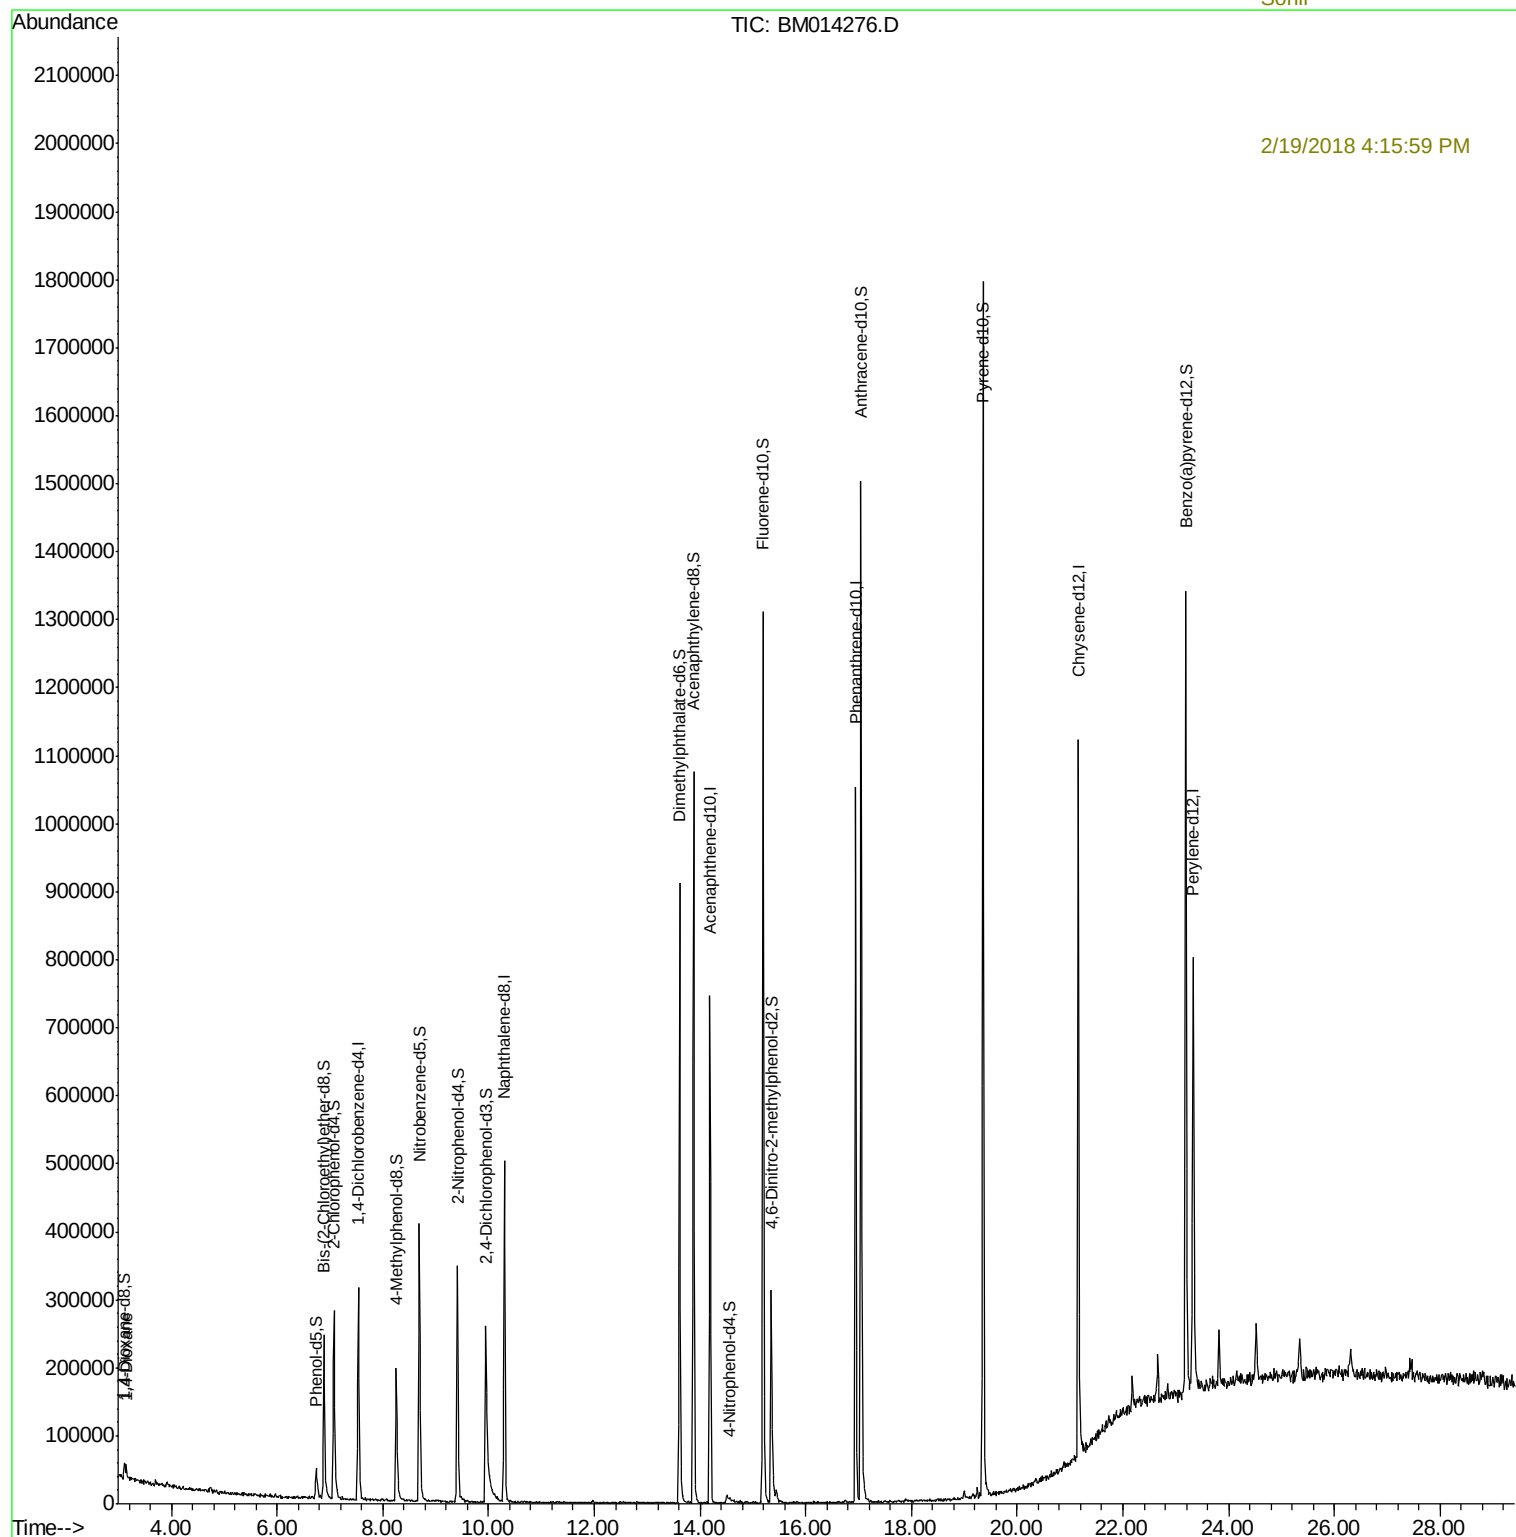



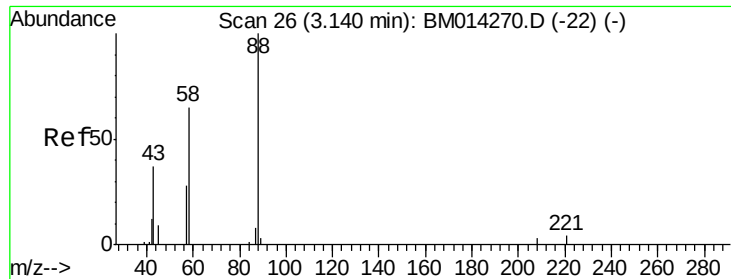


#2
 1,4-Dioxane
 Concen: 5.770 ng/uL
 RT: 3.14 min Scan# 26
 Delta R.T. 0.00 min
 Lab File: BM014276.D
 Acq: 16 Feb 2018 19:19

Instrument :
 BNA_M
 ClientSampleId :
 C02R0

Tot Ion	Ion	Ratio	Lower	Upper
88	100			
43	30.0	48.0	72.0#	
58	51.8	80.0	120.0#	

Manual Integrations
 APPROVED

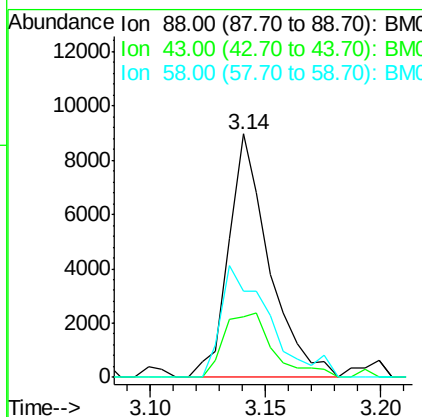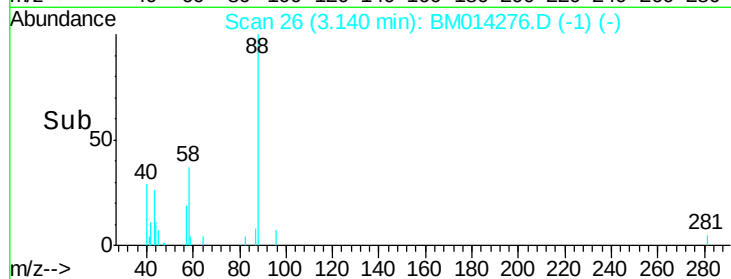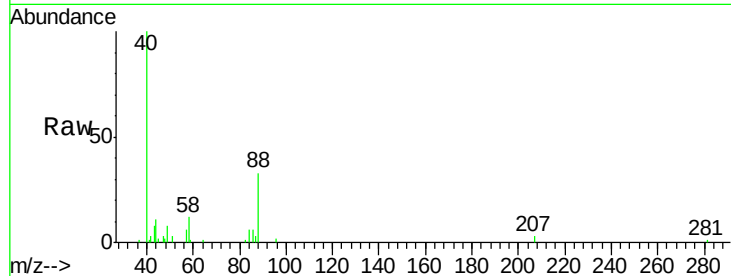

Sohil

2/19/2018 4:15:59 PM