


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021621\
 Data File : BM028739.D
 Acq On : 16 Feb 2021 09:05
 Operator : CG/JU
 Sample : DFTPP30
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP30

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 17 11:34:13 2021

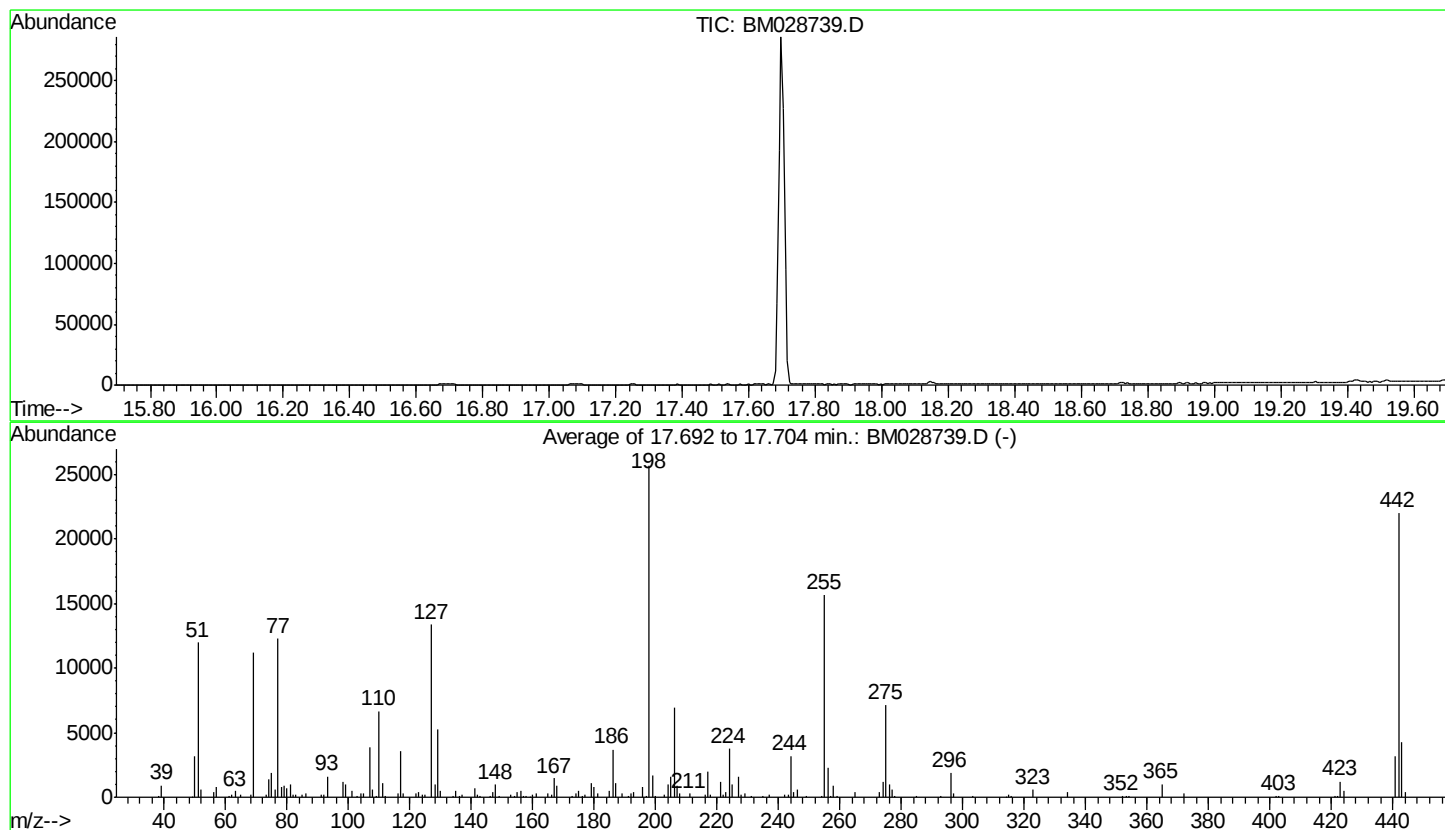

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	11954	PASS
68	69	0.00	2	1.6	182	PASS
69	198	0.00	100	43.7	11217	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	13338	PASS
197	198	0.00	2	0.5	123	PASS
198	198	100	100	100.0	25664	PASS
199	198	5	9	6.4	1655	PASS
275	198	10	60	27.8	7143	PASS
365	198	1	100	3.9	994	PASS
441	198	0.01	100	12.4	3175	PASS
442	198	50	100	85.9	22041	PASS
443	442	15	24	19.4	4267	PASS

Scan 2494 (17.657 min): BM028739.D
DFTPP30

m/z	Abundance
43.90	270.0
207.00	342.0

Instrument :
BNA_M
ClientSampleId :
DFTPP30

m/z	Abundance
39.10	875.0
43.90	242.0
50.10	3119.0
51.00	11738.0
52.00	627.0
56.00	344.0
57.00	698.0
62.00	197.0
63.00	410.0
65.00	273.0
68.00	238.0
69.00	10663.0
73.10	224.0
74.00	1292.0
75.00	1755.0
76.00	607.0
77.10	11747.0
78.00	759.0
79.00	884.0
80.00	677.0
81.00	887.0
81.90	224.0
82.90	182.0
84.90	161.0
85.90	265.0
91.00	197.0
92.00	227.0
93.00	1495.0
98.00	1073.0
98.90	950.0
101.00	419.0
102.90	170.0
104.00	301.0
105.00	287.0
107.00	3385.0
107.90	537.0
110.00	6088.0
111.00	959.0
112.00	162.0
116.00	213.0
117.00	3296.0
117.90	273.0
122.00	234.0
122.90	345.0
123.90	151.0
124.90	190.0
127.00	12008.0
128.00	917.0
129.00	4778.0
130.00	407.0
135.00	487.0
136.00	165.0
136.90	273.0
141.00	579.0
141.90	228.0
147.00	289.0
147.90	810.0
148.90	179.0
152.90	218.0
155.00	231.0
155.90	430.0
160.00	219.0
161.00	291.0
164.90	203.0
167.00	1208.0
168.00	777.0
173.90	236.0
175.00	423.0
176.80	172.0
179.00	890.0
180.00	726.0
180.90	261.0
185.00	452.0
186.00	2972.0
187.00	1001.0
188.90	233.0
191.90	236.0
193.00	305.0
195.90	643.0
197.10	188.0
198.00	20816.0
199.00	1405.0
203.00	152.0
204.00	935.0
205.00	1359.0
206.00	5596.0
207.00	1008.0
208.00	274.0
210.90	216.0
216.00	155.0
217.00	1499.0
217.90	208.0

Instrument :
BNA_M
ClientSampleId :
DFTPP30

221.00	979.0
221.90	212.0
223.00	324.0
224.00	2819.0
225.00	763.0
227.00	1420.0
227.90	159.0
229.00	248.0
237.00	168.0
243.00	153.0
244.00	2541.0
245.00	380.0
246.00	443.0
255.00	12031.0
256.00	1814.0
258.00	622.0
265.00	242.0
272.90	366.0
274.00	991.0
275.00	5559.0
276.00	727.0
277.00	461.0
296.00	1353.0
297.00	186.0
314.90	158.0
323.00	428.0
333.90	256.0
364.90	686.0
372.00	246.0
422.90	728.0
424.00	368.0
440.90	1923.0
442.00	13117.0
443.00	2769.0
443.90	295.0

Instrument :
BNA_M
ClientSampleId :
DFTPP30

m/z	Abundance
38.00	227.0
39.00	1084.0
44.00	279.0
49.00	152.0
50.10	3843.0
51.10	14544.0
52.00	654.0
56.00	481.0
57.00	1024.0
61.00	180.0
62.00	202.0
63.00	598.0
65.00	228.0
68.10	309.0
69.00	13595.0
73.00	201.0
74.00	1777.0
75.00	2281.0
76.00	863.0
77.10	14928.0
78.10	1017.0
79.00	1086.0
80.00	779.0
81.00	1195.0
82.00	247.0
82.90	253.0
84.90	165.0
86.00	338.0
91.00	292.0
91.90	259.0
93.00	1852.0
98.00	1441.0
99.00	1205.0
101.00	565.0
103.00	195.0
103.90	421.0
104.90	350.0
107.00	4754.0
108.00	634.0
109.00	168.0
110.00	8017.0
111.00	1463.0
112.00	203.0
116.00	363.0
117.00	4528.0
118.00	322.0
122.00	327.0
123.00	516.0
123.90	216.0
124.90	168.0
127.00	16061.0
128.00	1093.0
129.00	6563.0
130.00	585.0
134.00	212.0
135.00	542.0
135.90	231.0
137.00	275.0
141.00	822.0
141.90	282.0
142.90	165.0
146.00	167.0
147.00	455.0
147.90	1130.0
152.90	271.0
153.90	197.0
155.00	526.0
156.00	666.0
157.00	183.0
158.90	156.0
159.90	262.0
161.00	424.0
164.90	356.0
166.00	255.0
167.00	1807.0
168.00	952.0
172.90	227.0
173.90	346.0
175.00	603.0
175.90	162.0
176.90	317.0
178.90	1373.0
180.00	969.0
180.90	425.0
184.90	591.0
186.00	4620.0
187.00	1214.0
189.00	297.0
190.90	161.0
192.00	365.0
192.90	451.0
195.90	973.0

Instrument :
BNA_M
ClientSampleId :
DFTPP30

198.00	31176.0
198.90	2085.0
199.90	166.0
203.00	215.0
204.00	1175.0
205.00	1832.0
206.00	8618.0
207.00	1485.0
208.00	358.0
211.00	363.0
216.10	209.0
217.00	2493.0
217.90	283.0
221.00	1557.0
221.80	332.0
223.00	434.0
224.00	4585.0
225.00	1205.0
227.00	1812.0
228.00	212.0
229.00	315.0
231.00	172.0
235.00	185.0
237.00	242.0
242.00	274.0
243.00	270.0
244.10	3795.0
245.00	423.0
246.00	765.0
249.00	165.0
254.20	199.0
255.00	19120.0
256.00	2645.0
257.00	228.0
258.00	1167.0
265.00	455.0
273.00	497.0
274.00	1408.0
275.00	8455.0
276.00	1069.0
277.00	712.0
278.00	161.0
284.90	161.0
296.00	2476.0
297.00	334.0
303.00	223.0
313.90	151.0
315.00	228.0
315.90	174.0
323.00	736.0
334.00	455.0
351.90	192.0
354.00	253.0
364.90	1227.0
372.00	379.0
403.00	219.0
421.00	226.0
422.00	175.0
423.00	1493.0
424.00	571.0
441.00	3616.0
442.00	25552.0
443.00	4960.0
444.00	457.0

Instrument :
BNA_M
ClientSampleId :
DFTPP30

m/z	Abundance
39.10	797.0
44.00	279.0
50.00	2514.0
51.10	9581.0
52.00	402.0
55.90	284.0
57.00	557.0
60.90	163.0
62.00	162.0
63.00	427.0
64.90	168.0
69.00	9394.0
73.00	247.0
74.00	1074.0
75.00	1604.0
76.10	472.0
77.10	10048.0
78.00	621.0
79.00	740.0
80.00	536.0
81.00	842.0
82.00	173.0
83.00	170.0
84.90	153.0
85.90	230.0
91.00	159.0
91.90	198.0
93.00	1509.0
98.00	1033.0
99.00	802.0
100.90	427.0
103.90	319.0
105.00	300.0
107.00	3464.0
108.00	552.0
110.00	5816.0
111.00	821.0
115.90	215.0
117.00	3031.0
118.00	229.0
121.90	240.0
122.90	434.0
123.90	192.0
125.00	180.0
127.00	11947.0
128.00	866.0
129.00	4556.0
129.90	396.0
135.00	403.0
137.00	182.0
141.00	609.0
141.90	198.0
146.00	165.0
146.90	399.0
148.00	920.0
148.90	155.0
152.90	181.0
155.00	398.0
156.00	495.0
156.90	207.0
158.00	186.0
159.90	193.0
161.00	273.0
164.90	222.0
165.90	210.0
167.00	1323.0
168.00	850.0
173.90	299.0
175.00	517.0
176.00	156.0
176.90	258.0
179.00	1074.0
180.00	661.0
181.00	328.0
185.00	465.0
186.00	3548.0
187.00	954.0
188.90	261.0
191.00	196.0
192.00	274.0
193.00	395.0
195.90	790.0
197.10	182.0
198.00	25000.0
199.00	1475.0
202.90	211.0
204.00	903.0
205.00	1558.0
206.00	6697.0
207.00	1252.0
208.00	261.0
211.00	283.0

Instrument :
BNA_M
ClientSampleId :
DFTPP30

215.90	167.0
217.00	2005.0
218.00	239.0
221.00	1060.0
222.00	197.0
222.90	409.0
224.00	3836.0
225.00	1027.0
227.00	1610.0
227.90	261.0
229.00	318.0
230.90	176.0
237.00	173.0
242.00	191.0
243.10	183.0
244.00	3181.0
245.00	390.0
246.00	663.0
255.00	15941.0
256.00	2366.0
256.90	171.0
258.00	938.0
258.90	178.0
264.90	414.0
273.00	417.0
274.00	1206.0
275.00	7417.0
276.00	1101.0
276.90	571.0
278.00	175.0
293.00	160.0
296.00	1974.0
296.90	290.0
303.10	211.0
314.90	227.0
322.90	572.0
334.00	433.0
351.90	218.0
353.10	165.0
354.00	175.0
364.90	1069.0
371.90	398.0
401.90	176.0
402.90	216.0
421.00	185.0
422.00	248.0
423.00	1410.0
424.00	566.0
441.00	3988.0
442.00	27456.0
443.00	5074.0
443.90	394.0

Instrument :
BNA_M
ClientSampleId :
DFTPP30