
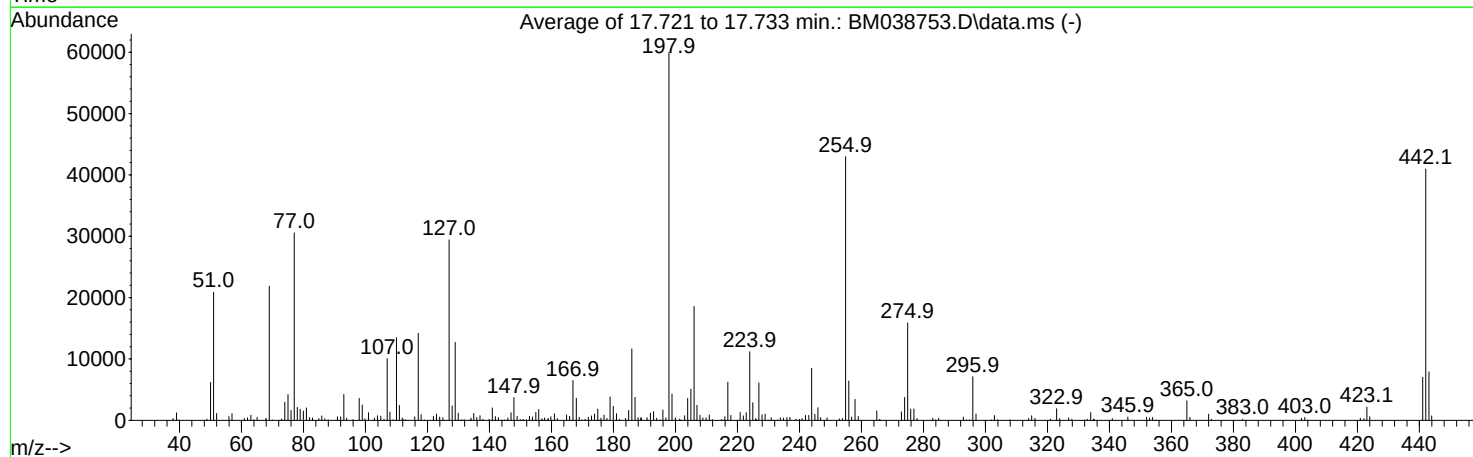


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021623\
Data File : BM038753.D
Acq On : 16 Feb 2023 12:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 17 06:10:11 2023

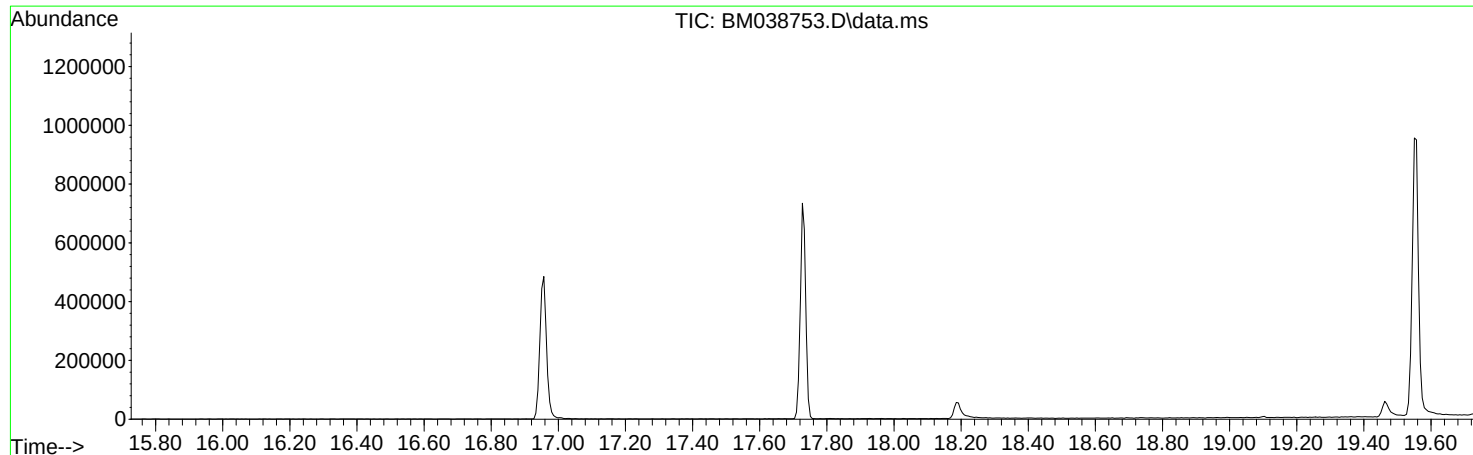




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	20891	PASS
68	69	0.00	2	1.5	325	PASS
69	198	0.00	100	36.5	21864	PASS
70	69	0.00	2	0.2	51	PASS
127	198	10	80	49.1	29416	PASS
197	198	0.00	2	0.7	415	PASS
198	198	100	100	100.0	59971	PASS
199	198	5	9	7.1	4269	PASS
275	198	10	60	26.5	15881	PASS
365	198	1	100	5.3	3176	PASS
441	198	0.01	100	11.7	6994	PASS
442	442	50	100	100.0	40960	PASS
443	442	15	24	19.3	7888	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021623\
Data File : BM038753.D
Acq On : 16 Feb 2023 12:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 17 07:33:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 06:10:11 2023
Response via : Initial Calibration

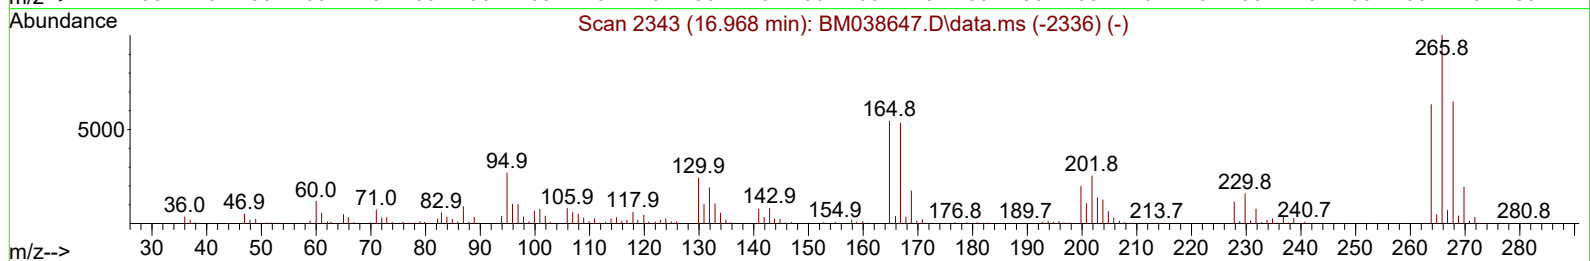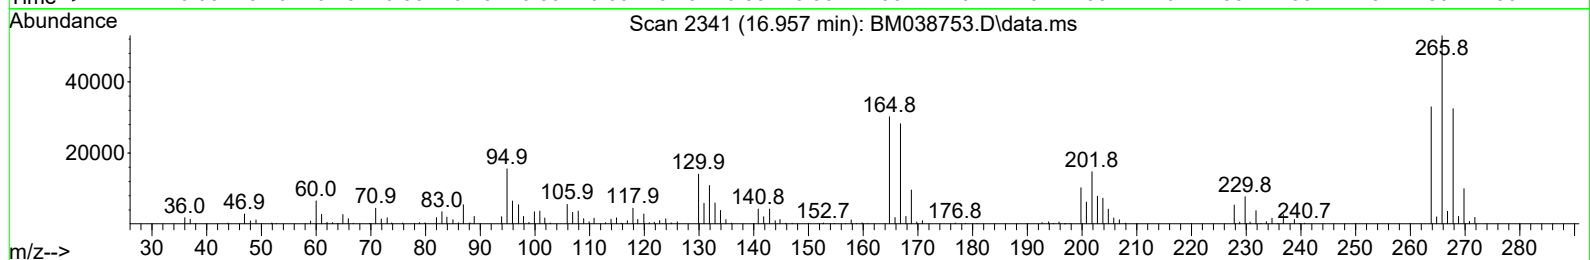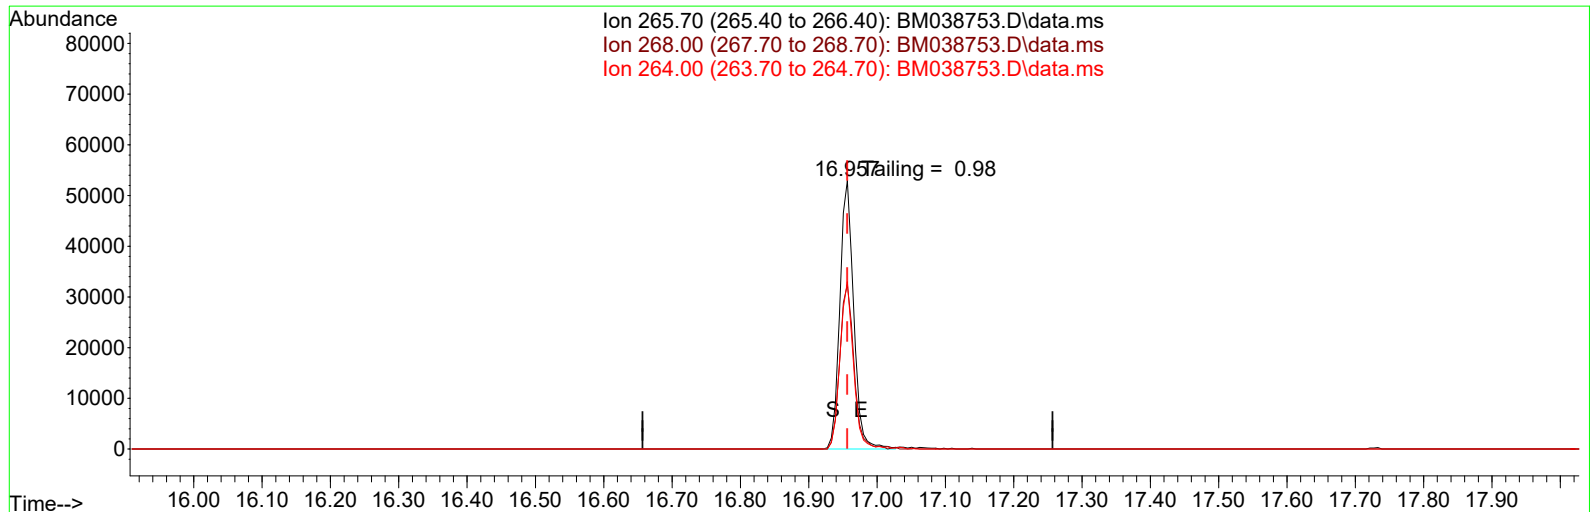

TIC: BM038753.D\data.ms

(70) Pentachlorophenol (C)

16.957min (-0.000) 0.00 ng




response 74270

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	61.30
264.00	63.30	62.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021623\
Data File : BM038753.D
Acq On : 16 Feb 2023 12:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 17 07:33:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 06:10:11 2023
Response via : Initial Calibration

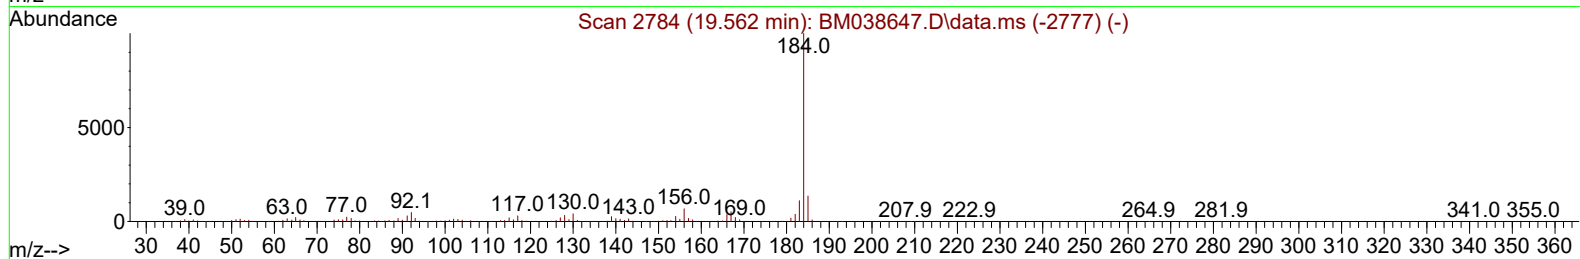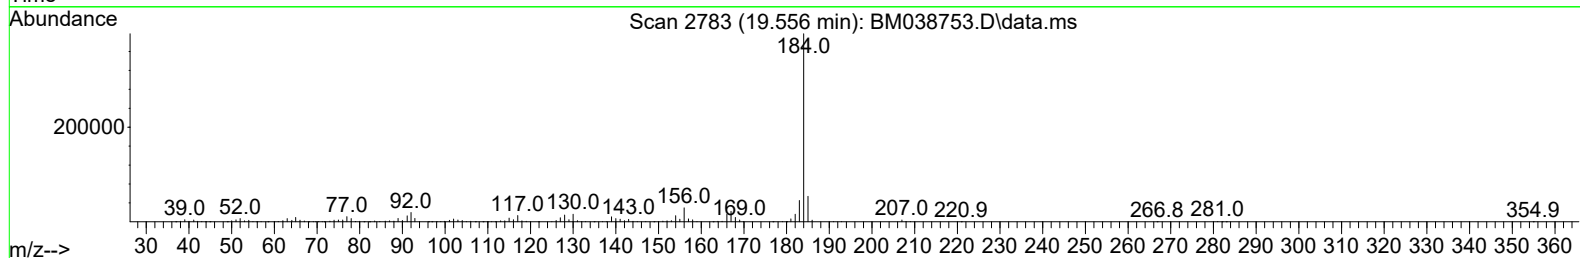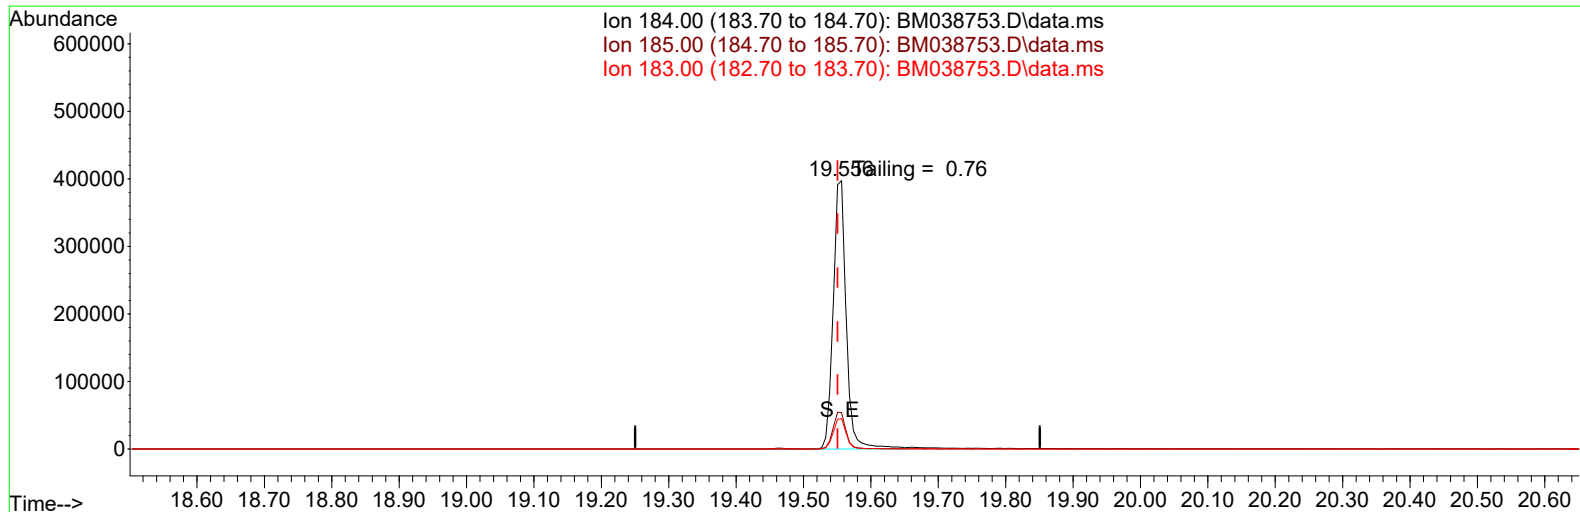

TIC: BM038753.D\data.ms

(77) Benzidine

19.556min (+ 0.006) 57324.92 ng

response 534072

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.56
183.00	11.00	11.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/16/2023	BNA_M	<u>BM038753.D</u>
Compound Name	Response	Retention Time
DDT	229542	20.774
DDD	2985	20.38
DDE	157	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3142	232684	1.35

Instrument :
BNA_M
ClientSampleId :
DFTPP