


Data Path : Z:\HPCHEM1\BNA_M\Data\BM021715\
Data File : BM000536.D
Acq On : 17 Feb 2015 11:38
Operator : TP/IZ
Sample : DFTPP24
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP24

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-SIM-BM021215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 12 16:45:55 2015

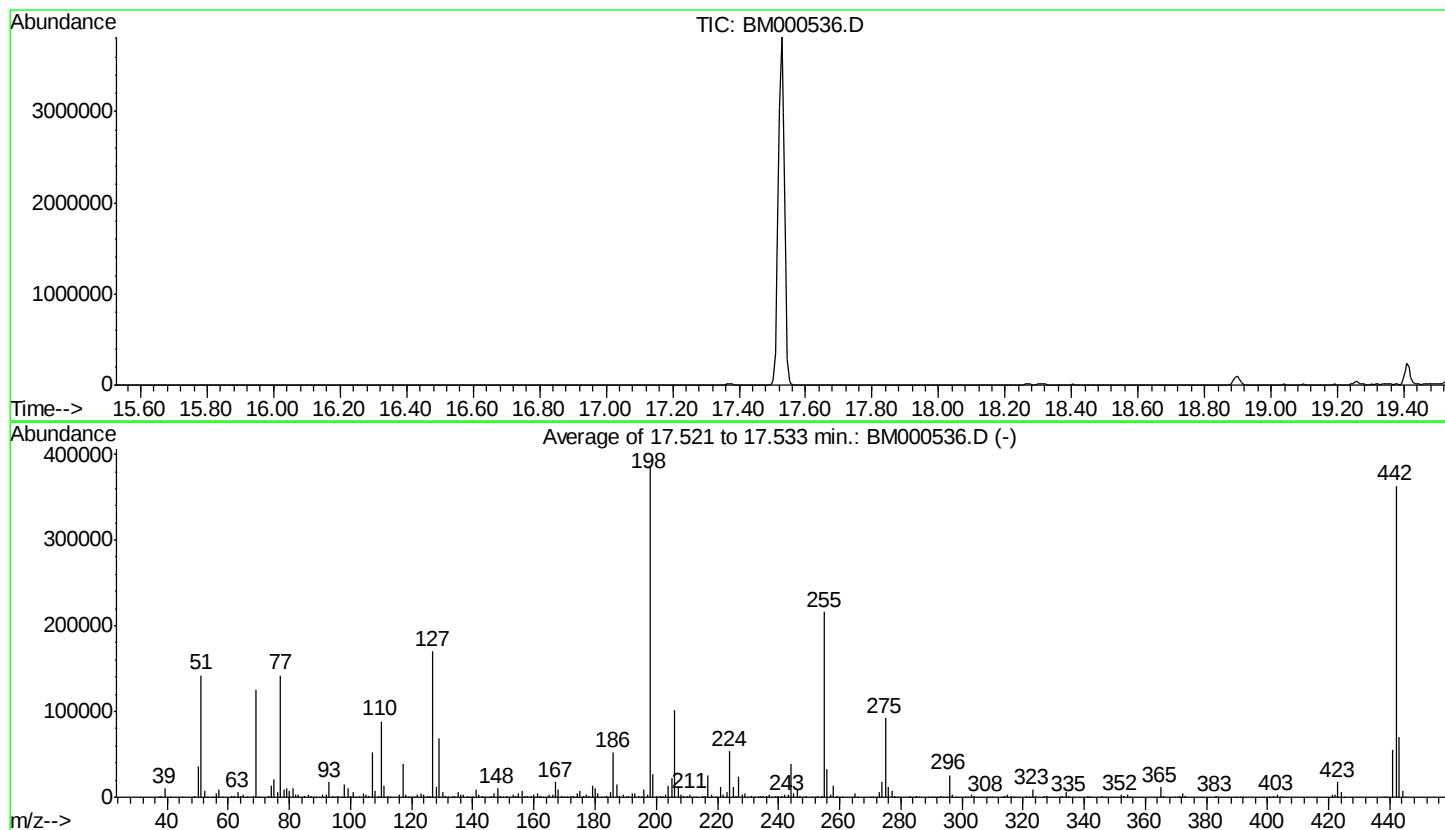

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	142538	PASS
68	69	0.00	2	1.7	2122	PASS
69	198	0.00	100	32.5	125709	PASS
70	69	0.00	2	0.5	574	PASS
127	198	10	80	44.0	170197	PASS
197	198	0.00	2	0.7	2770	PASS
198	198	100	100	100.0	386752	PASS
199	198	5	9	7.0	27032	PASS
275	198	10	60	23.9	92381	PASS
365	198	1	100	3.0	11633	PASS
441	443	0.01	100	77.9	54733	PASS
442	198	50	100	93.9	363221	PASS
443	442	15	24	19.4	70296	PASS