


Data Path : Z:\HPCHEM1\BNA_M\Data\BM021715\
 Data File : BM000536.D
 Acq On : 17 Feb 2015 11:38
 Operator : TP/IZ
 Sample : DFTPP24
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP24

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-SIM-BM021215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 12 16:45:55 2015

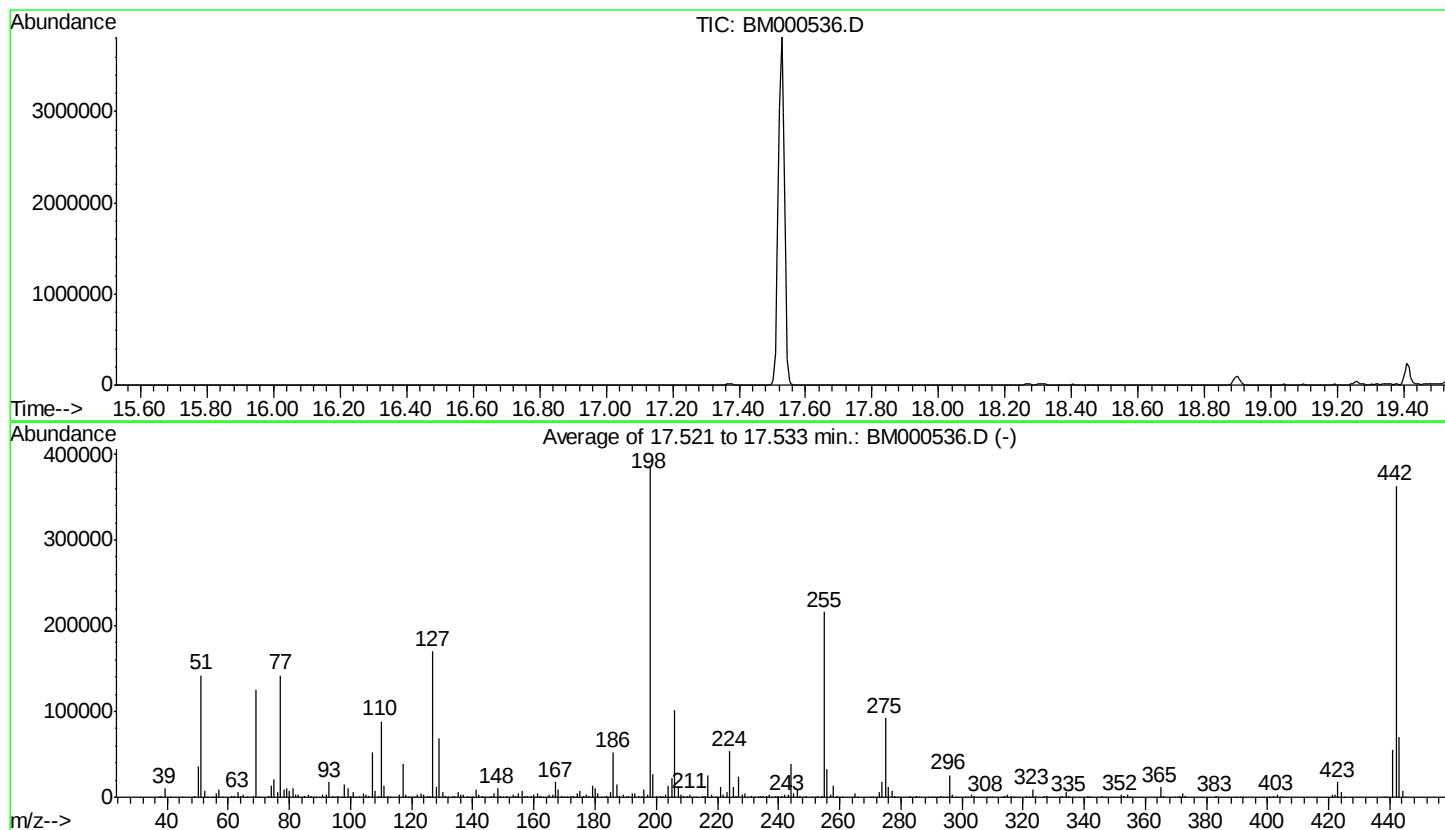

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	142538	PASS
68	69	0.00	2	1.7	2122	PASS
69	198	0.00	100	32.5	125709	PASS
70	69	0.00	2	0.5	574	PASS
127	198	10	80	44.0	170197	PASS
197	198	0.00	2	0.7	2770	PASS
198	198	100	100	100.0	386752	PASS
199	198	5	9	7.0	27032	PASS
275	198	10	60	23.9	92381	PASS
365	198	1	100	3.0	11633	PASS
441	443	0.01	100	77.9	54733	PASS
442	198	50	100	93.9	363221	PASS
443	442	15	24	19.4	70296	PASS

m/z	Abundance
37.10	449.0
38.10	1535.0
39.10	10516.0
40.00	526.0
41.00	390.0
44.00	2743.0
49.00	1087.0
50.10	37808.0
51.10	151424.0
52.10	8224.0
53.00	300.0
55.00	498.0
56.00	4512.0
57.10	10018.0
58.00	369.0
61.10	1588.0
62.10	1837.0
63.10	5897.0
64.10	959.0
65.00	2547.0
68.10	2242.0
69.00	131648.0
70.00	608.0
73.00	1263.0
74.10	13242.0
75.00	22784.0
76.10	7014.0
77.10	148736.0
78.10	9735.0
79.00	10974.0
80.00	7929.0
81.00	11257.0
82.00	2893.0
83.00	2838.0
85.10	1837.0
86.00	4071.0
87.00	1175.0
88.10	363.0
88.90	304.0
91.00	2956.0
92.00	2663.0
93.00	17976.0
94.00	1433.0
96.00	827.0
96.90	306.0
98.00	14705.0
99.00	11360.0
100.00	821.0
101.00	7042.0
101.90	491.0
103.00	2249.0
104.00	3798.0
105.00	4086.0
106.00	1038.0
107.00	52752.0
108.00	7612.0
109.10	1410.0
110.00	87608.0
111.00	13471.0
112.00	1796.0
113.10	574.0
116.10	2810.0
117.00	38416.0
118.00	3460.0
118.90	333.0
120.00	485.0
120.90	307.0
122.00	2925.0
123.00	5778.0
124.10	2689.0
125.10	1923.0
126.10	1051.0
127.00	169408.0
128.00	11931.0
129.00	66992.0
130.00	6054.0
131.00	1326.0
132.00	365.0
132.90	306.0
133.90	1528.0
135.00	5782.0
136.10	2301.0
137.00	3168.0
138.10	612.0
140.00	771.0
141.00	8720.0
142.00	2720.0
143.00	2089.0
144.10	596.0
145.10	704.0
146.10	1686.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

146.90	4593.0
148.00	9436.0
149.00	1972.0
150.20	401.0
151.10	1659.0
152.00	596.0
153.00	3214.0
154.00	2018.0
155.00	5050.0
156.10	7490.0
157.20	1200.0
158.00	1741.0
159.00	1100.0
160.10	2895.0
161.00	4207.0
161.90	897.0
162.90	359.0
163.90	598.0
164.90	3459.0
166.10	2781.0
167.10	16984.0
168.00	8919.0
169.00	1959.0
170.10	541.0
171.00	657.0
172.00	1538.0
173.00	2072.0
174.10	4502.0
175.00	6898.0
176.10	2404.0
177.00	3667.0
178.10	1255.0
179.00	13327.0
180.00	9419.0
181.00	3886.0
182.10	828.0
182.80	390.0
183.90	1075.0
185.10	6230.0
186.10	51344.0
187.10	15426.0
188.10	2306.0
189.00	3089.0
189.90	505.0
191.00	1604.0
192.00	3691.0
193.00	4840.0
194.00	940.0
194.90	567.0
196.00	7960.0
197.10	2622.0
198.00	365632.0
199.00	26720.0
200.00	1903.0
201.50	891.0
202.10	459.0
203.10	2743.0
204.00	13595.0
205.10	21528.0
206.10	91320.0
207.00	12940.0
208.00	3784.0
209.00	1738.0
210.10	1169.0
211.10	3393.0
212.10	594.0
212.90	304.0
215.00	1188.0
216.10	1985.0
217.00	24168.0
218.10	2594.0
219.90	451.0
221.10	10849.0
221.80	2863.0
223.00	4649.0
224.10	48816.0
225.00	12084.0
226.00	1616.0
227.00	22576.0
228.00	3419.0
229.00	4269.0
229.90	776.0
231.00	1517.0
233.10	406.0
234.00	1419.0
235.00	1149.0
236.00	1026.0
237.00	2313.0
238.00	378.0
239.00	994.0
240.00	790.0
241.10	1417.0
242.10	2480.0
243.10	2783.0
244.10	34408.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

245.10	4476.0
246.00	8235.0
247.00	1769.0
248.10	527.0
249.00	1430.0
252.10	516.0
253.10	1253.0
254.10	1594.0
255.00	189952.0
256.00	29640.0
257.10	2868.0
258.10	11618.0
259.00	1523.0
260.00	439.0
261.10	373.0
265.00	3907.0
266.00	615.0
270.90	369.0
272.10	613.0
273.00	5531.0
274.00	16100.0
275.00	79384.0
276.00	10944.0
277.00	7602.0
278.00	1404.0
279.10	343.0
283.00	1049.0
284.10	328.0
285.10	1468.0
286.00	345.0
289.00	381.0
290.10	337.0
291.00	324.0
292.90	1650.0
294.00	580.0
295.00	557.0
296.00	23848.0
297.00	2647.0
301.00	366.0
302.10	459.0
303.10	2612.0
304.00	613.0
308.00	614.0
309.00	447.0
314.10	1210.0
315.00	2555.0
316.00	1116.0
317.10	374.0
321.00	951.0
322.00	480.0
323.00	6811.0
324.10	1252.0
327.00	1500.0
328.10	787.0
332.90	754.0
334.10	4105.0
335.10	1474.0
336.00	385.0
341.10	999.0
346.00	1470.0
346.90	382.0
352.10	2049.0
353.00	2045.0
354.00	2569.0
355.00	645.0
365.00	9438.0
366.00	1515.0
370.80	541.0
371.20	532.0
372.10	3993.0
373.00	724.0
382.90	1141.0
390.00	539.0
391.00	428.0
402.00	1841.0
403.00	2391.0
403.90	763.0
405.00	398.0
421.00	2469.0
422.00	1508.0
423.00	12483.0
424.10	5199.0
425.00	816.0
441.10	38320.0
442.00	264960.0
443.10	51976.0
444.10	5380.0
445.00	498.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

m/z	Abundance
36.90	467.0
38.10	1956.0
39.10	11649.0
40.10	967.0
41.10	470.0
44.00	2063.0
44.90	308.0
49.10	971.0
50.10	41768.0
51.10	165440.0
52.10	8670.0
54.90	904.0
56.00	4046.0
57.00	10727.0
58.00	458.0
61.00	1598.0
62.00	2095.0
63.10	6004.0
64.00	901.0
65.10	2902.0
66.00	321.0
68.00	2595.0
69.00	147264.0
70.00	737.0
73.00	1199.0
74.10	15478.0
75.00	24832.0
76.10	7456.0
77.10	163328.0
78.10	10279.0
79.00	10856.0
80.00	10295.0
81.00	12808.0
82.10	3631.0
83.00	2907.0
84.00	413.0
85.10	2345.0
86.00	4209.0
87.00	1894.0
88.10	732.0
88.90	308.0
91.00	2863.0
92.10	3643.0
93.00	20232.0
94.00	1463.0
95.00	393.0
96.00	956.0
98.00	16384.0
99.00	12774.0
100.10	969.0
101.00	7026.0
101.90	639.0
103.00	2159.0
104.00	4733.0
105.00	4256.0
106.00	1883.0
107.00	61160.0
108.00	8874.0
109.00	1684.0
110.00	103384.0
111.00	14890.0
112.10	1500.0
113.00	643.0
116.00	3011.0
117.00	47856.0
118.10	3136.0
119.10	393.0
120.00	480.0
122.00	3591.0
123.00	5736.0
124.00	2756.0
125.00	2872.0
126.10	911.0
127.00	197376.0
128.00	14671.0
129.00	80832.0
130.00	7581.0
131.00	1565.0
131.90	697.0
132.90	427.0
134.10	2578.0
135.00	6458.0
136.10	2826.0
137.10	3279.0
137.90	837.0
138.90	382.0
140.00	870.0
141.00	9836.0
142.00	3163.0
143.00	2044.0
144.00	792.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

145.10	489.0
146.00	1935.0
147.00	5310.0
148.00	11736.0
149.10	2654.0
150.00	834.0
151.10	1479.0
151.80	609.0
152.10	586.0
153.00	4234.0
154.00	2621.0
155.00	6467.0
156.00	9810.0
157.10	1550.0
158.00	1481.0
159.00	1628.0
160.00	3925.0
161.00	4556.0
162.10	1386.0
163.00	456.0
164.00	603.0
165.00	3975.0
166.00	3196.0
167.00	20848.0
168.10	10711.0
169.00	1670.0
169.90	492.0
171.00	913.0
172.00	2137.0
173.00	2413.0
174.10	4258.0
175.00	8381.0
176.10	1893.0
177.10	4051.0
177.90	1651.0
179.00	15618.0
180.00	10862.0
181.00	5162.0
182.00	851.0
182.80	520.0
184.00	1662.0
185.00	7335.0
186.00	60248.0
187.10	17864.0
188.10	1784.0
189.10	3437.0
190.00	877.0
191.00	2219.0
192.00	4420.0
193.10	6628.0
194.10	1229.0
195.00	576.0
196.10	10557.0
197.10	3037.0
198.00	446464.0
199.00	30536.0
200.00	2229.0
201.30	1274.0
201.70	1525.0
203.00	3131.0
204.00	16022.0
205.10	26824.0
206.10	117976.0
207.10	15884.0
208.00	4109.0
209.00	1647.0
210.10	1910.0
211.10	4329.0
213.00	327.0
215.00	1299.0
216.00	2781.0
217.00	30088.0
218.00	3491.0
219.20	522.0
221.00	13115.0
221.90	3258.0
223.00	6396.0
224.10	61464.0
225.10	14377.0
226.10	2143.0
227.00	28256.0
228.10	3447.0
229.00	5532.0
229.90	726.0
231.00	2174.0
232.00	495.0
233.10	526.0
234.00	2413.0
235.10	1364.0
236.00	1320.0
237.00	3346.0
237.90	478.0
239.00	919.0
240.10	1082.0
241.00	1403.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

242.10	3206.0
243.10	3143.0
244.10	46456.0
245.10	5831.0
246.00	9808.0
247.00	1819.0
248.00	575.0
249.00	1526.0
250.80	325.0
252.00	687.0
253.10	1340.0
254.10	2645.0
255.00	252288.0
256.00	37136.0
257.00	3383.0
258.00	15499.0
259.00	2205.0
259.90	383.0
260.90	435.0
264.00	301.0
265.00	6056.0
265.90	860.0
270.20	306.0
270.90	498.0
272.00	580.0
273.00	8163.0
274.00	20864.0
275.00	108424.0
276.00	14773.0
277.00	9099.0
278.00	1766.0
283.00	733.0
283.90	676.0
285.10	1311.0
286.00	325.0
288.90	433.0
289.90	375.0
291.90	470.0
293.00	2205.0
293.80	785.0
295.00	765.0
296.00	28424.0
297.00	4520.0
301.00	482.0
302.10	637.0
303.10	3577.0
304.00	1505.0
307.80	438.0
309.90	371.0
314.00	1274.0
315.00	3055.0
316.00	2070.0
317.00	338.0
321.00	1042.0
322.00	578.0
323.10	9687.0
324.10	1752.0
327.00	1698.0
328.00	1307.0
331.90	680.0
333.00	1166.0
334.10	6818.0
335.00	1831.0
341.00	1543.0
346.00	2396.0
347.00	634.0
352.10	3104.0
353.00	1475.0
354.00	3862.0
355.10	664.0
365.00	13459.0
366.00	1732.0
369.90	395.0
370.90	716.0
372.00	5490.0
373.10	947.0
383.10	1522.0
384.10	408.0
390.00	648.0
391.00	606.0
391.90	459.0
400.80	637.0
402.00	2369.0
403.10	2794.0
404.10	1098.0
421.00	2739.0
422.00	2835.0
423.00	22088.0
424.10	6111.0
425.00	748.0
438.10	311.0
438.90	368.0
441.00	65696.0
442.00	418560.0
443.10	83248.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

444.10

8645.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

m/z	Abundance
37.00	364.0
38.00	1079.0
39.10	7437.0
40.00	585.0
41.00	318.0
44.00	2319.0
49.00	760.0
50.10	26960.0
51.10	110752.0
52.00	4998.0
54.90	579.0
56.00	3156.0
57.00	7695.0
61.00	1328.0
62.00	1576.0
63.00	3999.0
64.10	910.0
65.10	2306.0
68.00	1531.0
69.00	98216.0
70.00	377.0
73.10	1069.0
74.00	10450.0
75.00	16864.0
76.10	5072.0
77.10	114256.0
78.10	7080.0
79.00	8016.0
80.00	5697.0
81.00	9426.0
82.00	2366.0
83.00	2020.0
85.10	1657.0
86.10	2507.0
87.00	1547.0
88.00	384.0
91.00	2187.0
92.10	2591.0
93.00	15351.0
94.10	897.0
96.00	647.0
98.00	11931.0
99.00	8740.0
100.10	908.0
101.00	5141.0
102.00	376.0
103.00	1317.0
104.00	3171.0
105.10	3016.0
106.00	989.0
107.00	41480.0
108.00	5235.0
109.00	1018.0
110.00	73728.0
111.00	11421.0
112.00	1567.0
113.00	465.0
116.00	2310.0
117.00	32008.0
118.00	2268.0
118.90	338.0
119.90	355.0
122.00	2623.0
123.00	4303.0
124.00	1815.0
125.00	1980.0
126.10	713.0
127.00	143808.0
128.00	10383.0
129.00	57704.0
130.00	4136.0
131.00	1001.0
132.00	510.0
133.00	425.0
134.00	2265.0
135.00	4521.0
136.00	1748.0
137.10	2542.0
137.90	402.0
138.20	354.0
140.10	529.0
141.00	7668.0
142.10	2455.0
142.90	1585.0
143.90	415.0
144.90	364.0
146.10	1445.0
147.00	3698.0
148.00	10096.0
149.00	2236.0
150.00	597.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

151.20	1110.0
152.00	392.0
153.00	2669.0
154.00	1644.0
155.00	4317.0
156.00	6969.0
157.10	1768.0
158.00	1289.0
159.00	1188.0
159.90	2807.0
161.00	3749.0
162.00	1327.0
162.90	334.0
164.10	425.0
165.00	3518.0
166.00	2436.0
167.00	14915.0
168.00	7414.0
169.00	1529.0
170.10	372.0
170.80	706.0
171.90	1597.0
173.00	2012.0
174.00	3862.0
175.10	6779.0
176.10	1493.0
177.00	2729.0
178.10	719.0
179.00	11653.0
180.00	9762.0
181.00	3735.0
181.90	644.0
184.00	979.0
185.00	5475.0
186.00	45104.0
187.00	12941.0
188.00	1468.0
189.10	3236.0
190.00	528.0
191.10	1397.0
192.00	3600.0
193.10	3998.0
194.00	1083.0
195.20	647.0
196.00	8768.0
197.10	2653.0
198.00	348160.0
199.00	23840.0
200.00	1935.0
201.40	956.0
202.10	535.0
203.10	2222.0
204.00	13045.0
205.10	20000.0
206.10	93904.0
207.10	12091.0
208.10	3698.0
209.10	1131.0
210.00	1760.0
211.10	3484.0
215.10	1157.0
215.90	1564.0
217.00	23512.0
218.10	2964.0
221.00	10411.0
222.00	2873.0
223.00	4977.0
224.10	49048.0
225.10	11785.0
226.00	1615.0
227.00	20768.0
228.10	3438.0
229.00	4109.0
230.00	759.0
231.10	1768.0
232.00	334.0
233.10	380.0
234.10	1306.0
234.90	1382.0
236.00	1277.0
237.00	1990.0
238.00	375.0
238.90	595.0
240.00	762.0
240.90	962.0
242.00	2708.0
243.00	3004.0
244.10	37448.0
245.10	4985.0
246.00	7270.0
247.00	1867.0
248.10	338.0
249.00	1149.0
250.90	483.0
252.00	413.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

252.90	862.0
254.20	2212.0
255.00	205632.0
256.00	30104.0
257.10	2523.0
258.00	11791.0
259.00	1583.0
260.90	354.0
264.00	479.0
265.00	4880.0
266.00	696.0
271.00	523.0
272.00	409.0
273.00	6261.0
274.00	16808.0
275.00	89336.0
276.00	12135.0
277.00	7574.0
277.90	1071.0
283.00	1071.0
284.10	498.0
285.10	1244.0
289.00	341.0
291.90	477.0
293.00	2090.0
294.00	340.0
295.10	563.0
296.00	24872.0
297.00	3723.0
298.10	421.0
300.80	303.0
302.00	430.0
303.00	3096.0
304.00	1324.0
308.00	368.0
310.00	391.0
313.10	322.0
314.10	1669.0
315.00	3055.0
316.00	1467.0
321.00	815.0
321.90	333.0
323.10	8478.0
324.00	1306.0
327.00	2090.0
327.90	825.0
331.90	668.0
333.00	505.0
334.10	5723.0
335.10	787.0
341.10	948.0
342.00	448.0
346.00	1909.0
346.90	448.0
352.10	2040.0
353.00	1645.0
354.10	3018.0
354.90	468.0
365.00	12003.0
366.00	1732.0
369.90	312.0
371.00	801.0
372.00	4815.0
372.90	1211.0
382.90	1443.0
384.00	631.0
390.00	609.0
391.00	585.0
402.00	2189.0
403.00	3051.0
404.00	1064.0
405.00	418.0
421.10	2642.0
422.00	2971.0
423.10	18952.0
424.00	5837.0
424.90	566.0
441.00	60184.0
442.00	406144.0
443.00	75664.0
444.10	6448.0
444.90	341.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

Scan 2515 (17.480 min): BM000536.D
DFTPP24

m/z	Abundance
40.10	475.0
44.00	3060.0
207.10	1552.0
208.00	333.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24