


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021721\
 Data File : BM028763.D
 Acq On : 17 Feb 2021 09:33
 Operator : CG/JU
 Sample : DFTPP31
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP31

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 10:10:00 2021

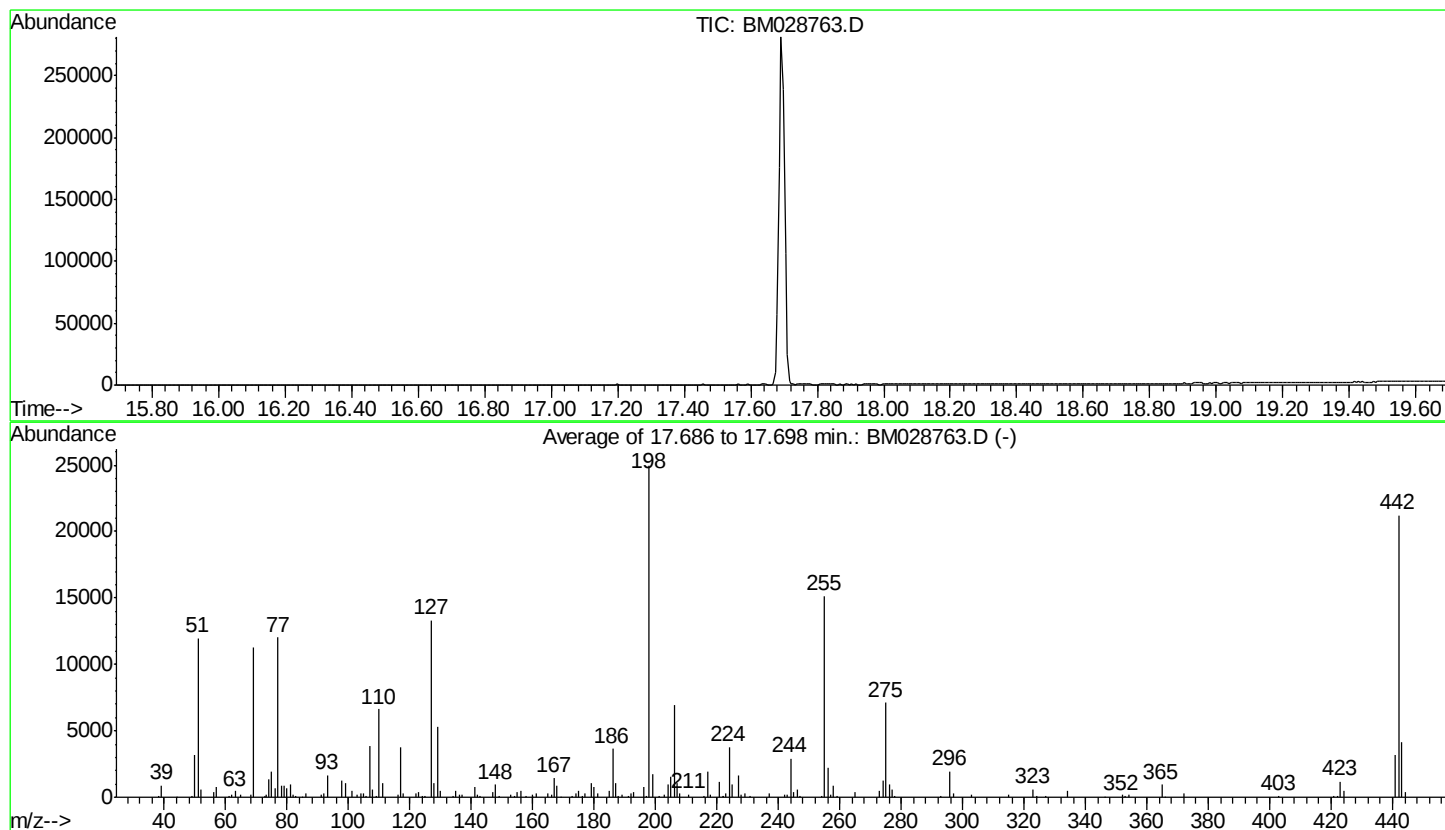

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.9	11958	PASS
68	69	0.00	2	2.0	231	PASS
69	198	0.00	100	45.2	11276	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	13320	PASS
197	198	0.00	2	0.5	135	PASS
198	198	100	100	100.0	24960	PASS
199	198	5	9	6.9	1714	PASS
275	198	10	60	28.4	7087	PASS
365	198	1	100	3.8	955	PASS
441	198	0.01	100	12.6	3140	PASS
442	198	50	100	85.0	21217	PASS
443	442	15	24	19.5	4140	PASS

Scan 2493 (17.651 min): BM028763.D
DFTPP31

m/z	Abundance
44.00	217.0
207.00	235.0

Instrument :

BNA_M

ClientSampleId :

DFTPP31

m/z	Abundance
38.00	167.0
39.00	804.0
43.90	248.0
50.00	3050.0
51.10	10910.0
52.00	627.0
56.00	310.0
57.00	628.0
62.00	151.0
63.00	471.0
65.00	166.0
68.10	220.0
69.00	10020.0
72.90	190.0
74.00	1189.0
75.00	1644.0
76.00	555.0
77.10	10525.0
78.00	752.0
79.00	839.0
80.00	634.0
80.90	805.0
81.90	217.0
85.90	282.0
91.00	159.0
91.90	287.0
93.00	1451.0
98.00	1067.0
99.00	918.0
101.00	416.0
102.90	159.0
104.00	308.0
105.00	237.0
107.00	3265.0
108.00	490.0
110.00	5691.0
110.90	970.0
117.00	3240.0
118.00	242.0
122.00	215.0
122.90	301.0
124.00	165.0
124.90	150.0
127.00	10924.0
128.00	903.0
129.00	4597.0
130.00	376.0
135.00	268.0
135.90	166.0
137.00	184.0
141.00	662.0
141.90	204.0
146.90	371.0
148.00	756.0
152.90	170.0
155.00	348.0
156.00	416.0
159.80	152.0
161.00	236.0
165.00	192.0
167.00	1162.0
167.90	766.0
173.90	235.0
175.00	342.0
176.90	156.0
179.00	867.0
180.00	626.0
181.00	246.0
185.00	341.0
186.00	2786.0
187.00	925.0
190.90	155.0
192.00	219.0
193.00	330.0
195.90	555.0
198.00	19320.0
198.90	1501.0
203.90	713.0
205.00	1212.0
206.00	5201.0
207.00	1091.0
208.00	208.0
210.90	186.0
217.00	1458.0
221.00	854.0
221.80	167.0
223.00	267.0
224.00	2772.0
225.00	690.0
227.00	1309.0
228.00	179.0
229.00	258.0

Instrument :
BNA_M
ClientSampleId :
DFTPP31

237.00	241.0
242.00	166.0
244.00	2044.0
245.00	245.0
246.00	484.0
255.00	10546.0
256.00	1581.0
256.90	160.0
258.00	640.0
264.90	300.0
273.00	358.0
274.00	821.0
275.00	4947.0
276.00	661.0
276.90	395.0
295.90	1292.0
297.00	198.0
303.00	164.0
323.00	325.0
333.90	226.0
364.90	541.0
372.00	188.0
423.00	681.0
424.00	350.0
441.00	1732.0
442.00	11413.0
443.00	2283.0
444.00	191.0

Instrument :
BNA_M
ClientSampleId :
DFTPP31

m/z	Abundance
38.00	170.0
39.10	1103.0
44.00	272.0
49.10	166.0
50.00	3851.0
51.10	14435.0
52.00	746.0
56.00	440.0
57.00	1042.0
61.00	190.0
62.00	164.0
63.00	597.0
65.00	252.0
68.10	266.0
69.00	13576.0
73.10	213.0
74.00	1703.0
75.00	2226.0
76.10	831.0
77.10	14675.0
78.00	1137.0
79.00	1037.0
80.00	746.0
81.00	1157.0
81.90	211.0
82.90	216.0
85.00	155.0
86.00	361.0
90.90	241.0
92.00	297.0
93.00	1972.0
98.00	1553.0
99.00	1250.0
101.00	635.0
102.90	296.0
103.90	415.0
104.90	375.0
105.90	159.0
107.00	4752.0
108.00	710.0
109.00	163.0
110.00	8036.0
111.00	1197.0
116.00	323.0
117.00	4640.0
117.90	362.0
121.90	331.0
123.00	542.0
123.90	256.0
124.90	209.0
127.00	16298.0
128.00	1237.0
129.00	6540.0
129.90	580.0
133.90	155.0
135.00	609.0
136.00	210.0
137.10	288.0
140.90	970.0
141.90	261.0
142.90	247.0
147.00	457.0
148.00	1081.0
148.90	245.0
152.90	251.0
153.90	171.0
155.00	454.0
156.00	557.0
157.90	175.0
160.00	255.0
161.00	355.0
165.00	303.0
166.00	204.0
167.00	1856.0
168.00	958.0
172.90	154.0
173.90	329.0
175.00	666.0
176.00	187.0
176.90	335.0
179.00	1296.0
180.00	988.0
181.00	397.0
185.00	606.0
186.00	4506.0
187.00	1221.0
188.00	169.0
189.00	282.0
192.00	319.0
193.00	487.0
196.00	855.0
197.00	234.0

Instrument :
BNA_M
ClientSampleId :
DFTPP31

198.00	29784.0
198.90	1996.0
201.20	185.0
203.00	316.0
204.00	1166.0
205.00	2002.0
206.00	8219.0
207.00	1483.0
208.00	388.0
211.00	322.0
215.90	175.0
217.00	2295.0
217.90	300.0
221.00	1246.0
223.00	435.0
224.00	4575.0
225.00	1149.0
227.00	1833.0
228.00	259.0
229.00	414.0
230.90	161.0
236.90	282.0
241.90	205.0
242.90	247.0
244.00	3446.0
245.00	380.0
246.00	716.0
247.00	174.0
254.10	166.0
255.00	17960.0
256.00	2644.0
257.00	278.0
258.00	998.0
258.90	193.0
265.00	411.0
272.90	548.0
274.00	1427.0
275.00	8618.0
276.00	1217.0
277.00	695.0
278.00	193.0
293.00	162.0
296.00	2329.0
296.90	331.0
303.00	275.0
315.00	232.0
323.00	663.0
327.00	206.0
334.00	589.0
352.00	249.0
352.90	172.0
354.00	226.0
364.90	1138.0
365.90	151.0
372.00	371.0
403.00	238.0
421.00	202.0
421.90	157.0
423.00	1400.0
423.90	645.0
441.00	3651.0
442.00	24912.0
443.00	4792.0
444.00	446.0

Instrument :
BNA_M
ClientSampleId :
DFTPP31

m/z	Abundance
39.00	728.0
43.90	277.0
50.00	2783.0
51.10	10529.0
52.00	501.0
56.00	293.0
57.00	612.0
60.90	155.0
62.00	161.0
63.00	375.0
65.00	162.0
68.10	207.0
69.00	10232.0
73.10	235.0
74.00	1093.0
75.00	1781.0
76.00	542.0
77.10	10882.0
78.10	748.0
79.00	854.0
80.00	555.0
80.90	823.0
81.90	212.0
82.90	168.0
86.00	244.0
91.00	175.0
92.00	251.0
93.00	1588.0
98.00	1037.0
99.00	930.0
101.00	534.0
103.00	186.0
103.90	297.0
105.00	292.0
107.00	3641.0
108.00	546.0
110.00	6219.0
111.00	964.0
116.00	185.0
117.00	3512.0
118.00	275.0
121.90	200.0
122.90	326.0
127.00	12740.0
128.00	922.0
129.00	4912.0
129.90	416.0
133.90	155.0
135.00	463.0
135.90	223.0
137.00	231.0
140.90	669.0
142.00	246.0
146.90	353.0
148.00	932.0
148.90	193.0
152.90	210.0
154.90	345.0
156.00	525.0
159.90	215.0
161.00	341.0
165.00	287.0
166.00	257.0
167.00	1332.0
167.90	802.0
168.90	155.0
173.00	153.0
174.00	272.0
175.00	490.0
176.00	192.0
177.00	243.0
178.90	1013.0
180.00	776.0
180.90	297.0
185.00	514.0
186.00	3623.0
187.00	1060.0
188.90	213.0
191.00	185.0
192.00	321.0
193.00	421.0
195.90	860.0
197.10	173.0
198.00	25776.0
198.90	1645.0
202.90	248.0
204.00	982.0
205.00	1489.0
206.00	7259.0
207.00	1232.0
207.90	345.0
210.80	193.0

Instrument :
BNA_M
ClientSampleId :
DFTPP31

216.00	190.0
217.00	1989.0
217.90	211.0
220.90	1303.0
222.00	278.0
222.90	299.0
224.00	4066.0
225.00	1054.0
227.00	1652.0
228.00	212.0
228.90	344.0
236.90	213.0
242.00	243.0
242.90	250.0
244.00	3193.0
245.00	429.0
246.00	600.0
255.00	16928.0
256.00	2422.0
257.00	222.0
258.00	1000.0
264.90	422.0
273.00	521.0
274.00	1442.0
275.00	7696.0
276.00	1037.0
276.90	647.0
296.00	2164.0
296.90	287.0
303.00	254.0
315.00	325.0
323.00	758.0
324.00	166.0
326.90	176.0
334.00	499.0
346.00	151.0
352.00	310.0
352.80	194.0
353.90	269.0
364.90	1188.0
372.00	365.0
402.90	188.0
420.90	162.0
421.90	199.0
423.00	1473.0
423.90	533.0
441.00	4037.0
442.00	27328.0
443.00	5347.0
444.00	468.0

Instrument :

BNA_M

ClientSampleId :

DFTPP31