




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021725\
Data File : BM049665.D
Acq On : 17 Feb 2025 12:47
Operator : RC/JU
Sample : PB166627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK627

Manual IntegrationsAPPROVED

Quant Time: Feb 18 17:26:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

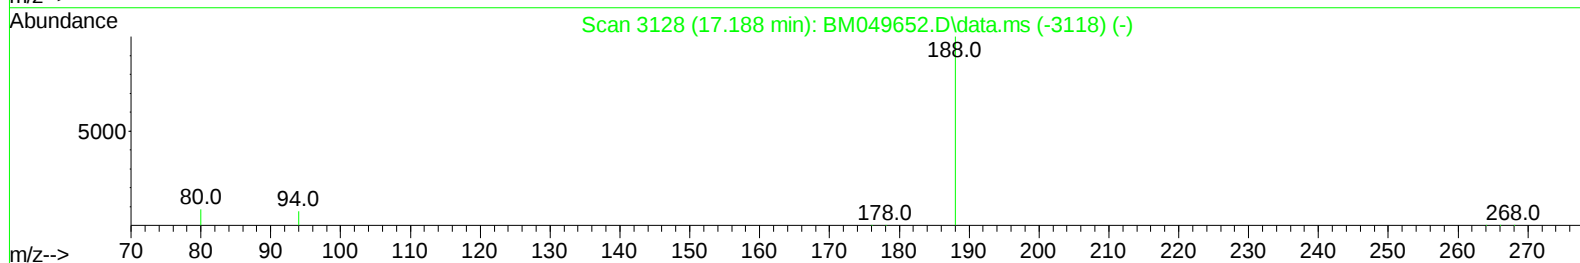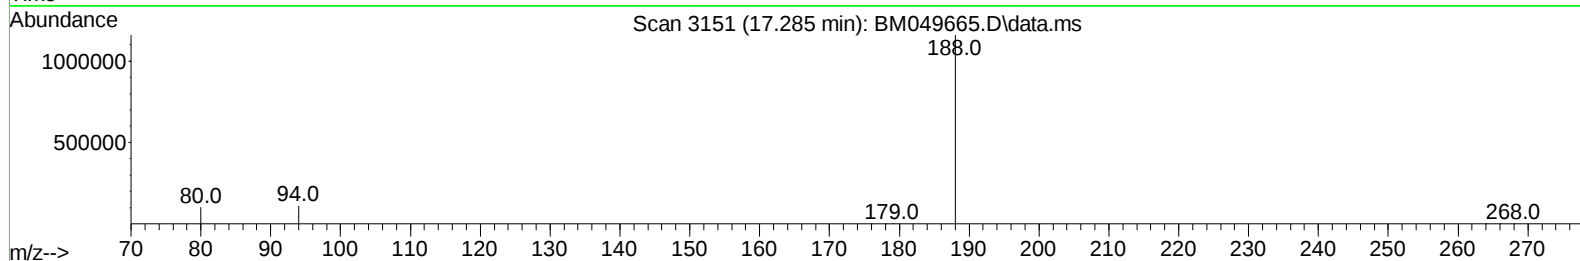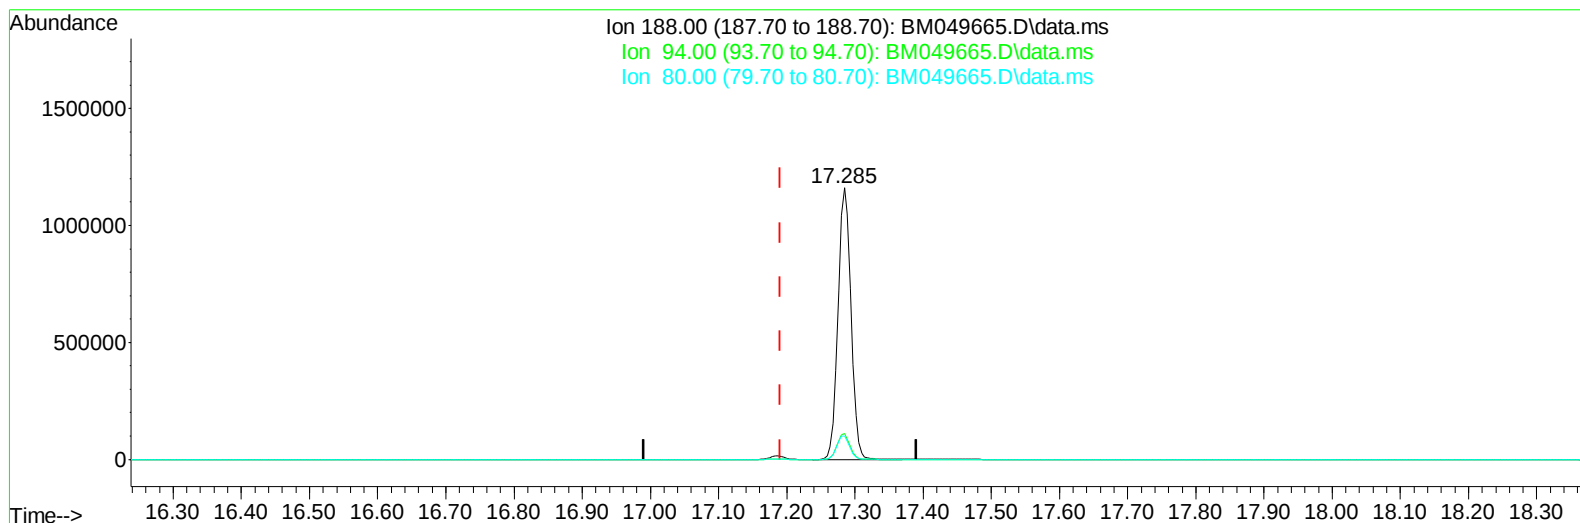

TIC: BM049665.D\data.ms

(13) Phenanthrene-d10 (I)

17.285min (+ 0.094) 0.40 ng/u1

response 1532155

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	8.50	9.48
80.00	9.30	8.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021725\
Data File : BM049665.D
Acq On : 17 Feb 2025 12:47
Operator : RC/JU
Sample : PB166627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK627

Manual IntegrationsAPPROVED

Quant Time: Feb 18 17:26:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

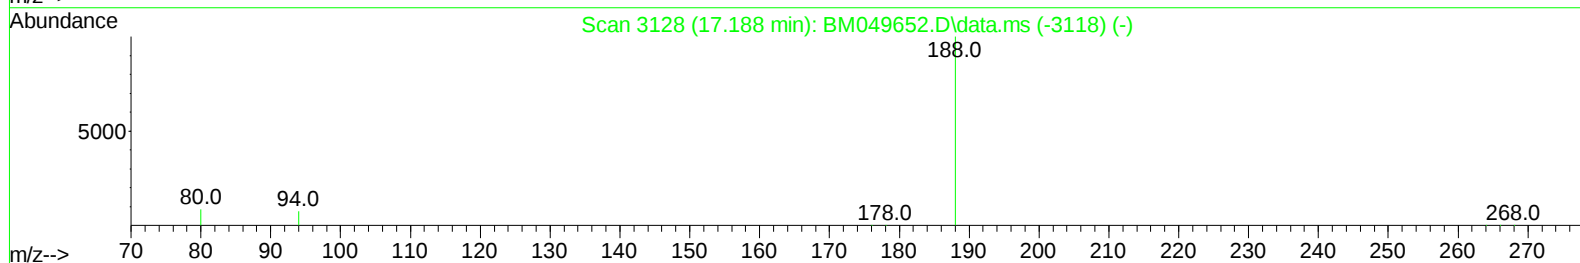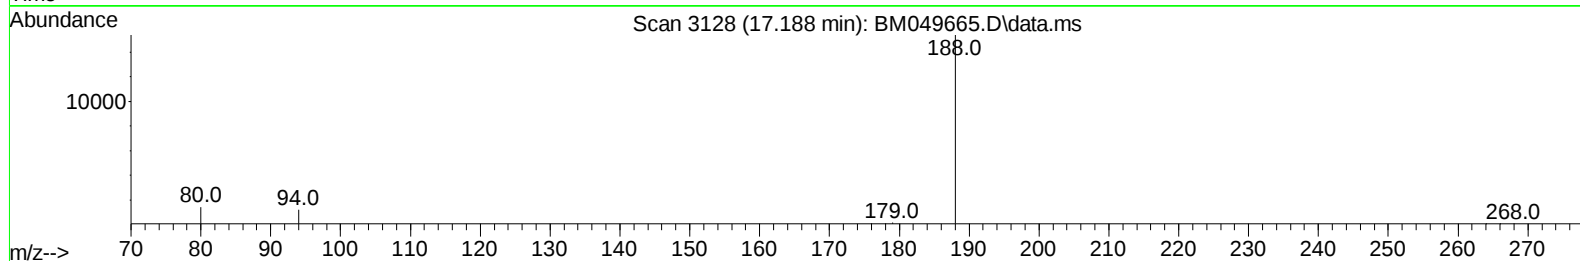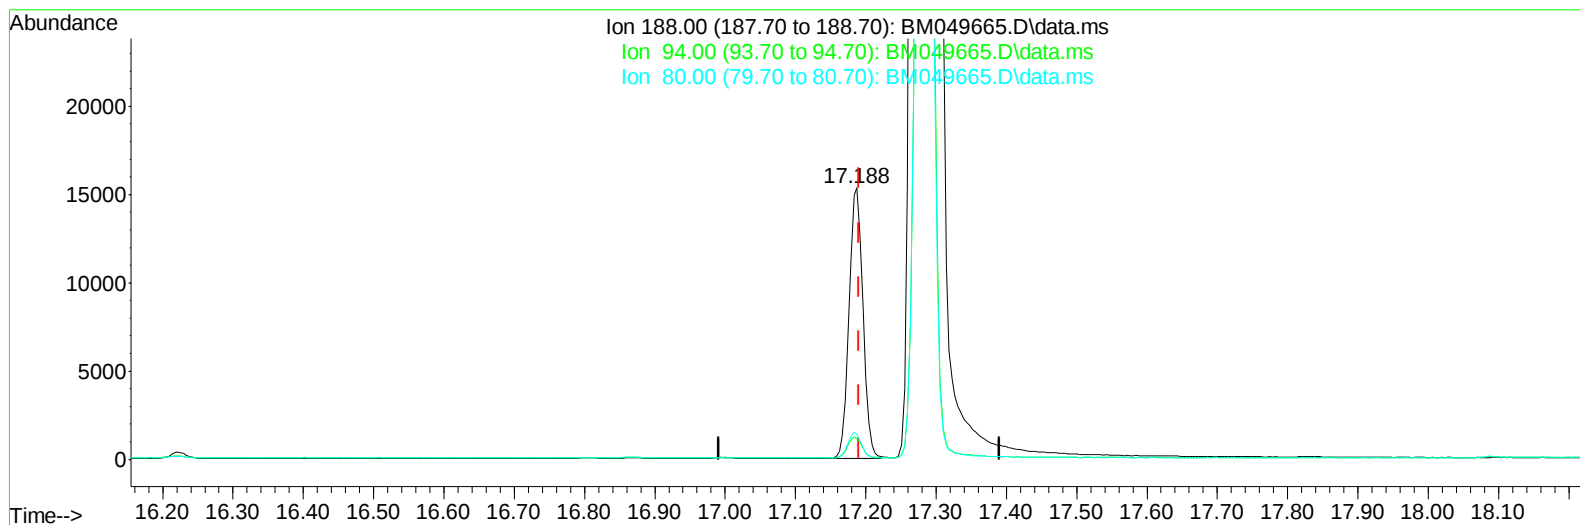

TIC: BM049665.D\data.ms

(13) Phenanthrene-d10 (I)

17.188min (-0.003) 0.40 ng/ul m

response 20820

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	8.50	7.73
80.00	9.30	9.29
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021725\
Data File : BM049665.D
Acq On : 17 Feb 2025 12:47
Operator : RC/JU
Sample : PB166627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK627

Manual IntegrationsAPPROVED

Quant Time: Feb 18 17:26:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

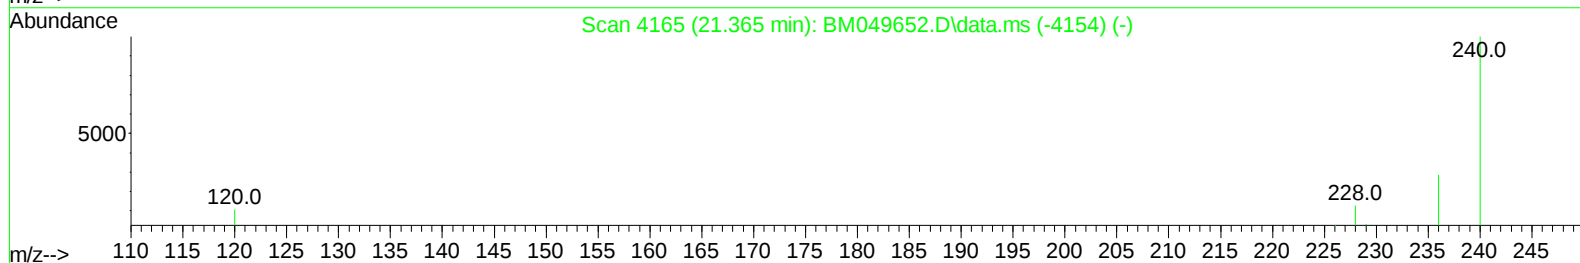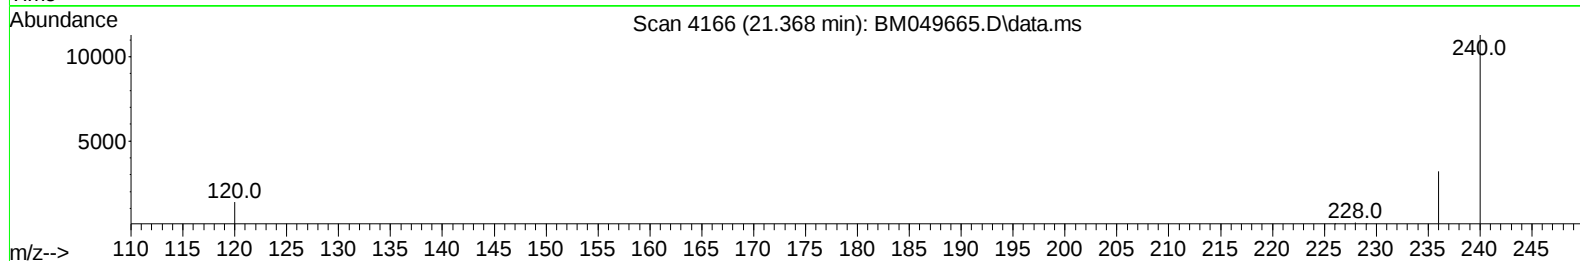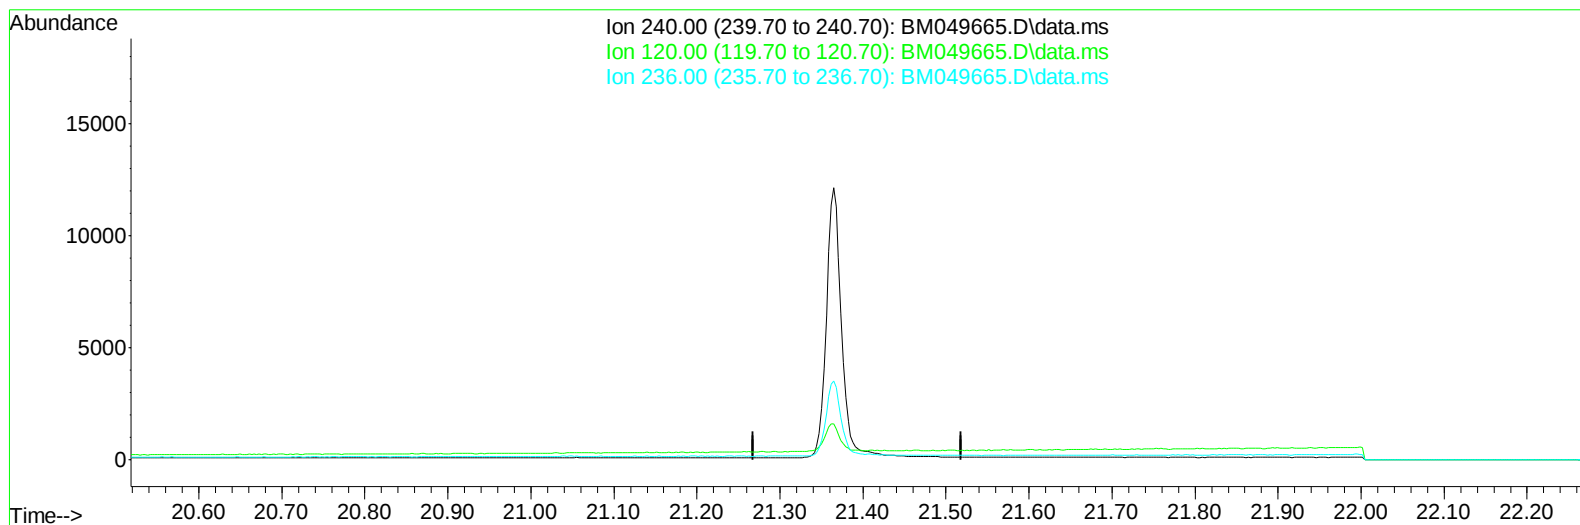

TIC: BM049665.D\data.ms

(17) Chrysene-d12

21.368min (-21.368) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	12.90	0.00#
236.00	29.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021725\
Data File : BM049665.D
Acq On : 17 Feb 2025 12:47
Operator : RC/JU
Sample : PB166627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK627

Manual IntegrationsAPPROVED

Quant Time: Feb 18 17:26:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

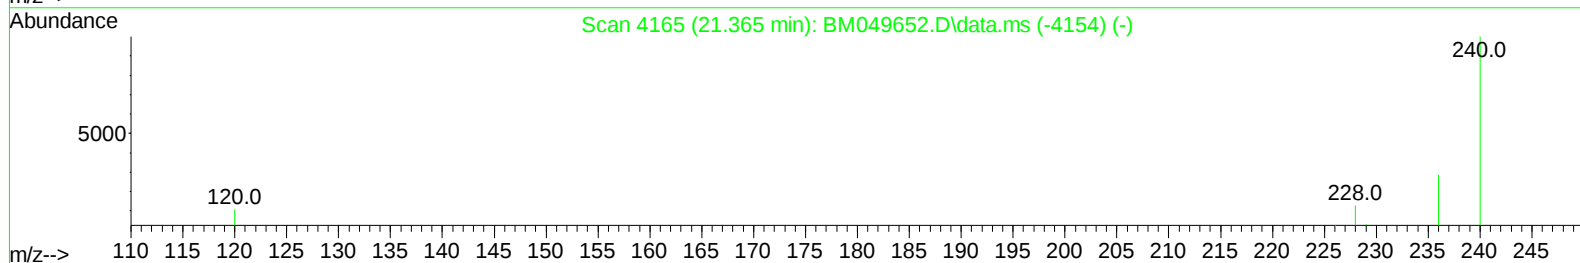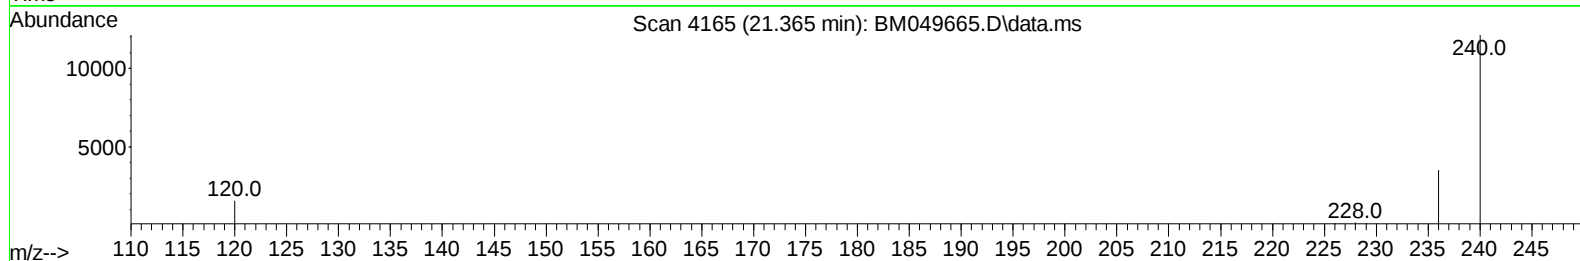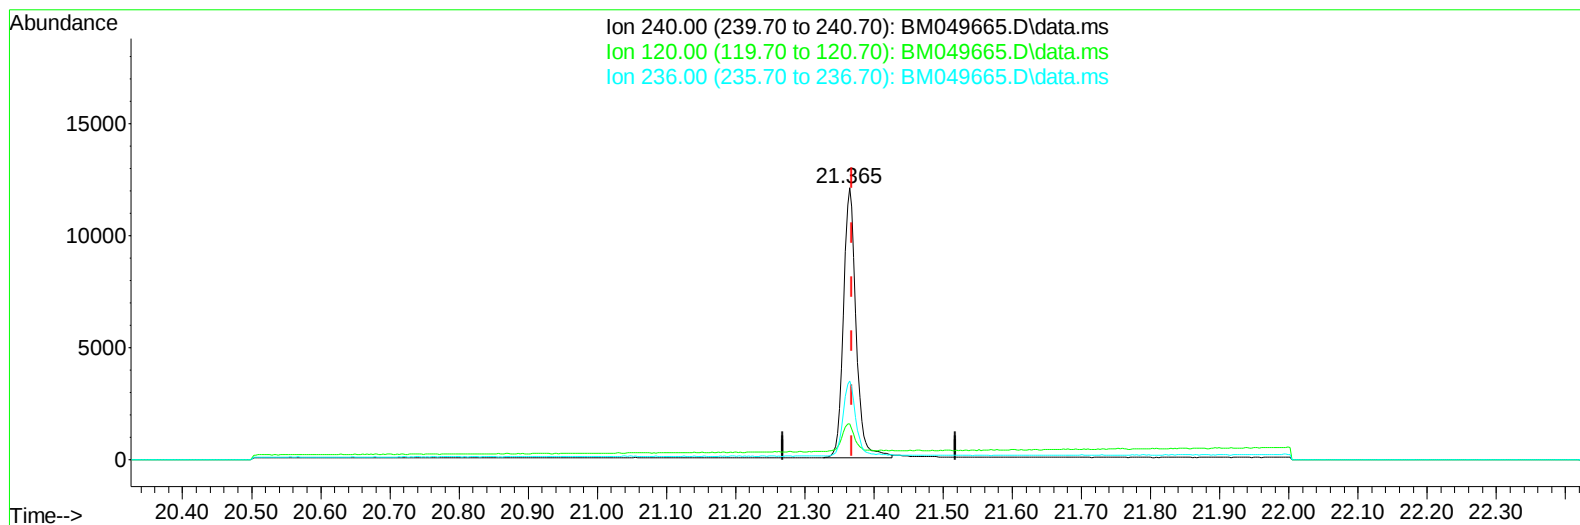

TIC: BM049665.D\data.ms

(17) Chrysene-d12

21.365min (-0.004) 0.40 ng/u1 m

response 15318

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	12.90	13.05
236.00	29.30	28.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021725\
Data File : BM049665.D
Acq On : 17 Feb 2025 12:47
Operator : RC/JU
Sample : PB166627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK627

Manual IntegrationsAPPROVED

Quant Time: Feb 18 17:26:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

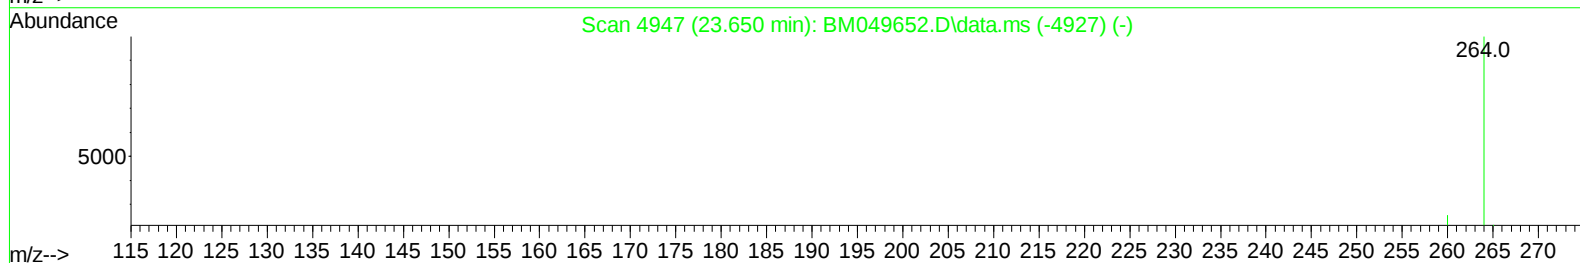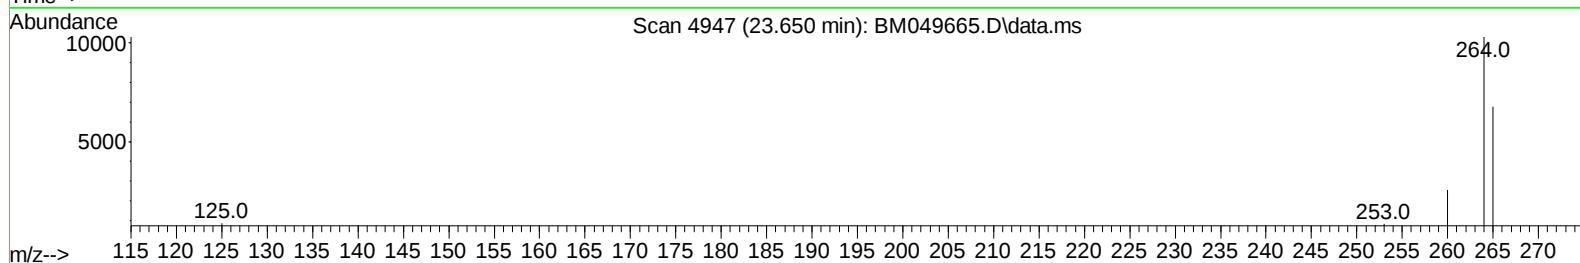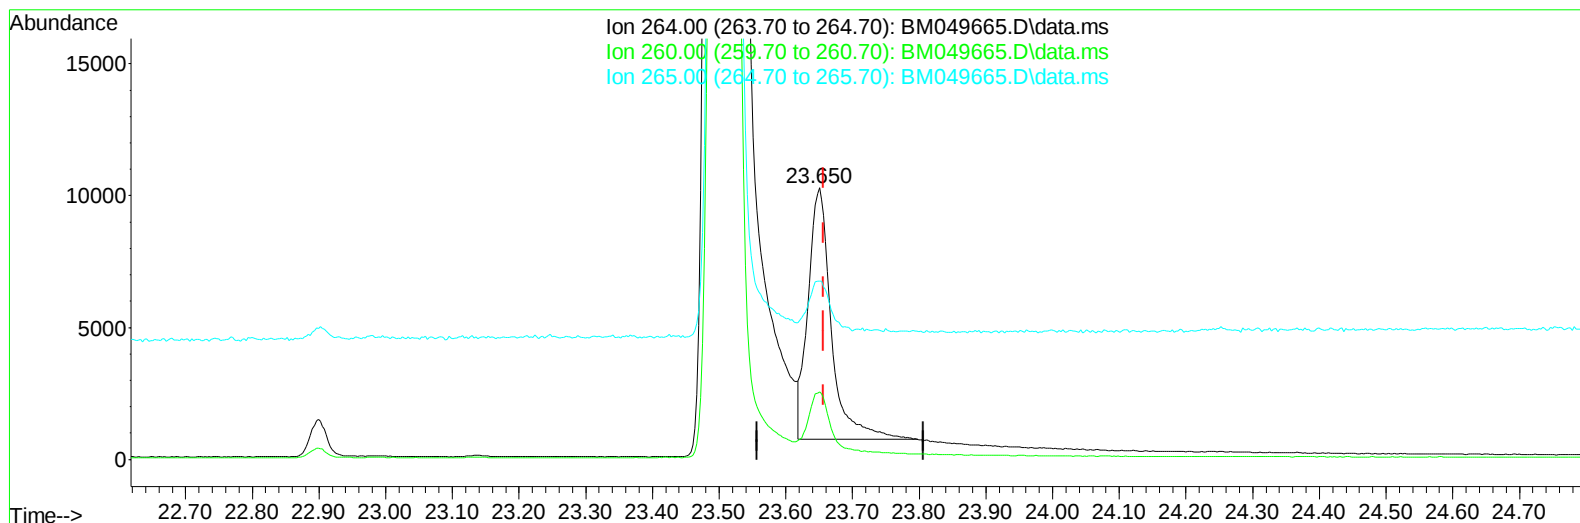

TIC: BM049665.D\data.ms

(23) Perylene-d12 (I)

23.650min (-0.007) 0.40 ng/u1

response 22930

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	24.91
265.00	67.10	65.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021725\
Data File : BM049665.D
Acq On : 17 Feb 2025 12:47
Operator : RC/JU
Sample : PB166627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK627

Manual IntegrationsAPPROVED

Quant Time: Feb 18 17:26:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

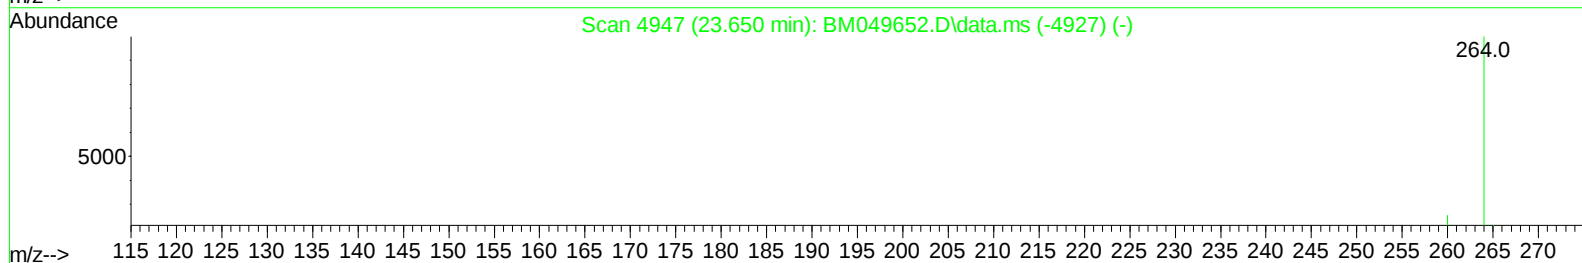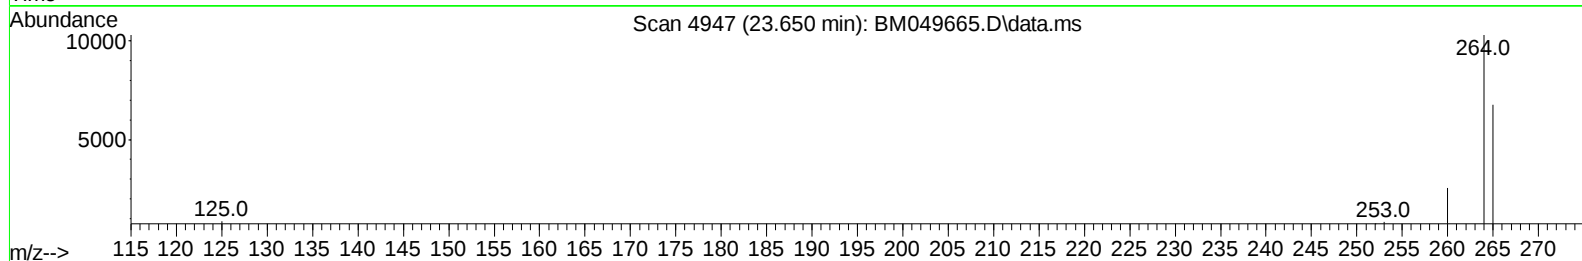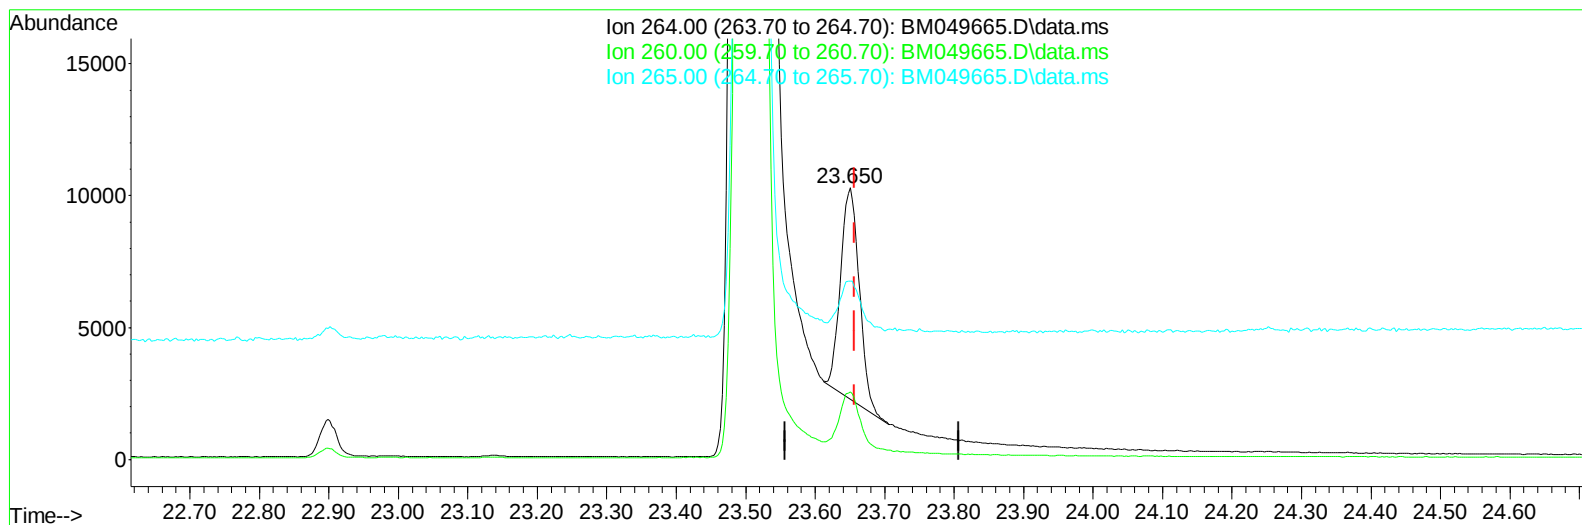

TIC: BM049665.D\data.ms

(23) Perylene-d12 (I)

23.650min (-0.007) 0.40 ng/ul m

response 14869

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	24.91
265.00	67.10	65.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021725\
 Data File : BM049665.D
 Acq On : 17 Feb 2025 12:47
 Operator : RC/JU
 Sample : PB166627BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK627

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 02/19/2025
 Supervised By :Jagrut Upadhyay 02/19/2025

Quant Time: Feb 18 17:26:51 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 12 16:40:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.809	152	7194	0.400	ng/ul	0.00
4) Naphthalene-d8	10.601	136	19072	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.446	164	10433	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.188	188	20820m	0.400	ng/ul	0.00
17) Chrysene-d12	21.365	240	15318m	0.400	ng/ul	0.00
23) Perylene-d12	23.650	264	14869m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	47765	5.902	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.196	152	8415	0.321	ng/ul	0.00
18) Fluoranthene-d10	19.211	212	14874	0.319	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021725\
Data File : BM049665.D
Acq On : 17 Feb 2025 12:47
Operator : RC/JU
Sample : PB166627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK627

Manual IntegrationsAPPROVED

Quant Time: Feb 18 17:26:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 16:40:36 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 02/19/2025
Supervised By :Jagrut Upadhyay 02/19/2025

