
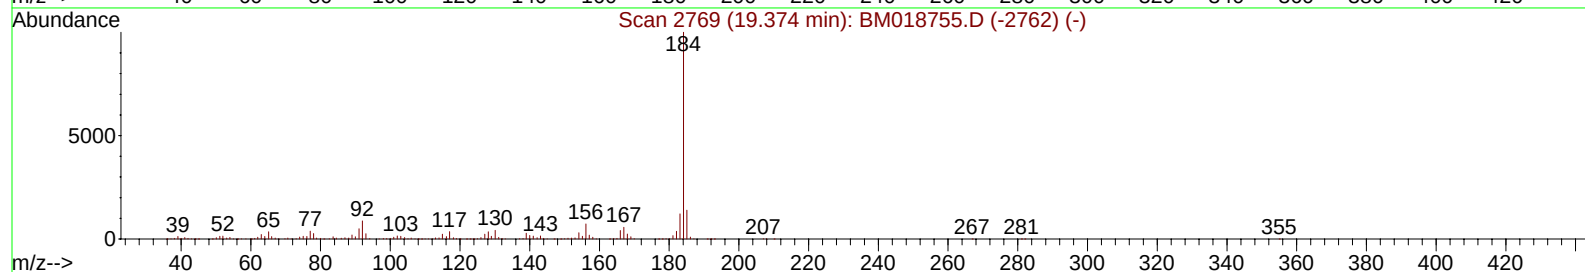
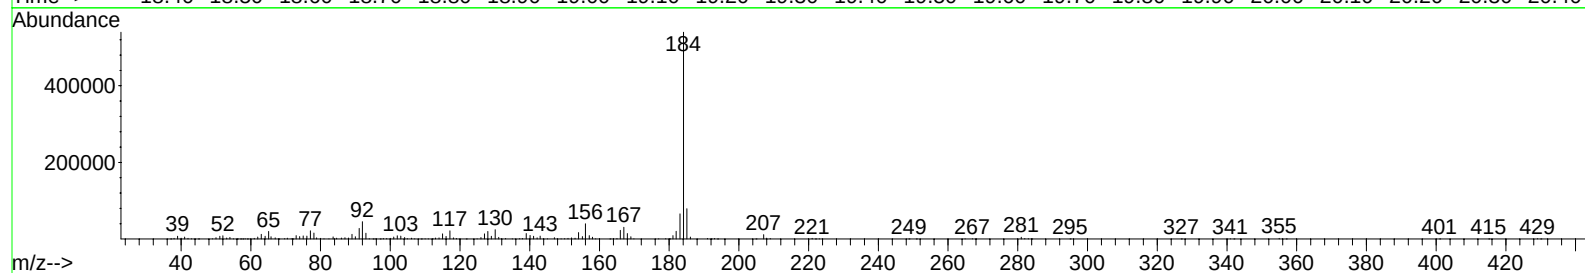


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021819\
Data File : BM018833.D
Acq On : 18 Feb 2019 12:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 17:30:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

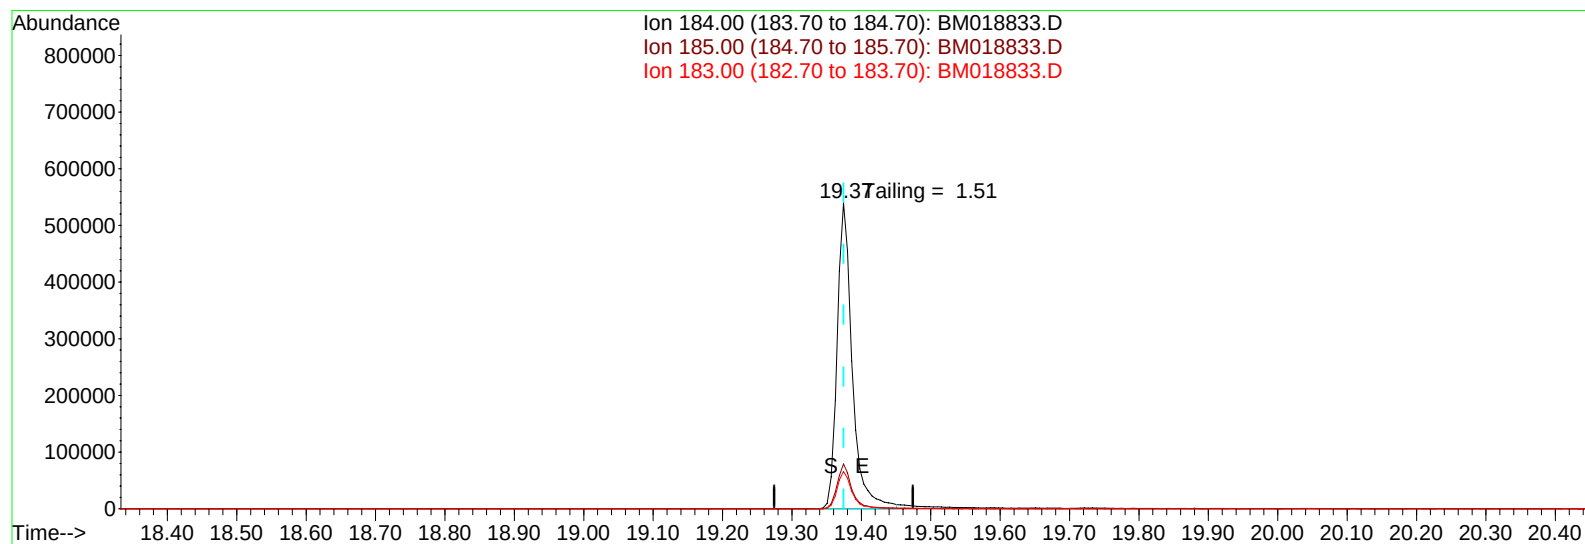

TIC: BM018833.D

(77) Benzidine




19.374min (-0.000) 721.97ng

response 813173

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.65
183.00	12.10	12.18
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021819\
Data File : BM018833.D
Acq On : 18 Feb 2019 12:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 17:30:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

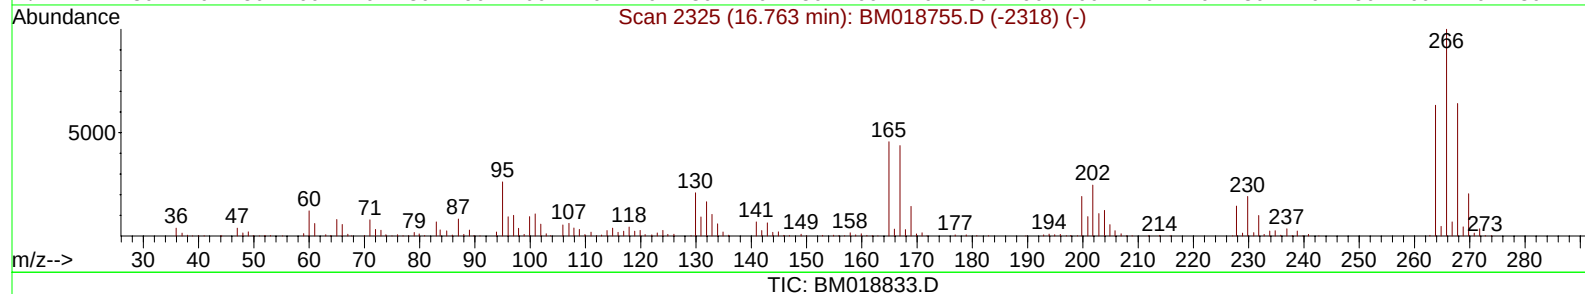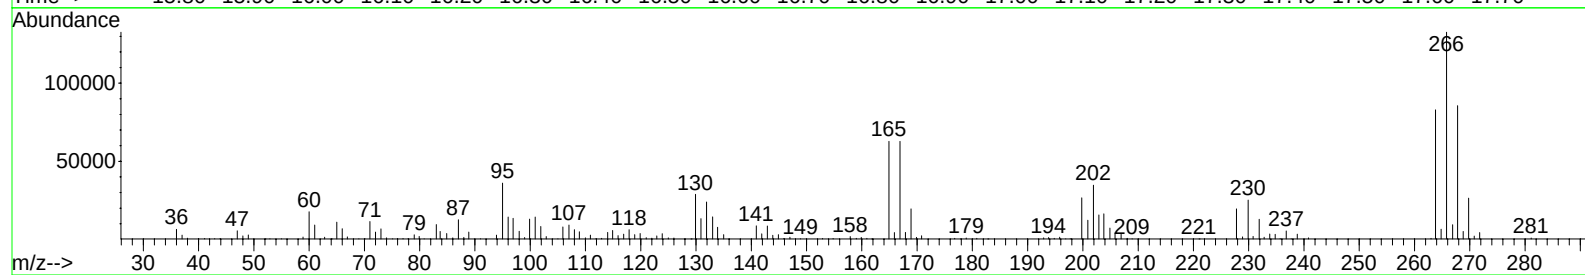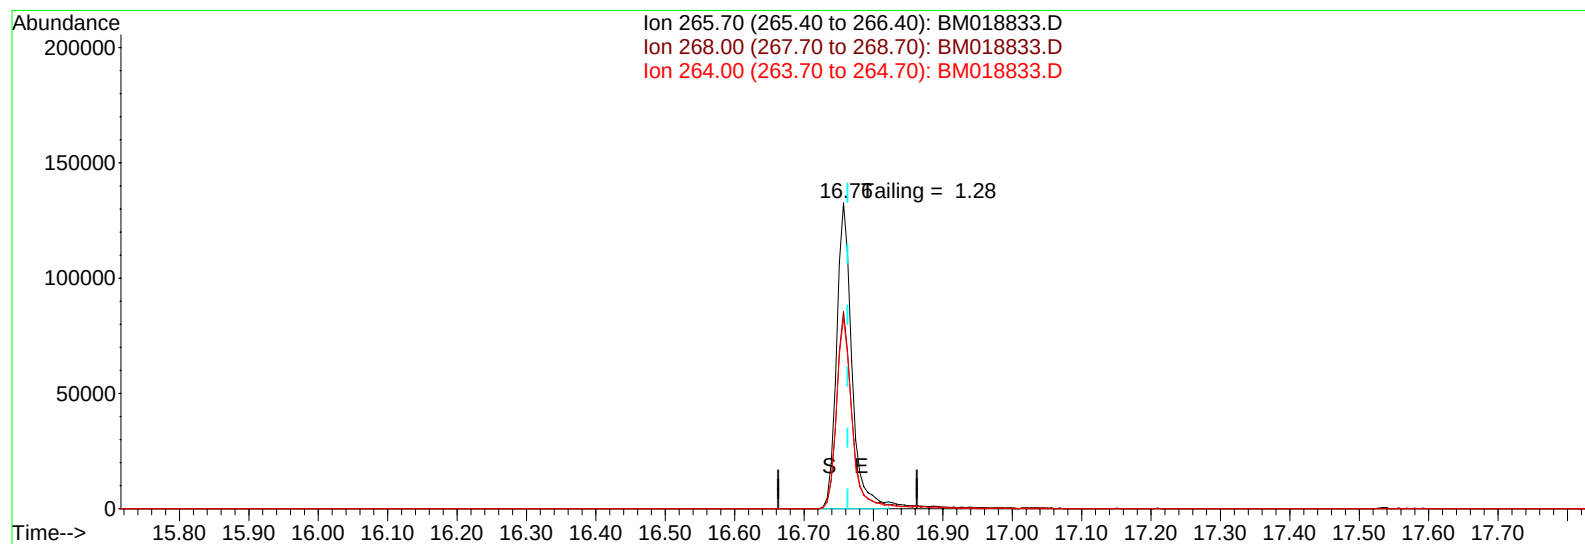

(70) Pentachlorophenol (C)

16.757min (-0.006) 65652.29ng

response 203493

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	64.55
264.00	63.20	62.52
0.00	0.00	0.00