


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021819\
 Data File : BM018833.D
 Acq On : 18 Feb 2019 12:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 11 16:02:12 2019

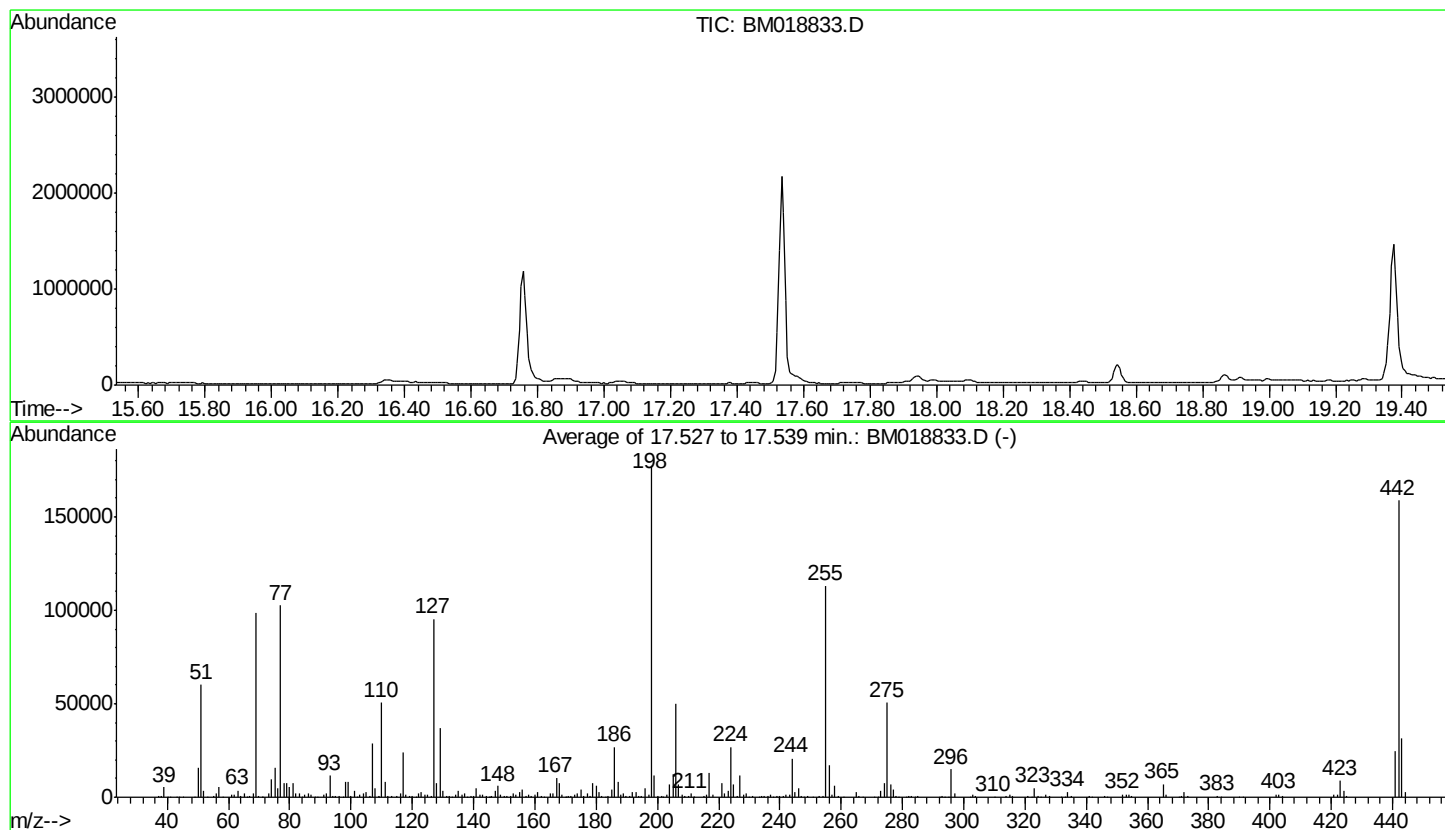

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	60162	PASS
68	69	0.00	2	1.9	1825	PASS
69	198	0.00	100	55.4	98310	PASS
70	69	0.00	2	0.9	863	PASS
127	198	10	80	53.7	95269	PASS
197	198	0.00	2	0.7	1272	PASS
198	198	100	100	100.0	177408	PASS
199	198	5	9	6.6	11668	PASS
275	198	10	60	28.4	50370	PASS
365	198	1	100	4.0	7085	PASS
441	198	0.01	100	13.7	24365	PASS
442	198	50	100	89.5	158802	PASS
443	442	15	24	19.8	31501	PASS