


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028796.D
Acq On : 18 Feb 2021 14:50
Operator : CG/JU
Sample : M1379-11DL 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGZ1DL

Manual Integrations
APPROVED

mohammad
2/19/2021 1:19:45 PM

Quant Time: Feb 18 15:22:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 18 13:03:27 2021
Response via : Initial Calibration

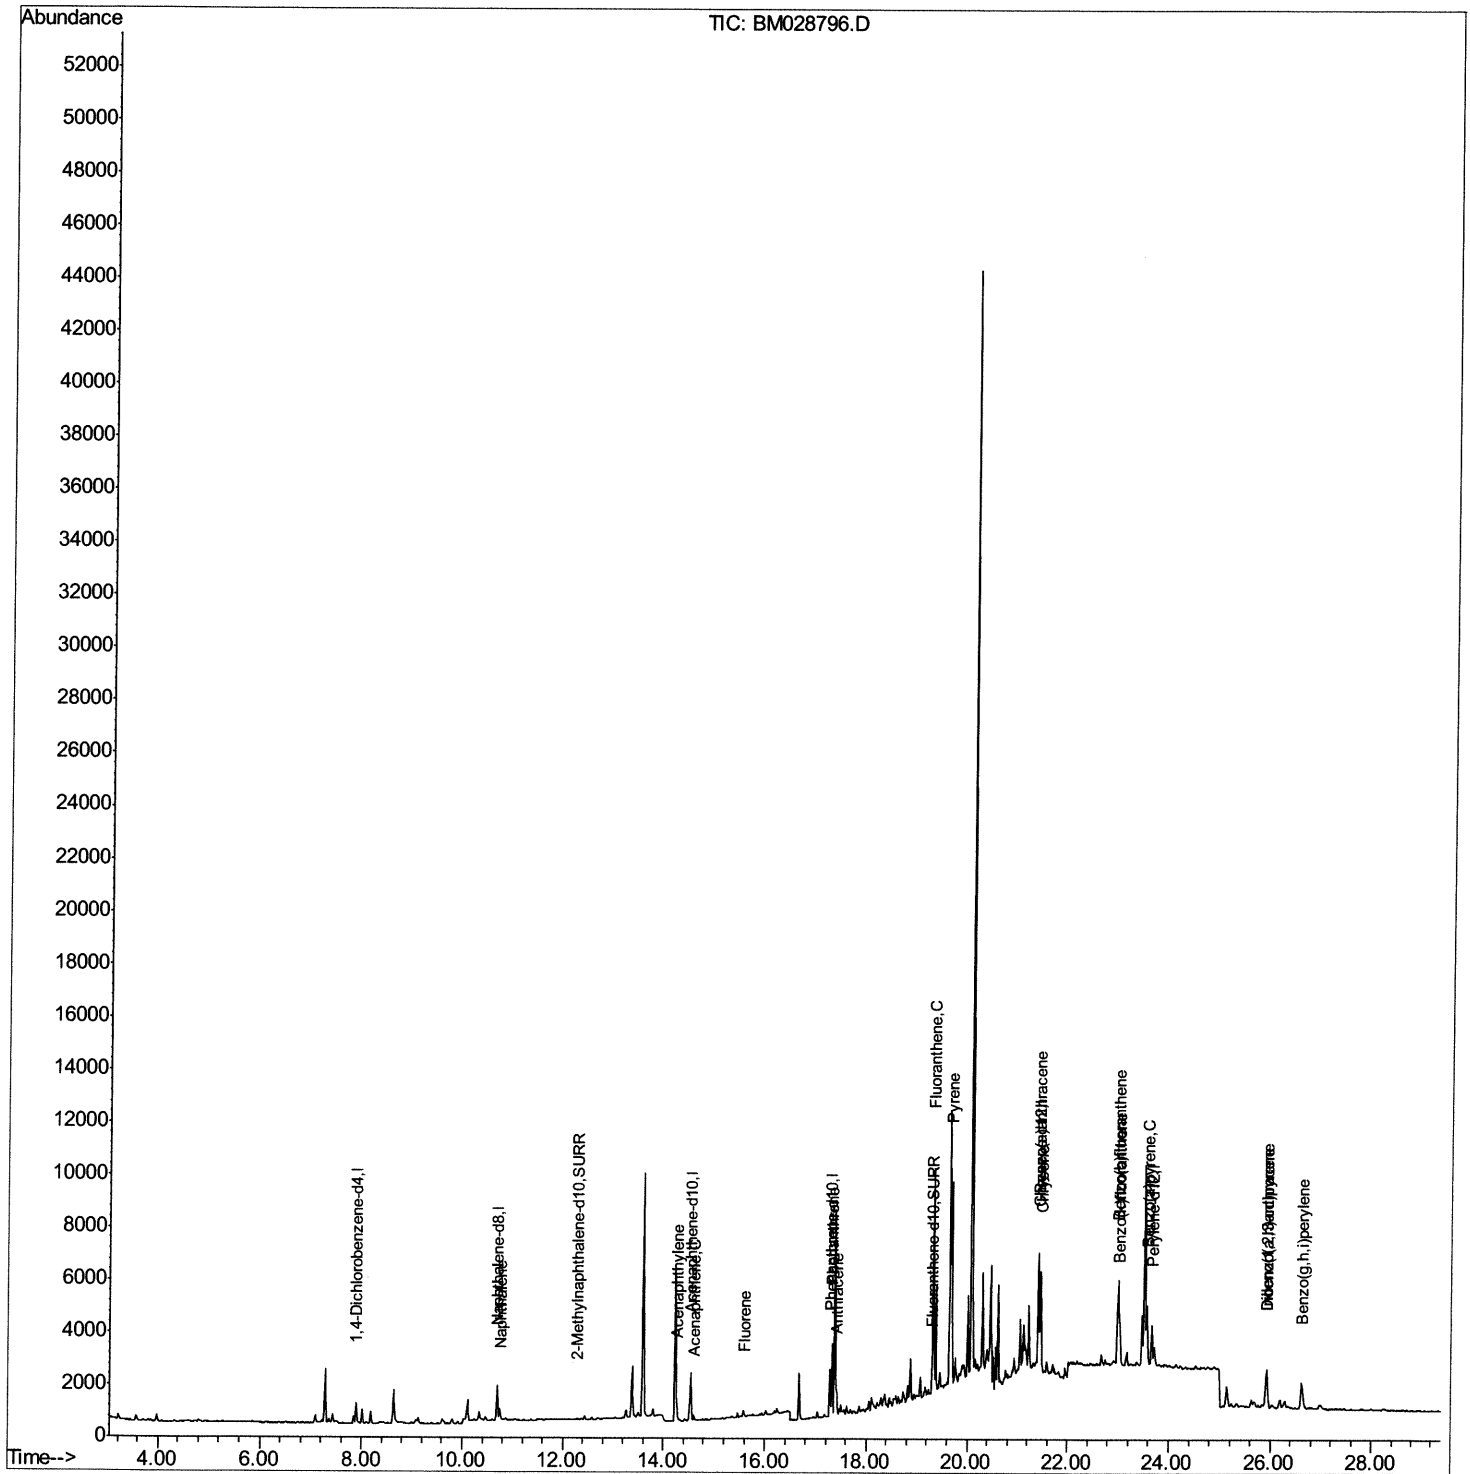




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028796.D
Acq On : 18 Feb 2021 14:50
Operator : CG/JU
Sample : M1379-11DL 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGZ1DL

Manual Integrations
APPROVED

mohammad
2/19/2021 1:19:45 PM

Quant Time: Feb 18 15:21:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 18 13:03:27 2021
Response via : Initial Calibration

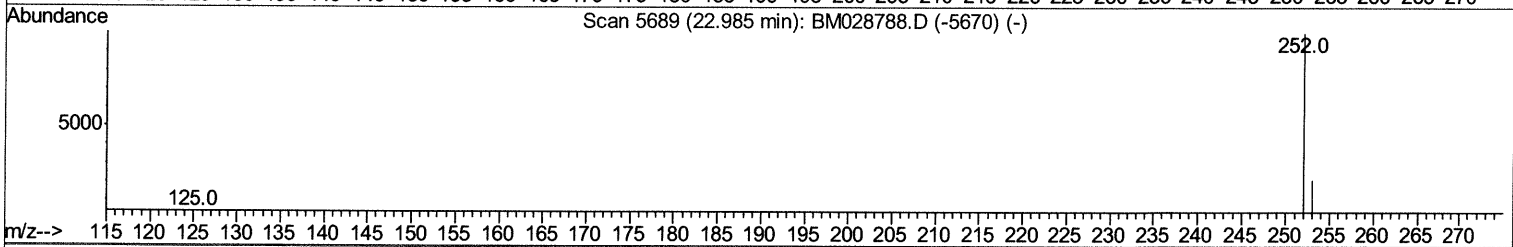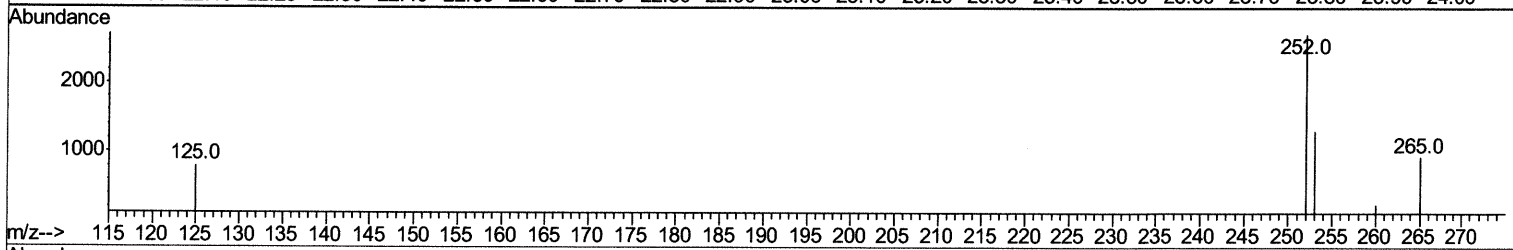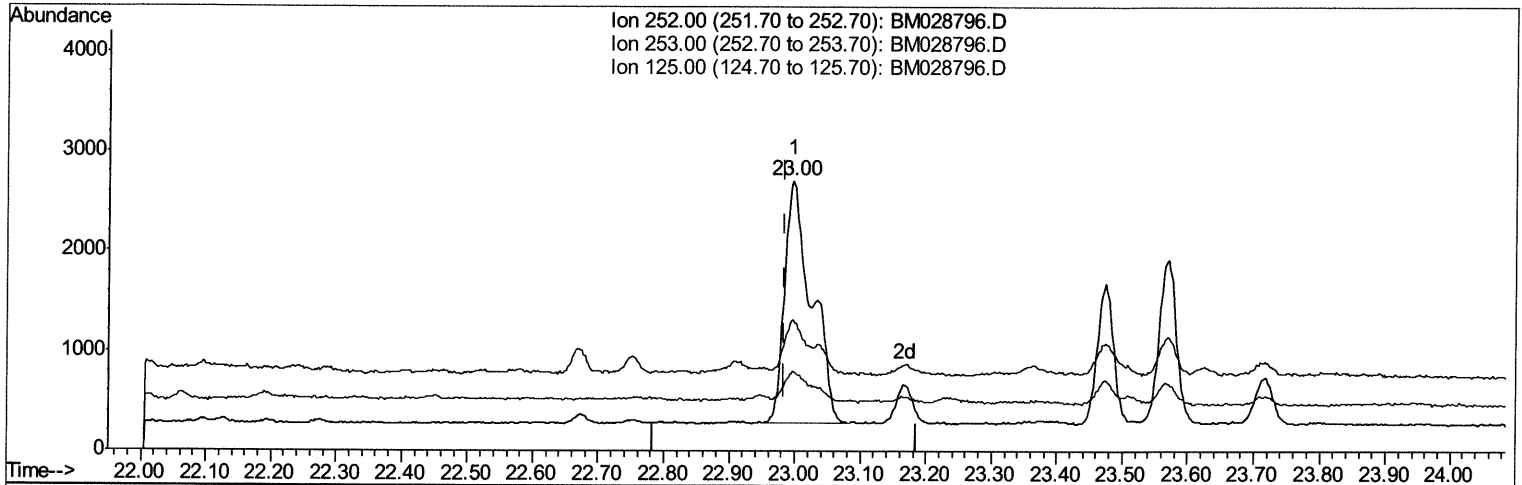

TIC: BM028796.D

(21) Benzo(b)fluoranthene

22.997min (+0.012) 1.09ng/ul

response 6963

Ion	Exp%	Act%
252.00	100	100
253.00	33.50	48.56
125.00	28.70	29.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028796.D
 Acq On : 18 Feb 2021 14:50
 Operator : CG/JU
 Sample : M1379-11DL 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGZ1DL

Manual Integrations
 APPROVED

mohammad
 2/19/2021 1:19:45 PM

Quant Time: Feb 18 15:21:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 18 13:03:27 2021
 Response via : Initial Calibration

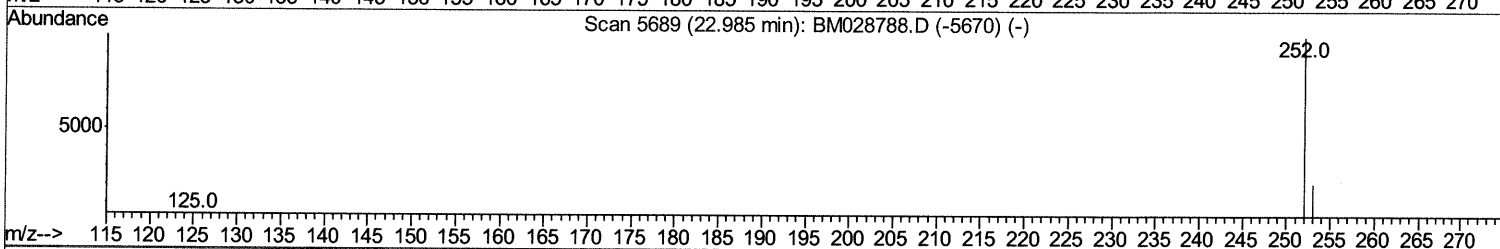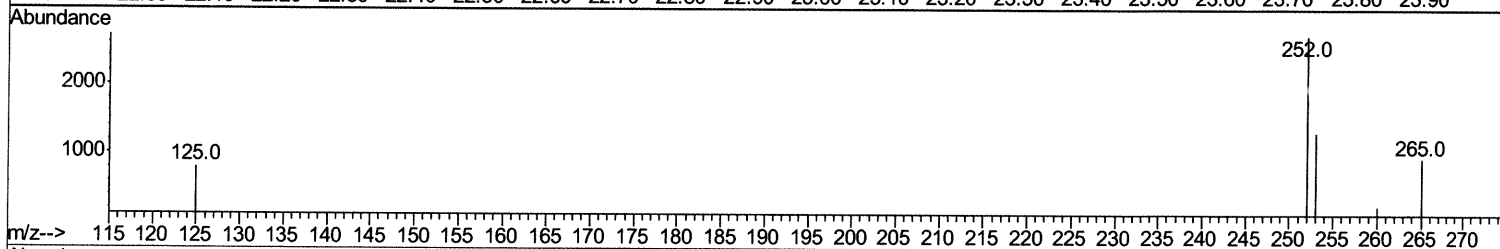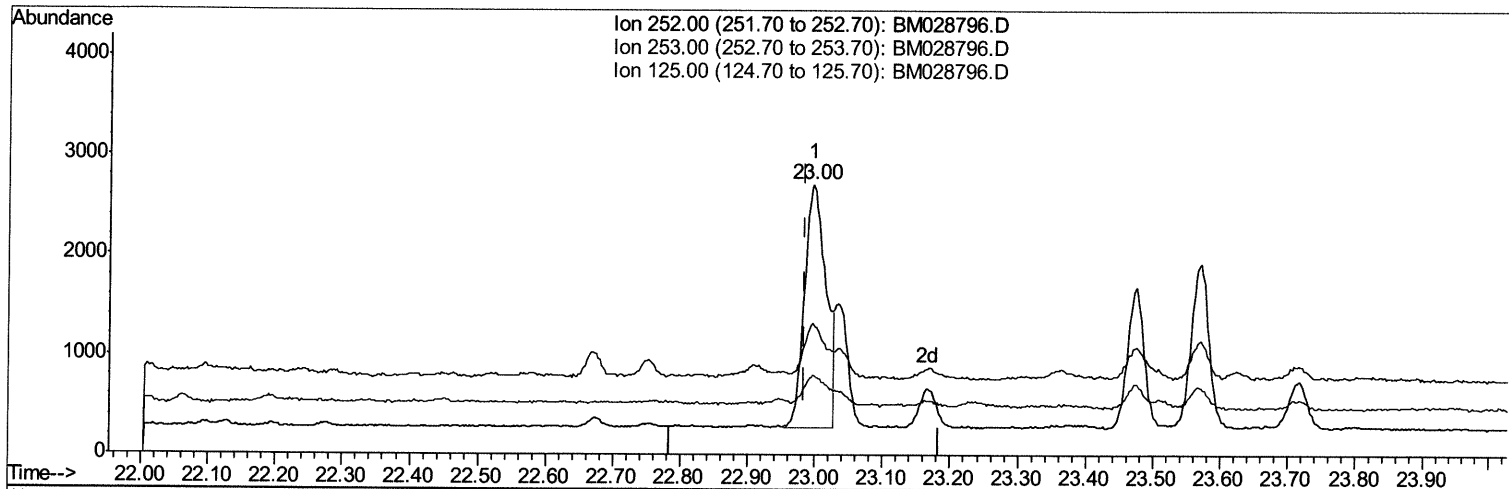

TIC: BM028796.D

(21) Benzo(b)fluoranthene

22.997min (+0.012) 0.82ng/ul m 02/22/21 JU

response 5284

Ion	Exp%	Act%
252.00	100	100
253.00	33.50	48.56
125.00	28.70	29.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028796.D
 Acq On : 18 Feb 2021 14:50
 Operator : CG/JU
 Sample : M1379-11DL 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGZ1DL

Manual Integrations
 APPROVED

mohammad
 2/19/2021 1:19:45 PM

Quant Time: Feb 18 15:21:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 18 13:03:27 2021
 Response via : Initial Calibration

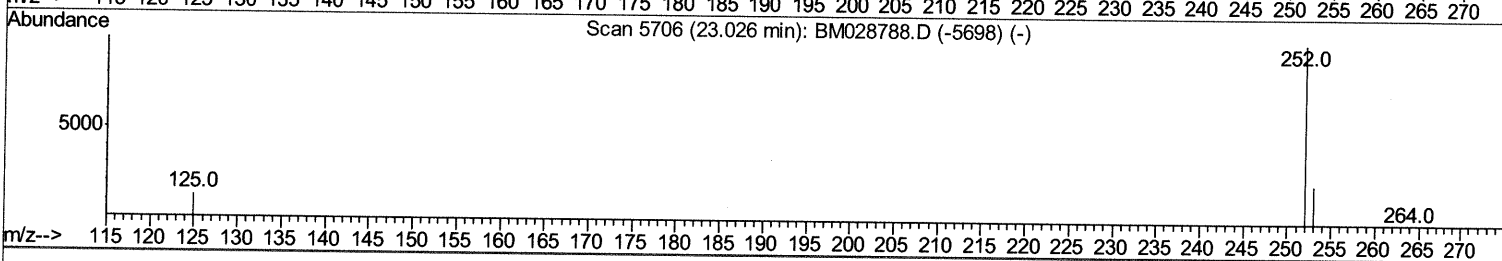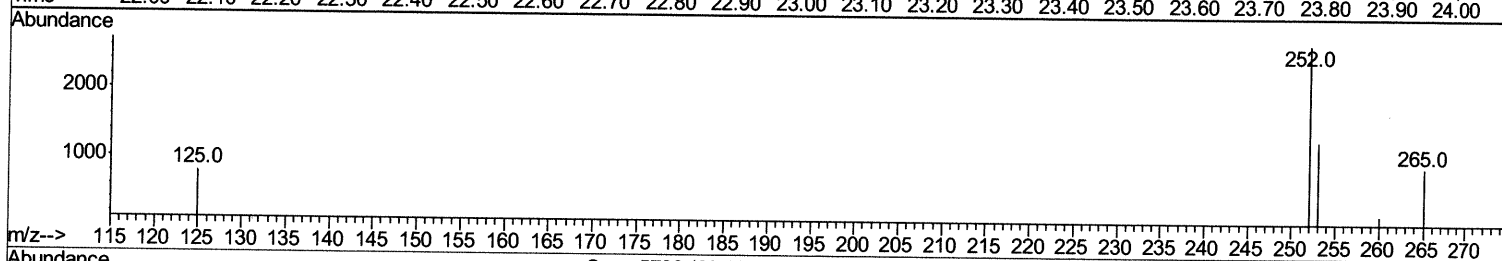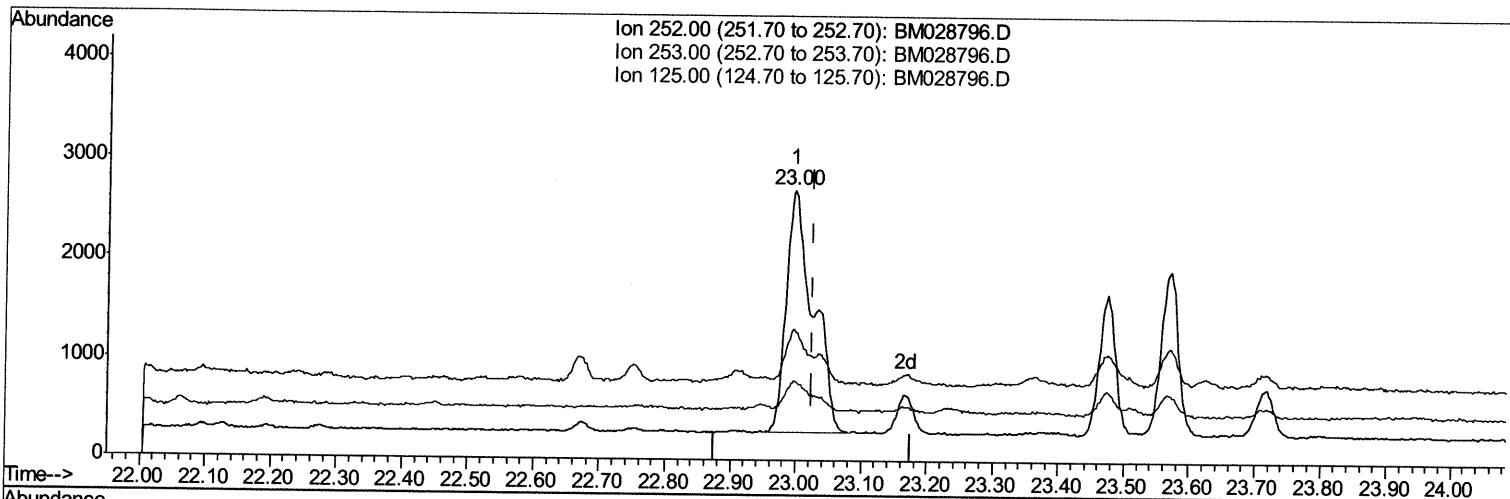

TIC: BM028796.D

(22) Benzo(k)fluoranthene
 22.997min (-0.029) 1.09ng/ul
 response 6963

Ion	Exp%	Act%
252.00	100	100
253.00	32.90	48.56#
125.00	28.60	29.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028796.D
 Acq On : 18 Feb 2021 14:50
 Operator : CG/JU
 Sample : M1379-11DL 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGZ1DL

Manual Integrations
 APPROVED

mohammad
 2/19/2021 1:19:45 PM

Quant Time: Feb 18 15:21:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 18 13:03:27 2021
 Response via : Initial Calibration

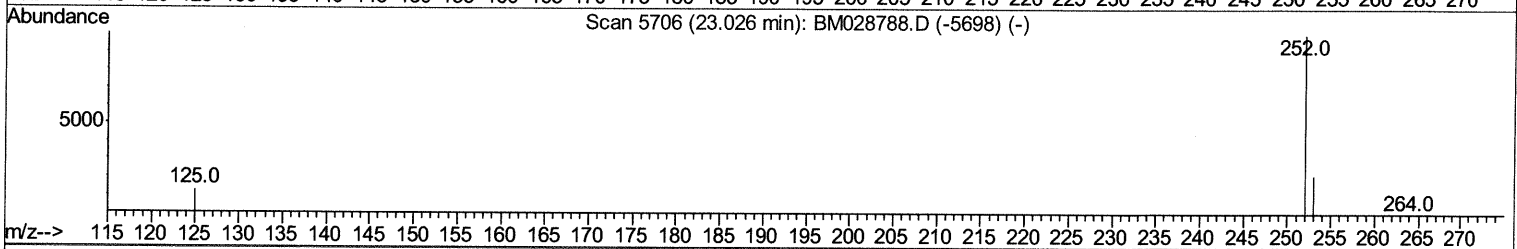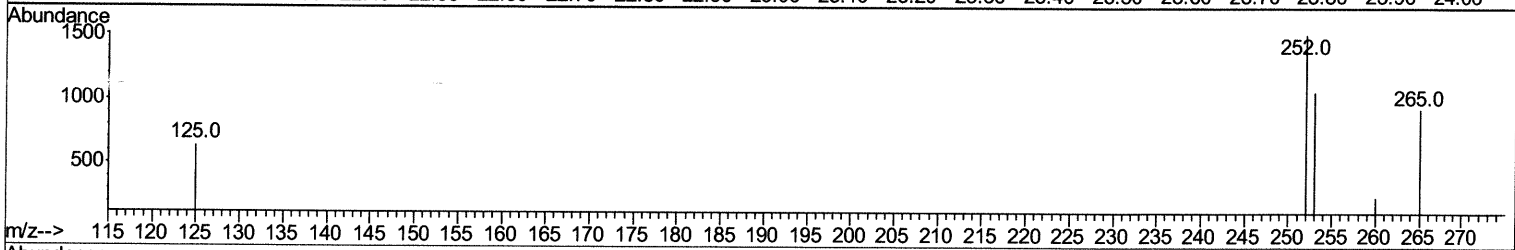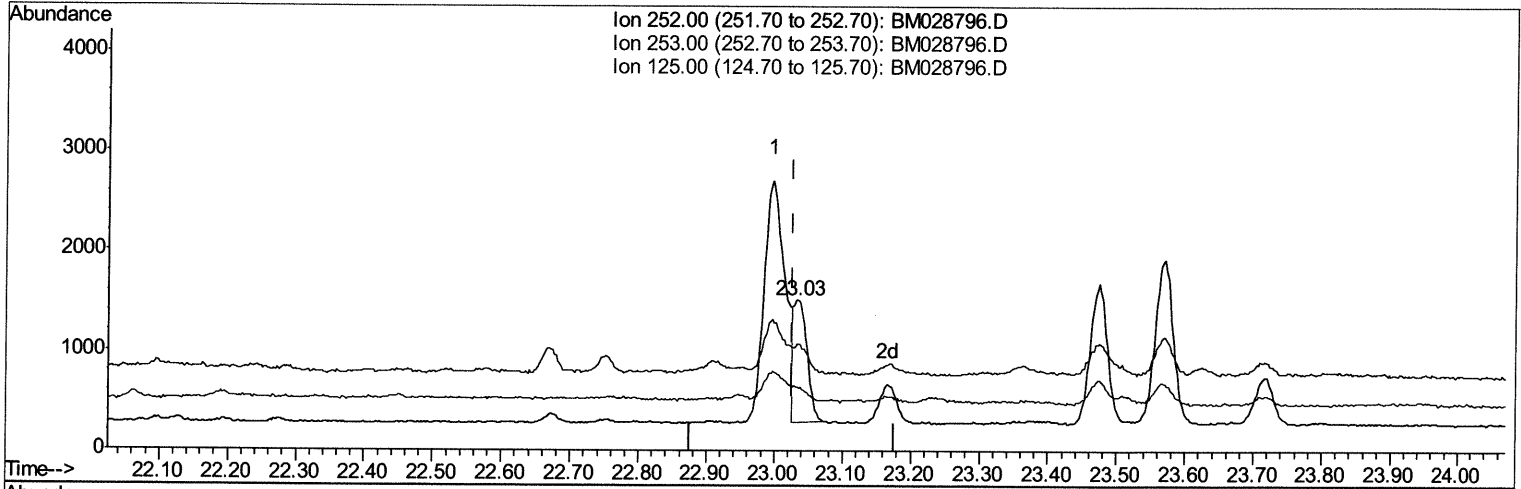

TIC: BM028796.D

(22) Benzo(k)fluoranthene

23.033min (+0.007) 0.26ng/ul m 02/22/21 JU

response 1645

Ion	Exp%	Act%
252.00	100	100
253.00	32.90	70.68#
125.00	28.60	42.29#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028796.D
 Acq On : 18 Feb 2021 14:50
 Operator : CG/JU
 Sample : M1379-11DL 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGZ1DL

Manual Integrations
 APPROVED

mohammad
 2/19/2021 1:19:45 PM

Quant Time: Feb 18 15:22:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 18 13:03:27 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	453	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	1831	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	1040	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.28	188	1978	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	2051	0.40	ng/ul	0.01
20) Perylene-d12	23.67	264	1874	0.40	ng/ul	0.01

Svstem Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	58	0.02	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	135	0.03	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.75	128	142	0.031	ng/ul#	21
7) Acenaphthylene	14.27	152	371	0.087	ng/ul#	65
8) Acenaphthene	14.61	153	121	0.036	ng/ul#	89
9) Fluorene	15.59	166	140	0.037	ng/ul#	61
12) Phenanthrene	17.32	178	2898	0.524	ng/ul	98
13) Anthracene	17.41	178	732	0.139	ng/ul#	70
15) Fluoranthene	19.33	202	7031	1.117	ng/ul	96
17) Pyrene	19.69	202	6192	0.831	ng/ul	98
18) Benzo(a)anthracene	21.42	228	3601	0.514	ng/ul#	88
19) Chrysene	21.47	228	3766	0.541	ng/ul#	84
21) Benzo(b)fluoranthene	23.00	252	5284m	0.824	ng/ul	02/22/21 JU
22) Benzo(k)fluoranthene	23.03	252	1645m	0.257	ng/ul	
23) Benzo(a)pyrene	23.57	252	3008	0.527	ng/ul#	80
24) Indeno(1,2,3-cd)pyrene	25.93	276	2218	0.298	ng/ul#	100
25) Dibenzo(a,h)anthracene	25.93	278	611	0.098	ng/ul#	1
26) Benzo(a,h,i)perylene	26.62	276	1973	0.319	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed