


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\  
Data File : BM028797.D  
Acq On : 18 Feb 2021 15:27  
Operator : CG/JU  
Sample : PB134703BL  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK03

Manual Integrations  
APPROVED

mohammad  
2/19/2021 1:19:48 PM

Quant Time: Feb 18 16:02:13 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 18 13:03:27 2021  
Response via : Initial Calibration

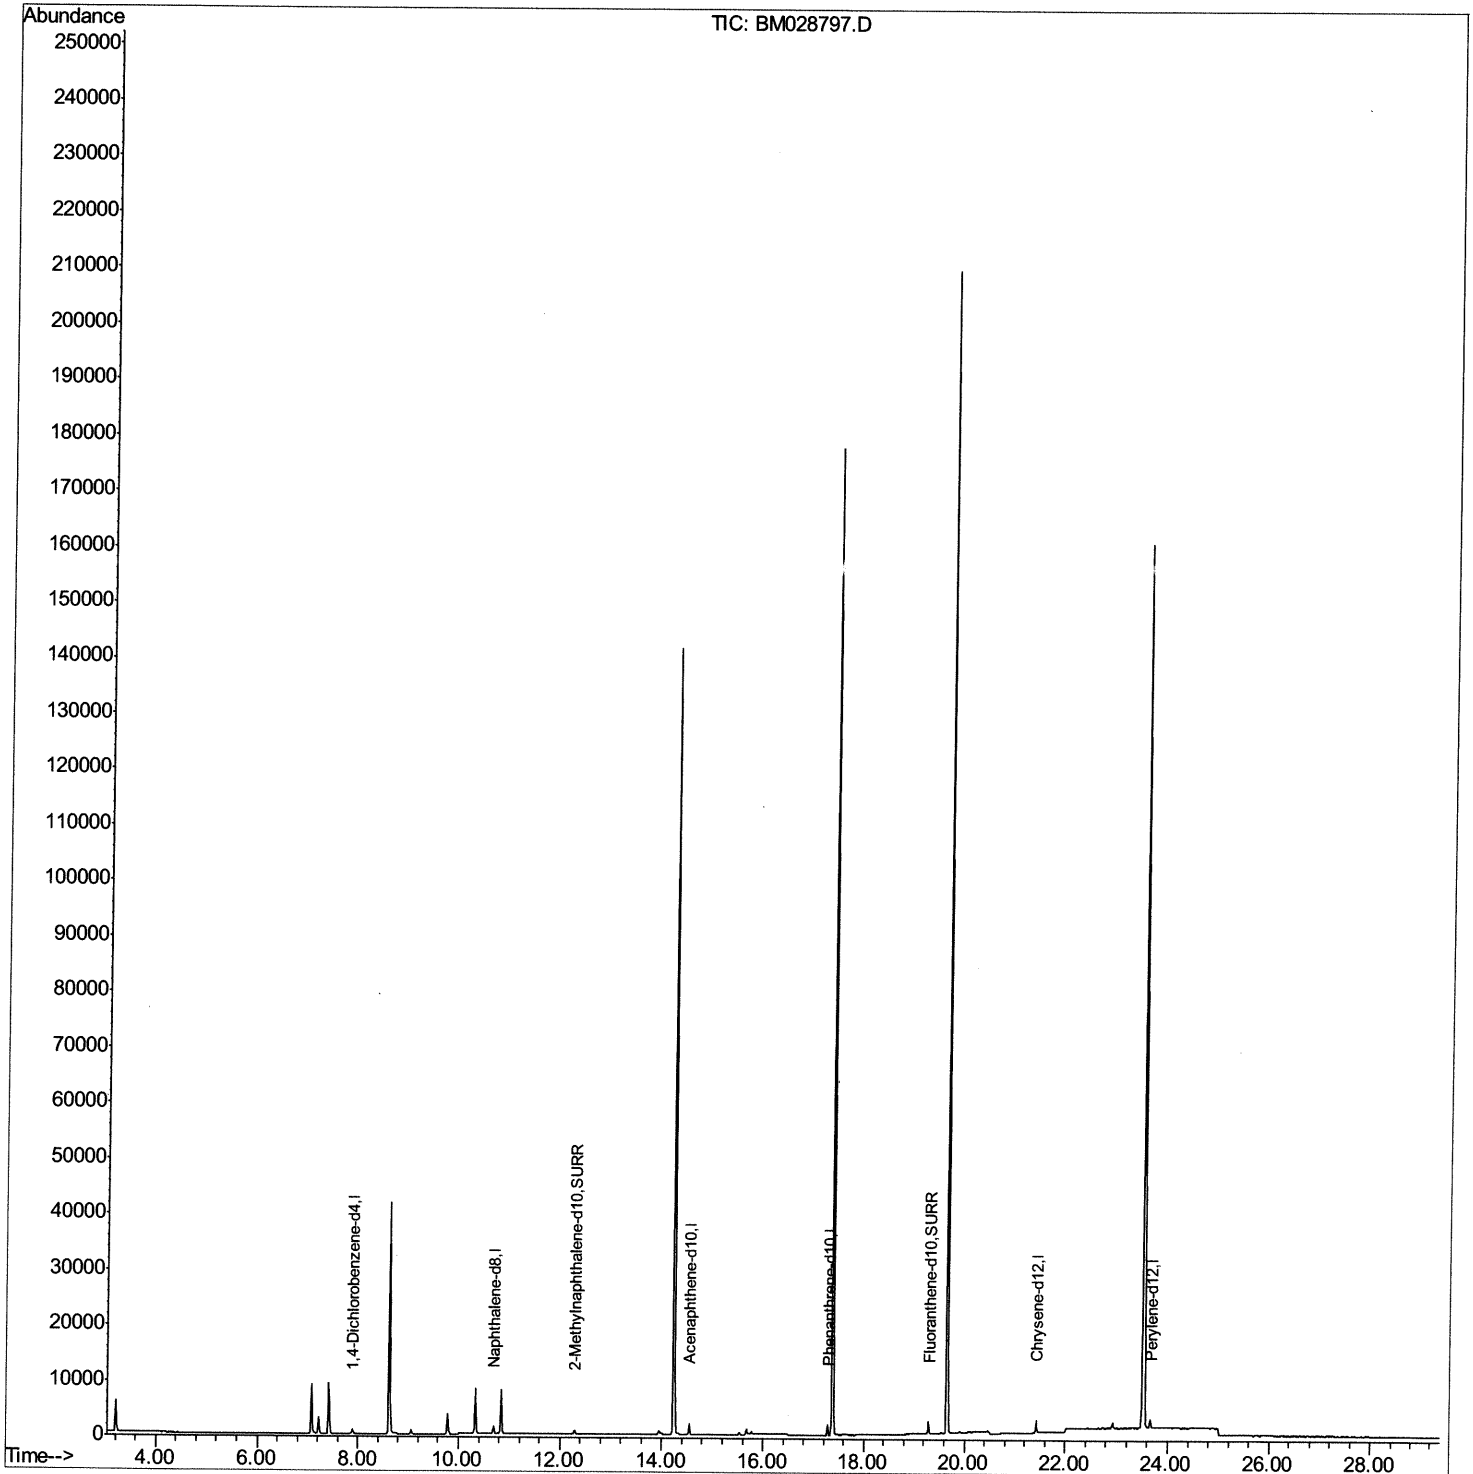

# Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\  
 Data File : BM028797.D  
 Acq On : 18 Feb 2021 15:27  
 Operator : CG/JU  
 Sample : PB134703BL  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
 BNA\_M  
**ClientSampleId :**  
 SBLK03

**Manual Integrations**  
**APPROVED**

mohammad  
 2/19/2021 1:19:48 PM

Quant Time: Feb 18 15:59:11 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Feb 18 13:03:27 2021  
 Response via : Initial Calibration

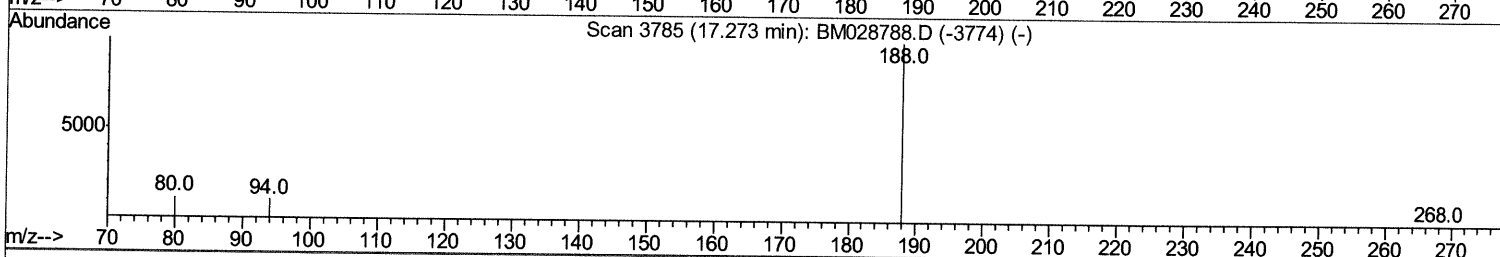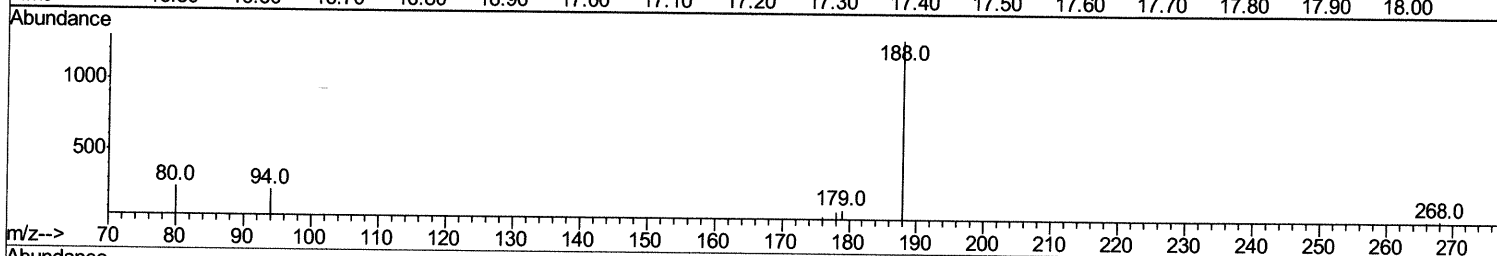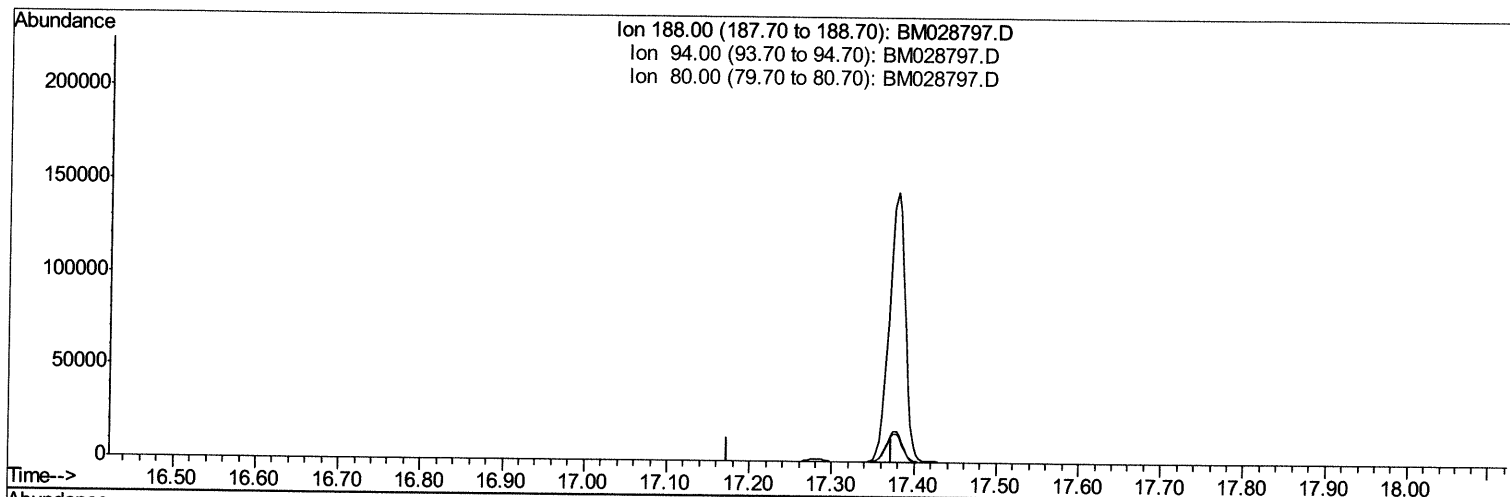

TIC: BM028797.D

(10) Phenanthrene-d10 (I)

17.273min (-17.273) 0.00ng/ul

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 188.00 | 100   | 0.00  |
| 94.00  | 13.50 | 0.00# |
| 80.00  | 14.00 | 0.00# |
| 0.00   | 0.00  | 0.00  |

# Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\  
 Data File : BM028797.D  
 Acq On : 18 Feb 2021 15:27  
 Operator : CG/JU  
 Sample : PB134703BL  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
 BNA\_M  
**ClientSampleId :**  
 SBLK03

**Manual Integrations**  
**APPROVED**

mohammad  
 2/19/2021 1:19:48 PM

Quant Time: Feb 18 15:59:11 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Feb 18 13:03:27 2021  
 Response via : Initial Calibration

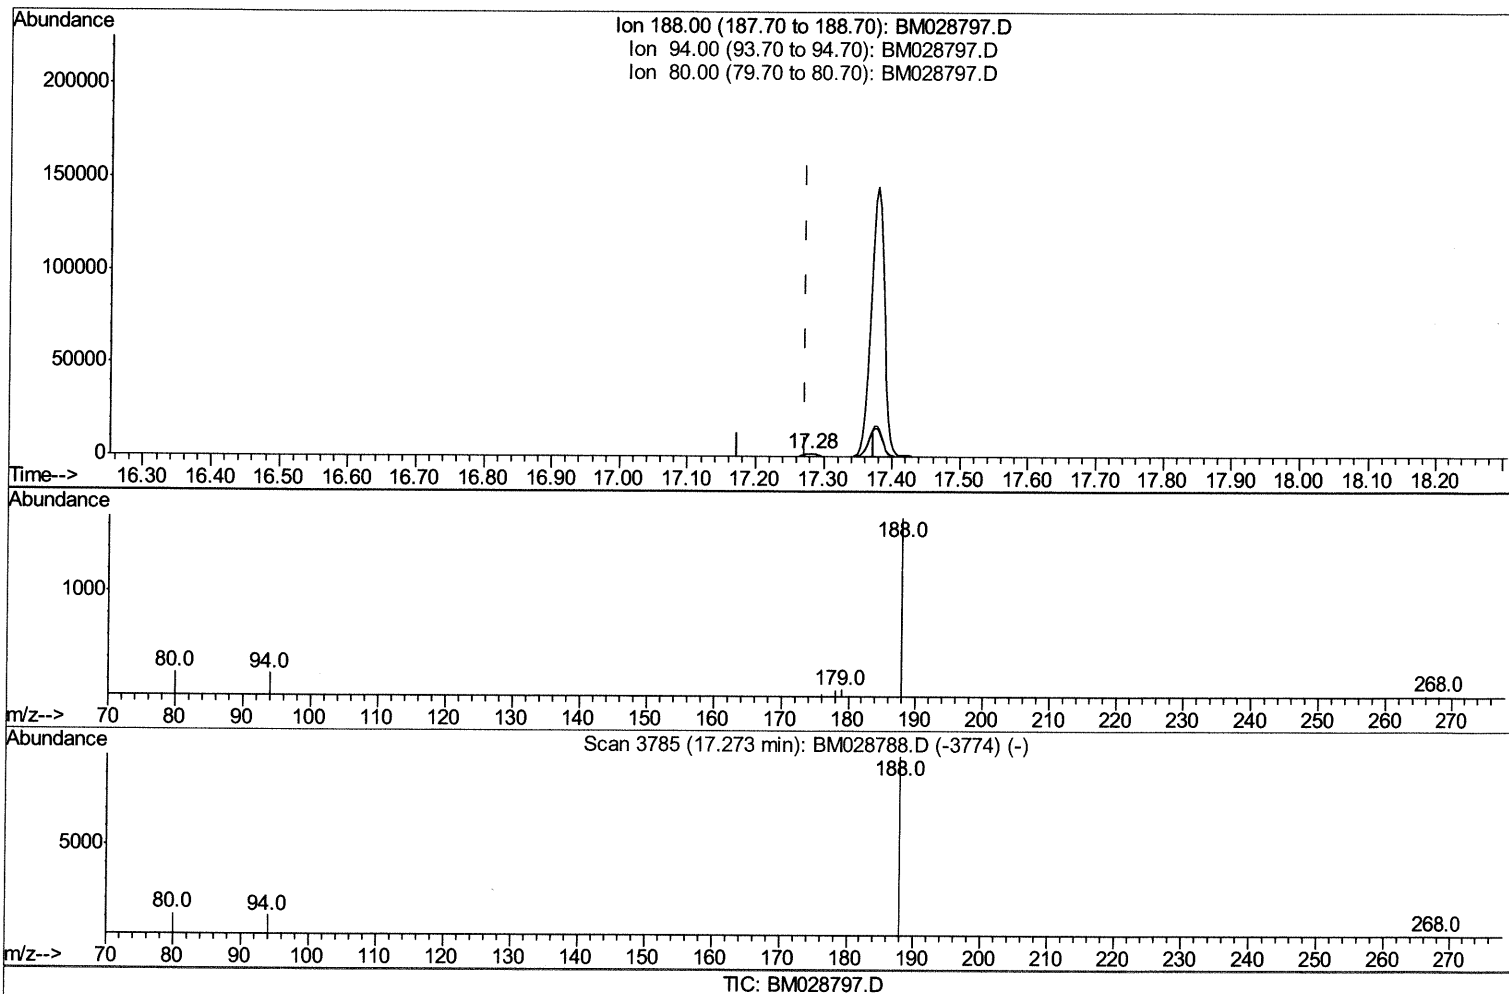

(10) Phenanthrene-d10 (I)

17.280min (+0.007) 0.40ng/ul m 02/22/21 JU

response 2396

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 188.00 | 100   | 100   |
| 94.00  | 13.50 | 14.67 |
| 80.00  | 14.00 | 15.32 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\  
 Data File : BM028797.D  
 Acq On : 18 Feb 2021 15:27  
 Operator : CG/JU  
 Sample : PB134703BL  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SBLK03

Manual Integrations  
 APPROVED

mohammad  
 2/19/2021 1:19:48 PM

Quant Time: Feb 18 16:02:13 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Feb 18 13:03:27 2021  
 Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc | Units  | Dev(Min) |
|-----------------------------|-------|------|----------|------|--------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 7.89  | 152  | 458      | 0.40 | ng/ul  | 0.00     |
| 2) Naphthalene-d8           | 10.70 | 136  | 1921     | 0.40 | ng/ul  | 0.00     |
| 6) Acenaphthene-d10         | 14.54 | 164  | 1138     | 0.40 | ng/ul  | 0.00     |
| 10) Phenanthrene-d10        | 17.28 | 188  | 2396m>   | 0.40 | ng/ul> | 0.00     |
| 16) Chrysene-d12            | 21.43 | 240  | 2054     | 0.40 | ng/ul  | 0.00     |
| 20) Perylene-d12            | 23.66 | 264  | 2022     | 0.40 | ng/ul  | 0.00     |
| System Monitoring Compounds |       |      |          |      |        |          |
| 4) 2-Methylnaphthalene-d10  | 12.29 | 152  | 1124     | 0.41 | ng/ul  | 0.00     |
| 14) Fluoranthene-d10        | 19.29 | 212  | 2331     | 0.38 | ng/ul  | 0.00     |

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed