


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028808.D
Acq On : 18 Feb 2021 22:42
Operator : CG/JU
Sample : M1429-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGQ7

Manual Integrations
APPROVED

mohammad
2/19/2021 1:20:17 PM

Quant Time: Feb 19 01:02:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 18 11:30:02 2021
Response via : Initial Calibration

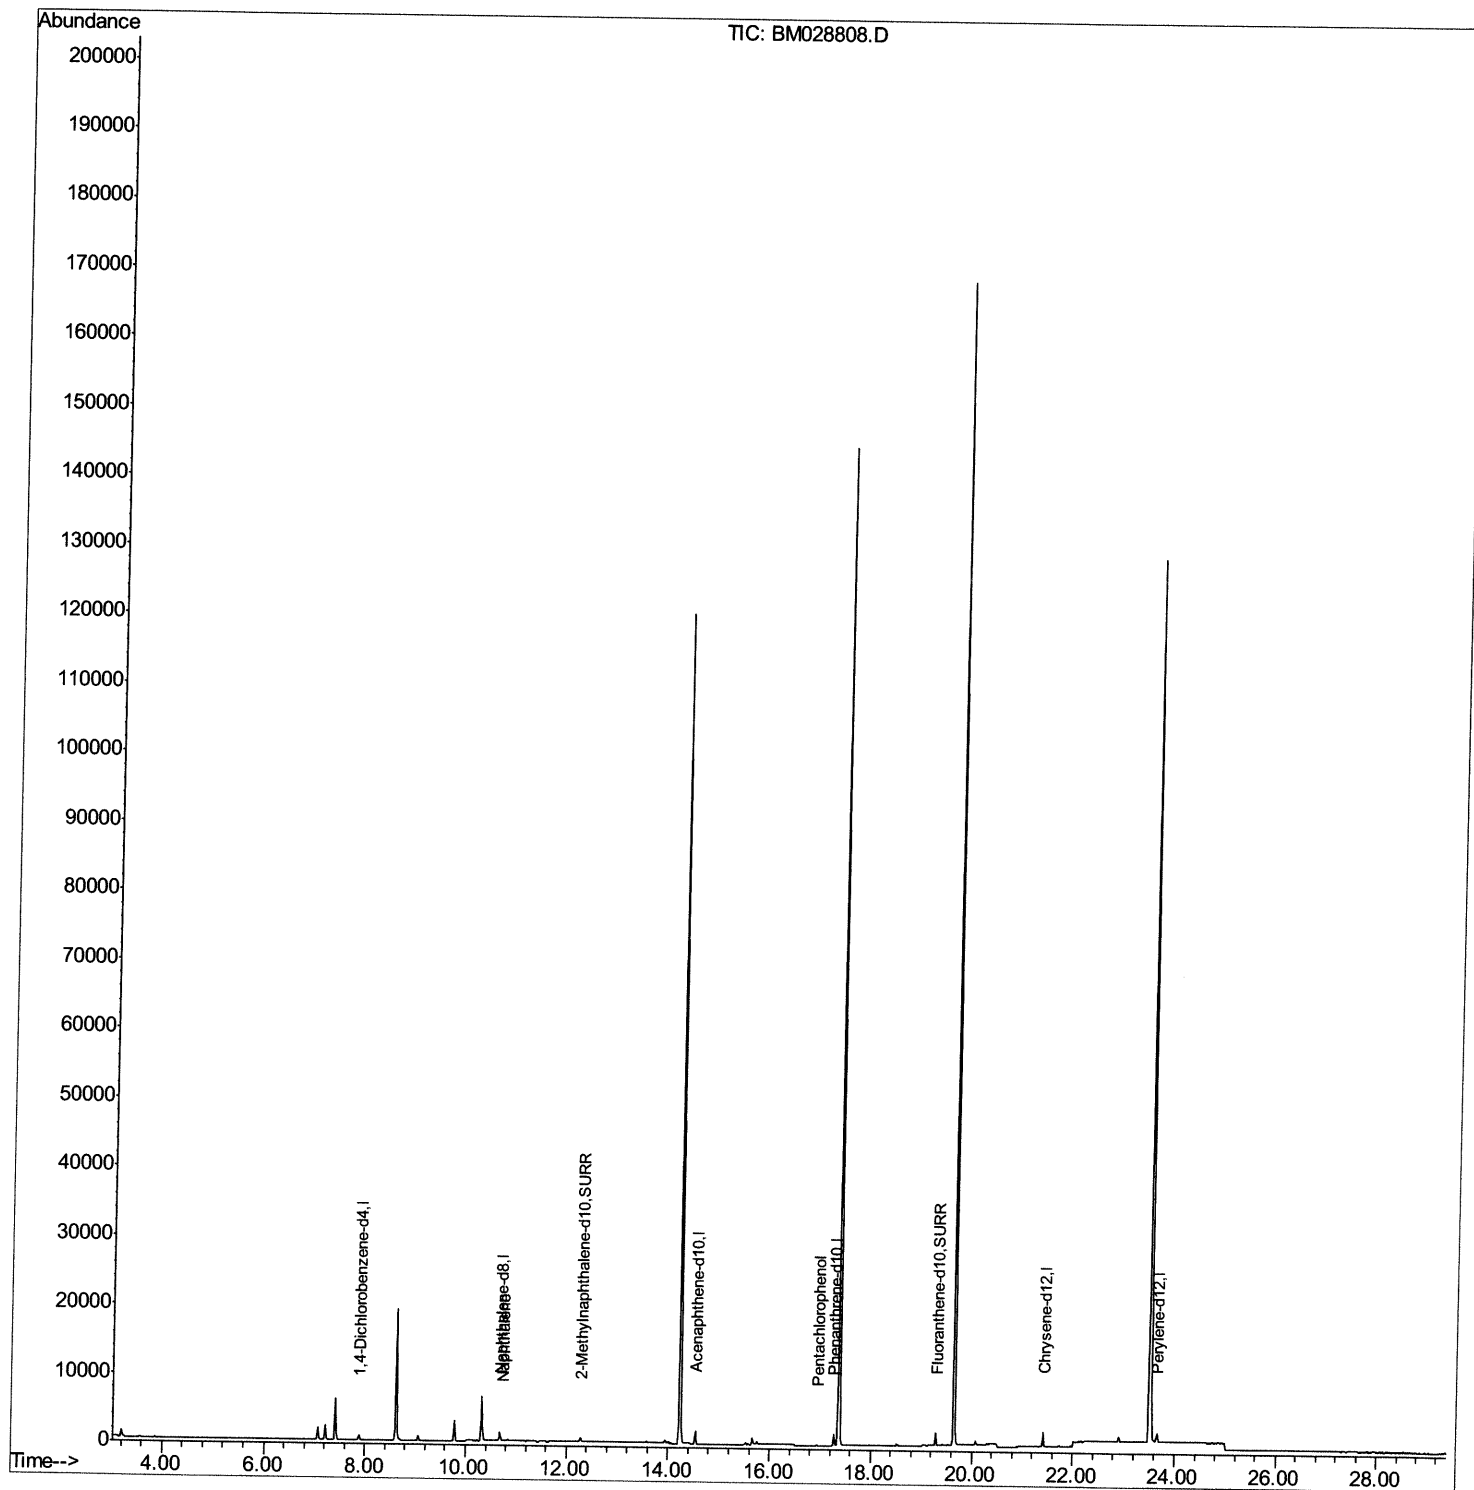

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028808.D
Acq On : 18 Feb 2021 22:42
Operator : CG/JU
Sample : M1429-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGQ7

Manual Integrations
APPROVED

mohammad
2/19/2021 1:20:17 PM

Quant Time: Feb 18 23:36:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 18 11:30:02 2021
Response via : Initial Calibration

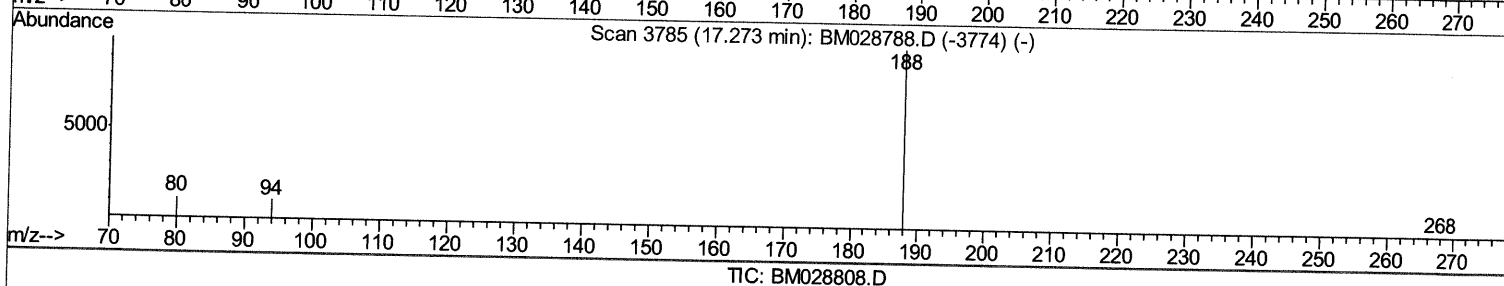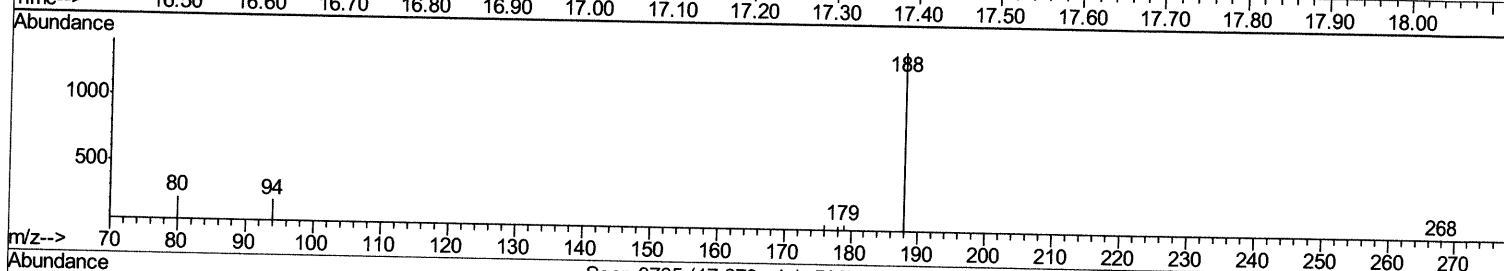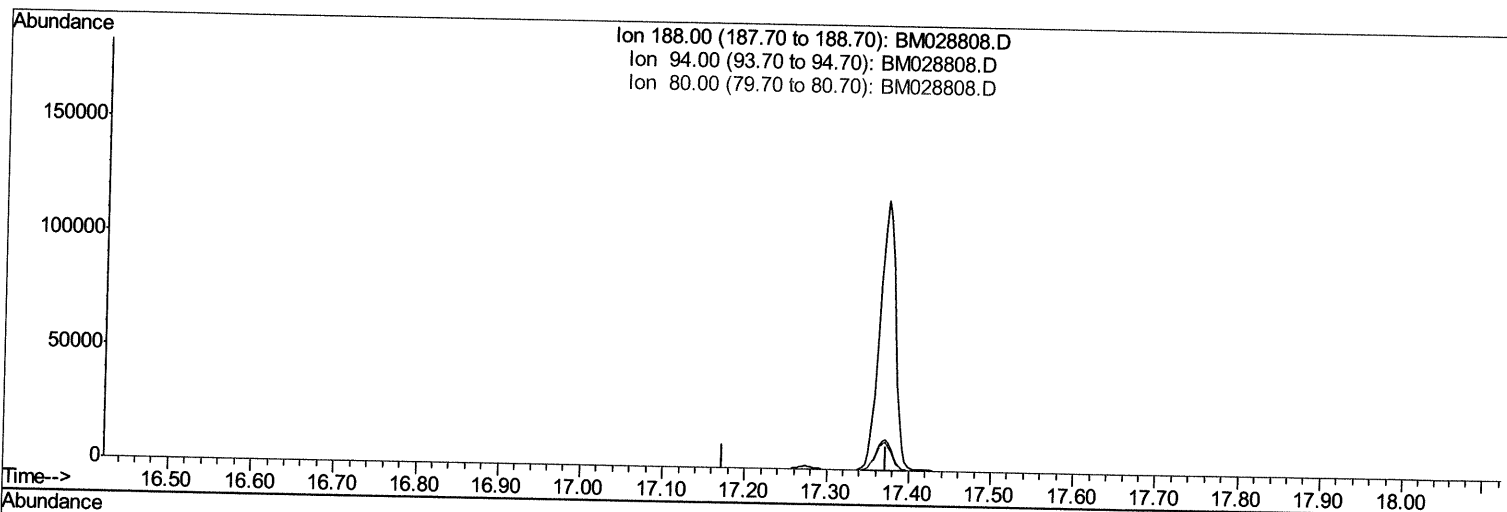

(10) Phenanthrene-d10 (I)

17.273min (-17.273) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	13.50	0.00#
80.00	14.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028808.D
 Acq On : 18 Feb 2021 22:42
 Operator : CG/JU
 Sample : M1429-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGQ7

Manual Integrations
 APPROVED

mohammad
 2/19/2021 1:20:17 PM

Quant Time: Feb 18 23:36:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 18 11:30:02 2021
 Response via : Initial Calibration

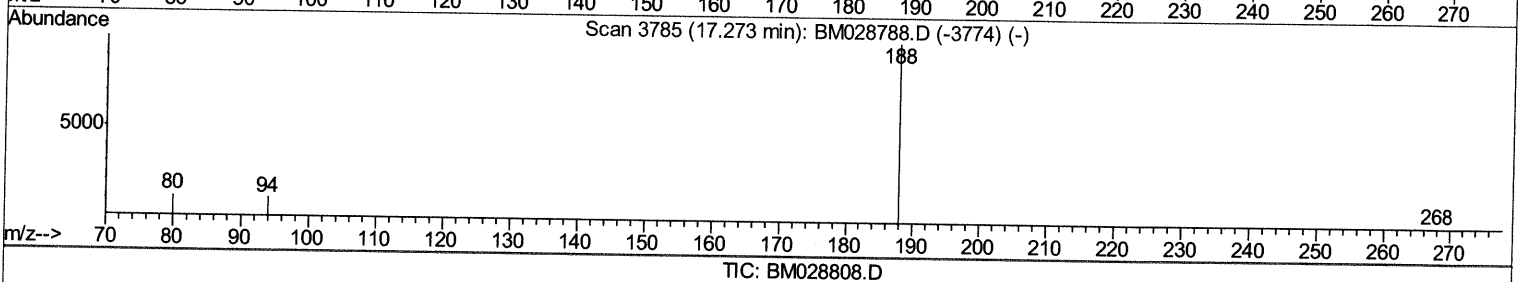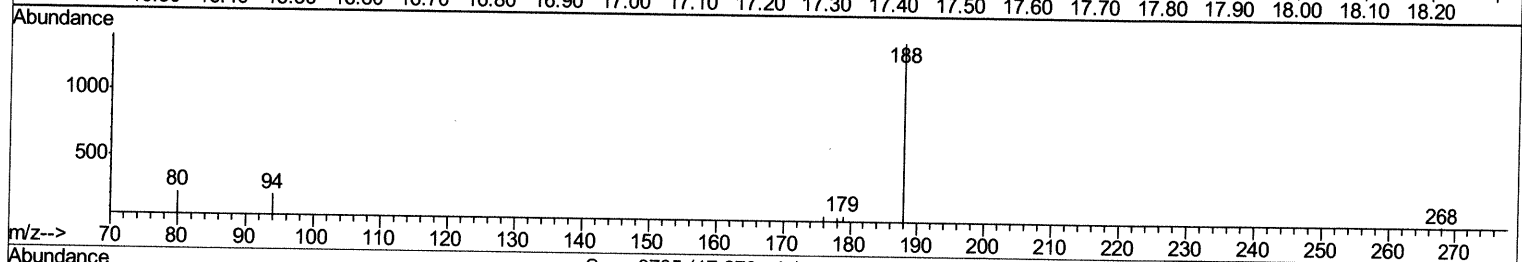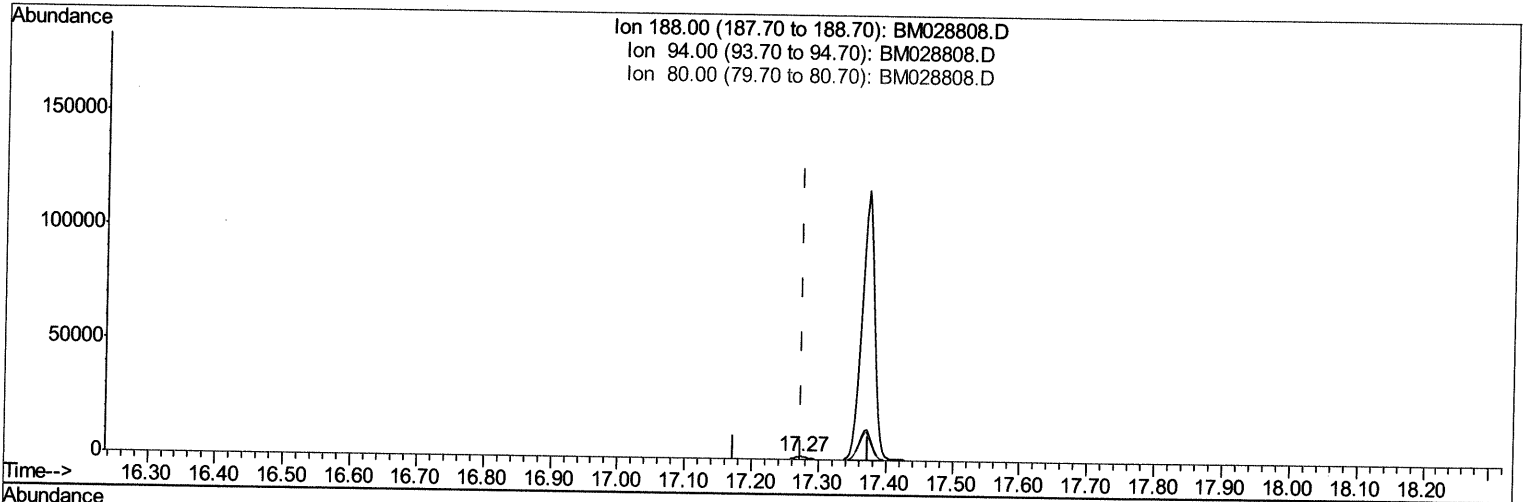

TIC: BM028808.D

(10) Phenanthrene-d10 (I)

17.273min (-0.000) 0.40ng/ul m 02/22/21 JU

response 1904

Ion	Exp%	Act%
188.00	100	100
94.00	13.50	14.48
80.00	14.00	15.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028808.D
 Acq On : 18 Feb 2021 22:42
 Operator : CG/JU
 Sample : M1429-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGQ7

Manual Integrations
 APPROVED

mohammad
 2/19/2021 1:20:17 PM

Quant Time: Feb 19 01:02:06 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 18 11:30:02 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	420	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	1745	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	1019	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.27	188	1904m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.42	240	1780	0.40	ng/ul	0.00
20) Perylene-d12	23.65	264	1820	0.40	ng/ul	0.00

02/22/21 JU

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	909	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	1886	0.38	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.74	128	89	0.020	ng/ul#	5
11) Pentachlorophenol	16.94	266	18	0.036	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed