


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028817.D
Acq On : 19 Feb 2021 13:22
Operator : CG/JU
Sample : PB134691BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Manual Integrations
APPROVED

mohammad
2/22/2021 2:07:44 PM

Quant Time: Feb 19 13:54:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 10:10:00 2021
Response via : Initial Calibration

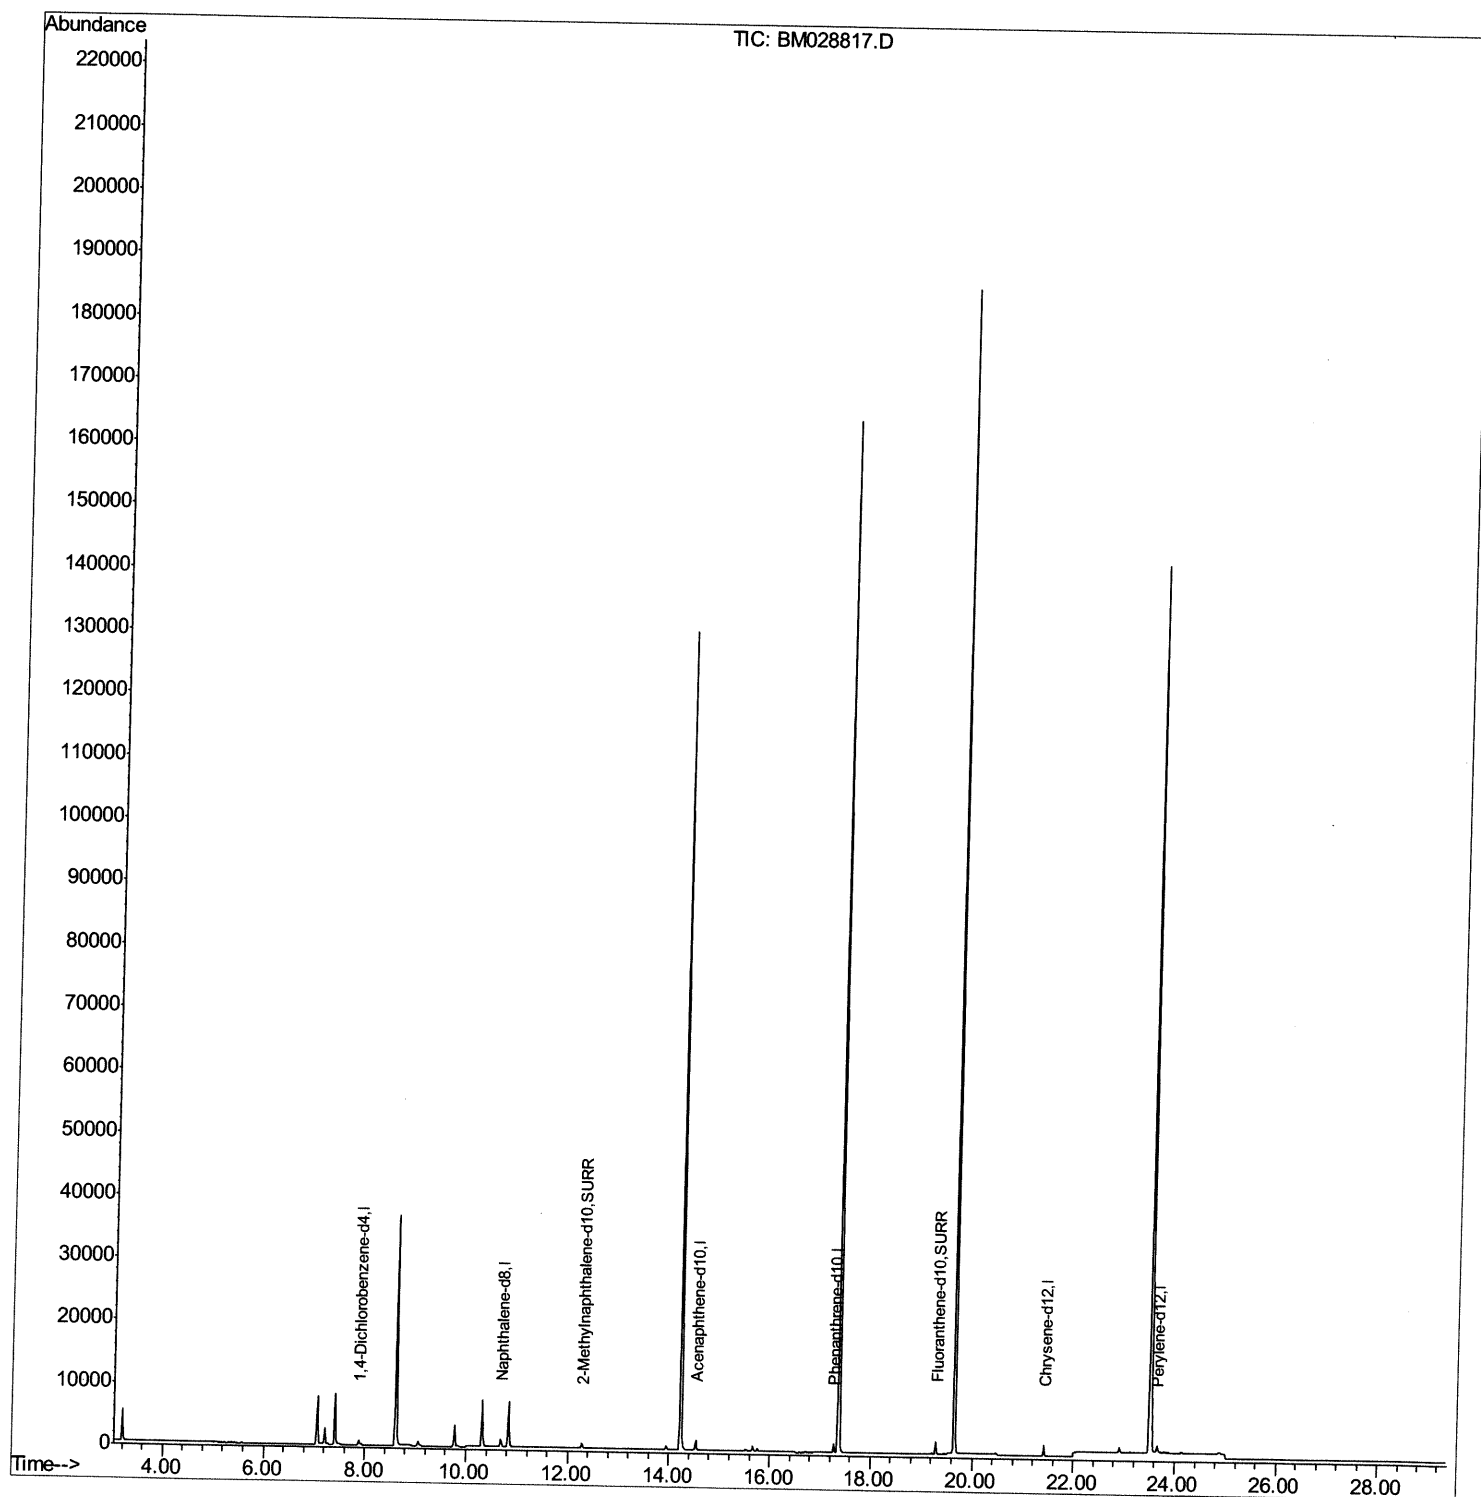

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028817.D
 Acq On : 19 Feb 2021 13:22
 Operator : CG/JU
 Sample : PB134691BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK91

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:07:44 PM

Quant Time: Feb 19 13:53:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 10:10:00 2021
 Response via : Initial Calibration

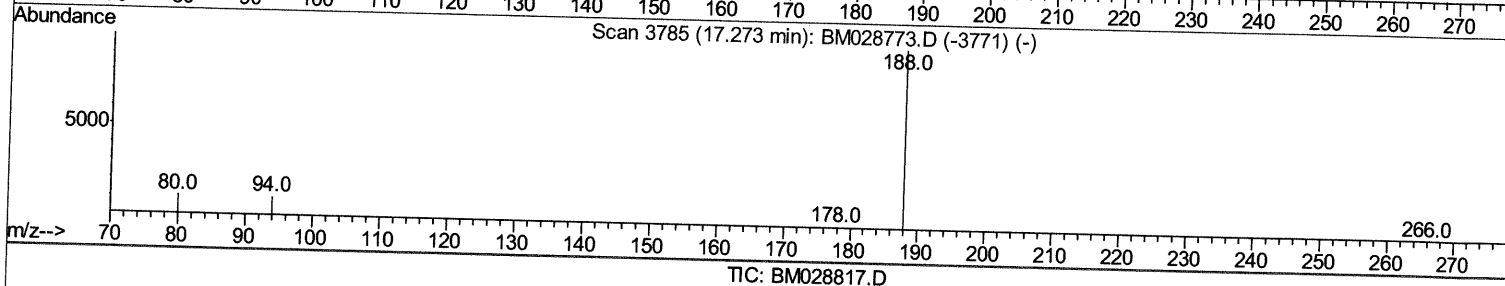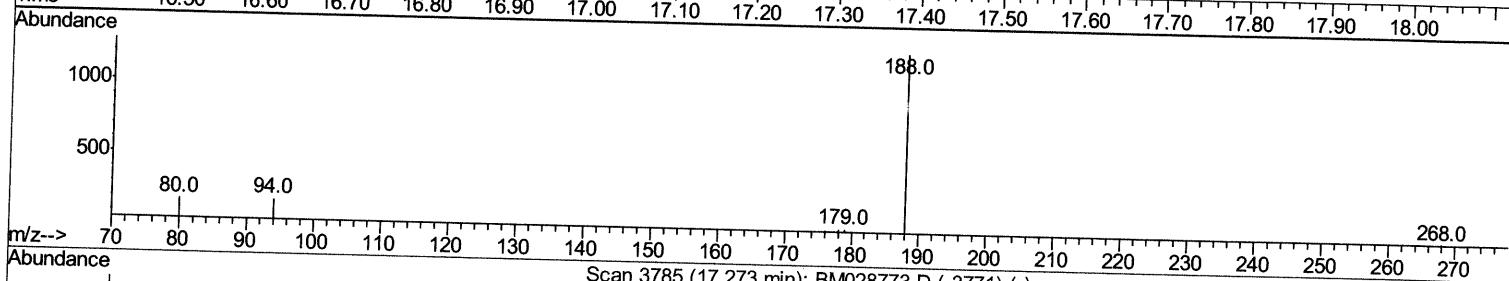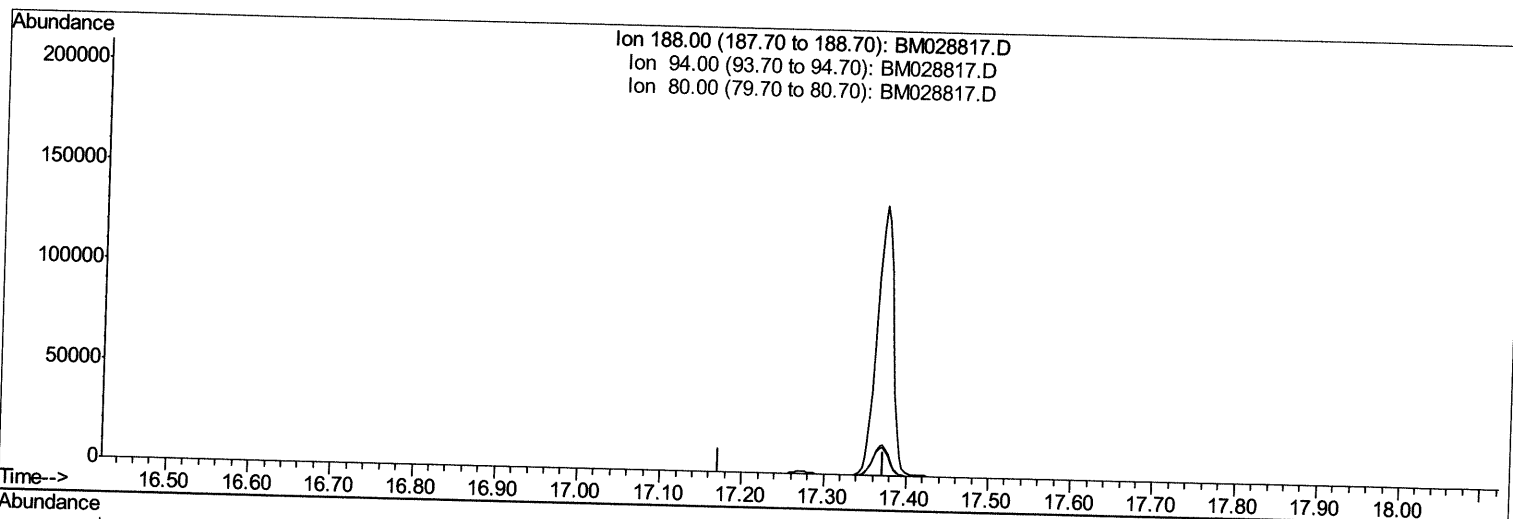

TIC: BM028817.D

(10) Phenanthrene-d10 (I)

17.272min (-17.272) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	13.50	0.00#
80.00	14.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028817.D
 Acq On : 19 Feb 2021 13:22
 Operator : CG/JU
 Sample : PB134691BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK91

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:07:44 PM

Quant Time: Feb 19 13:53:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 10:10:00 2021
 Response via : Initial Calibration

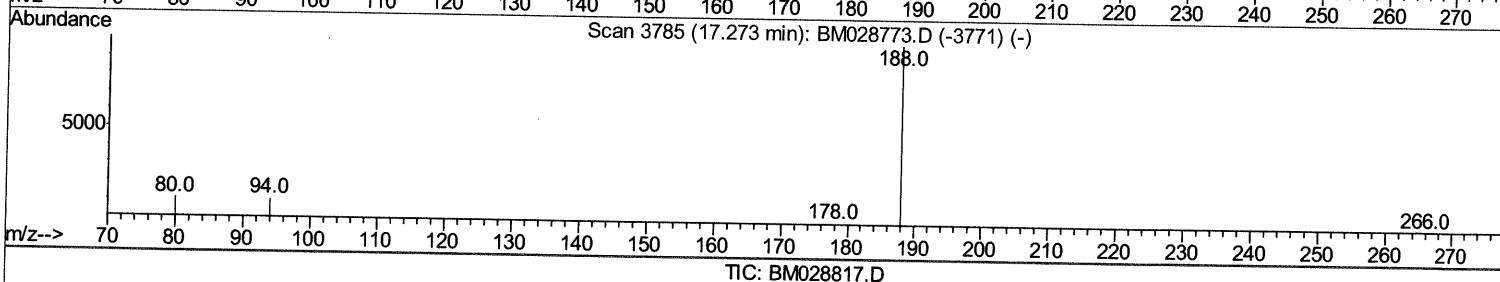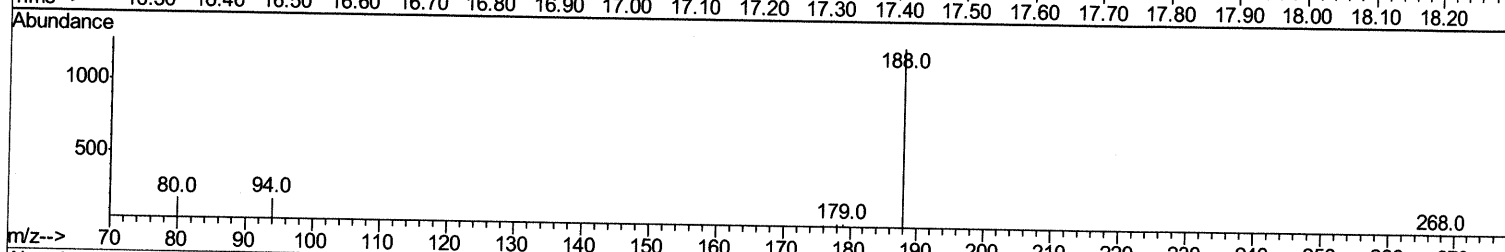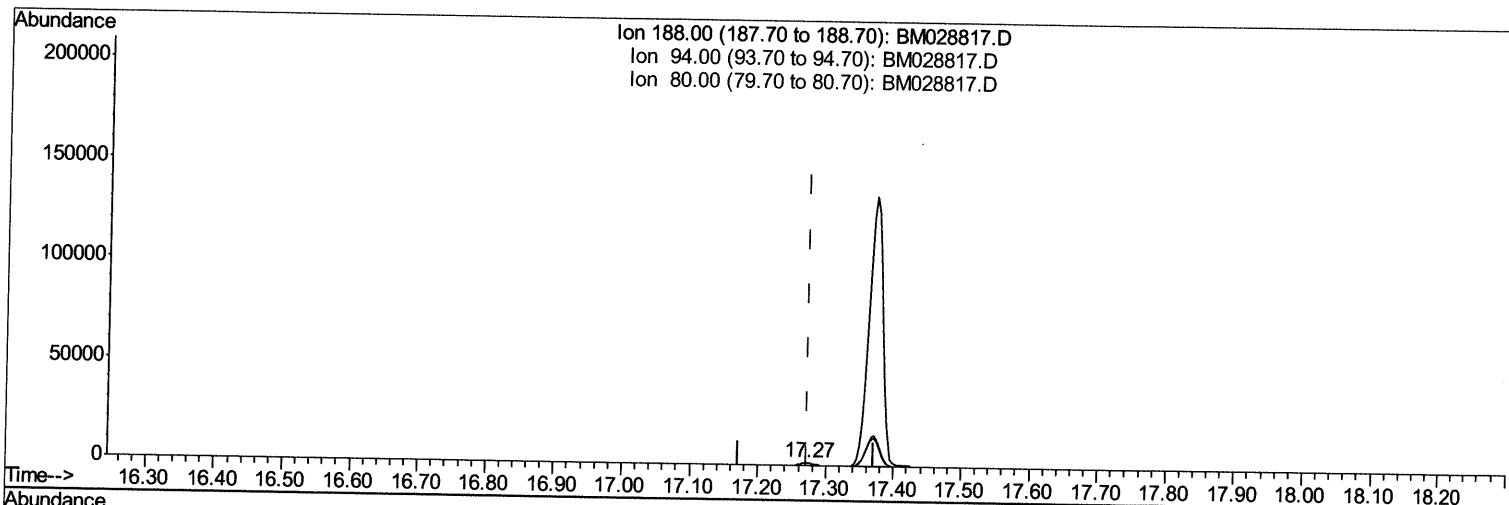

(10) Phenanthrene-d10 (I)

17.273min (+0.001) 0.40ng/ul m 02/22/21JU

response 1833

Ion	Exp%	Act%
188.00	100	100
94.00	13.50	14.41
80.00	14.00	14.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028817.D
 Acq On : 19 Feb 2021 13:22
 Operator : CG/JU
 Sample : PB134691BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK91

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:07:44 PM

Quant Time: Feb 19 13:54:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 10:10:00 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	360	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	1467	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	894	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.27	188	1833m	0.40	ng/ul	0.00
16) Chrysene-d12	21.42	240	1528	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	1508	0.40	ng/ul	0.00

02/22/21 JU

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.28	152	990	0.47	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	2097	0.44	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed