


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028823.D
Acq On : 19 Feb 2021 17:03
Operator : CG/JU
Sample : M1412-13
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGX8

Manual Integrations
APPROVED

mohammad
2/22/2021 2:07:59 PM

Quant Time: Feb 19 17:39:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 10:10:00 2021
Response via : Initial Calibration

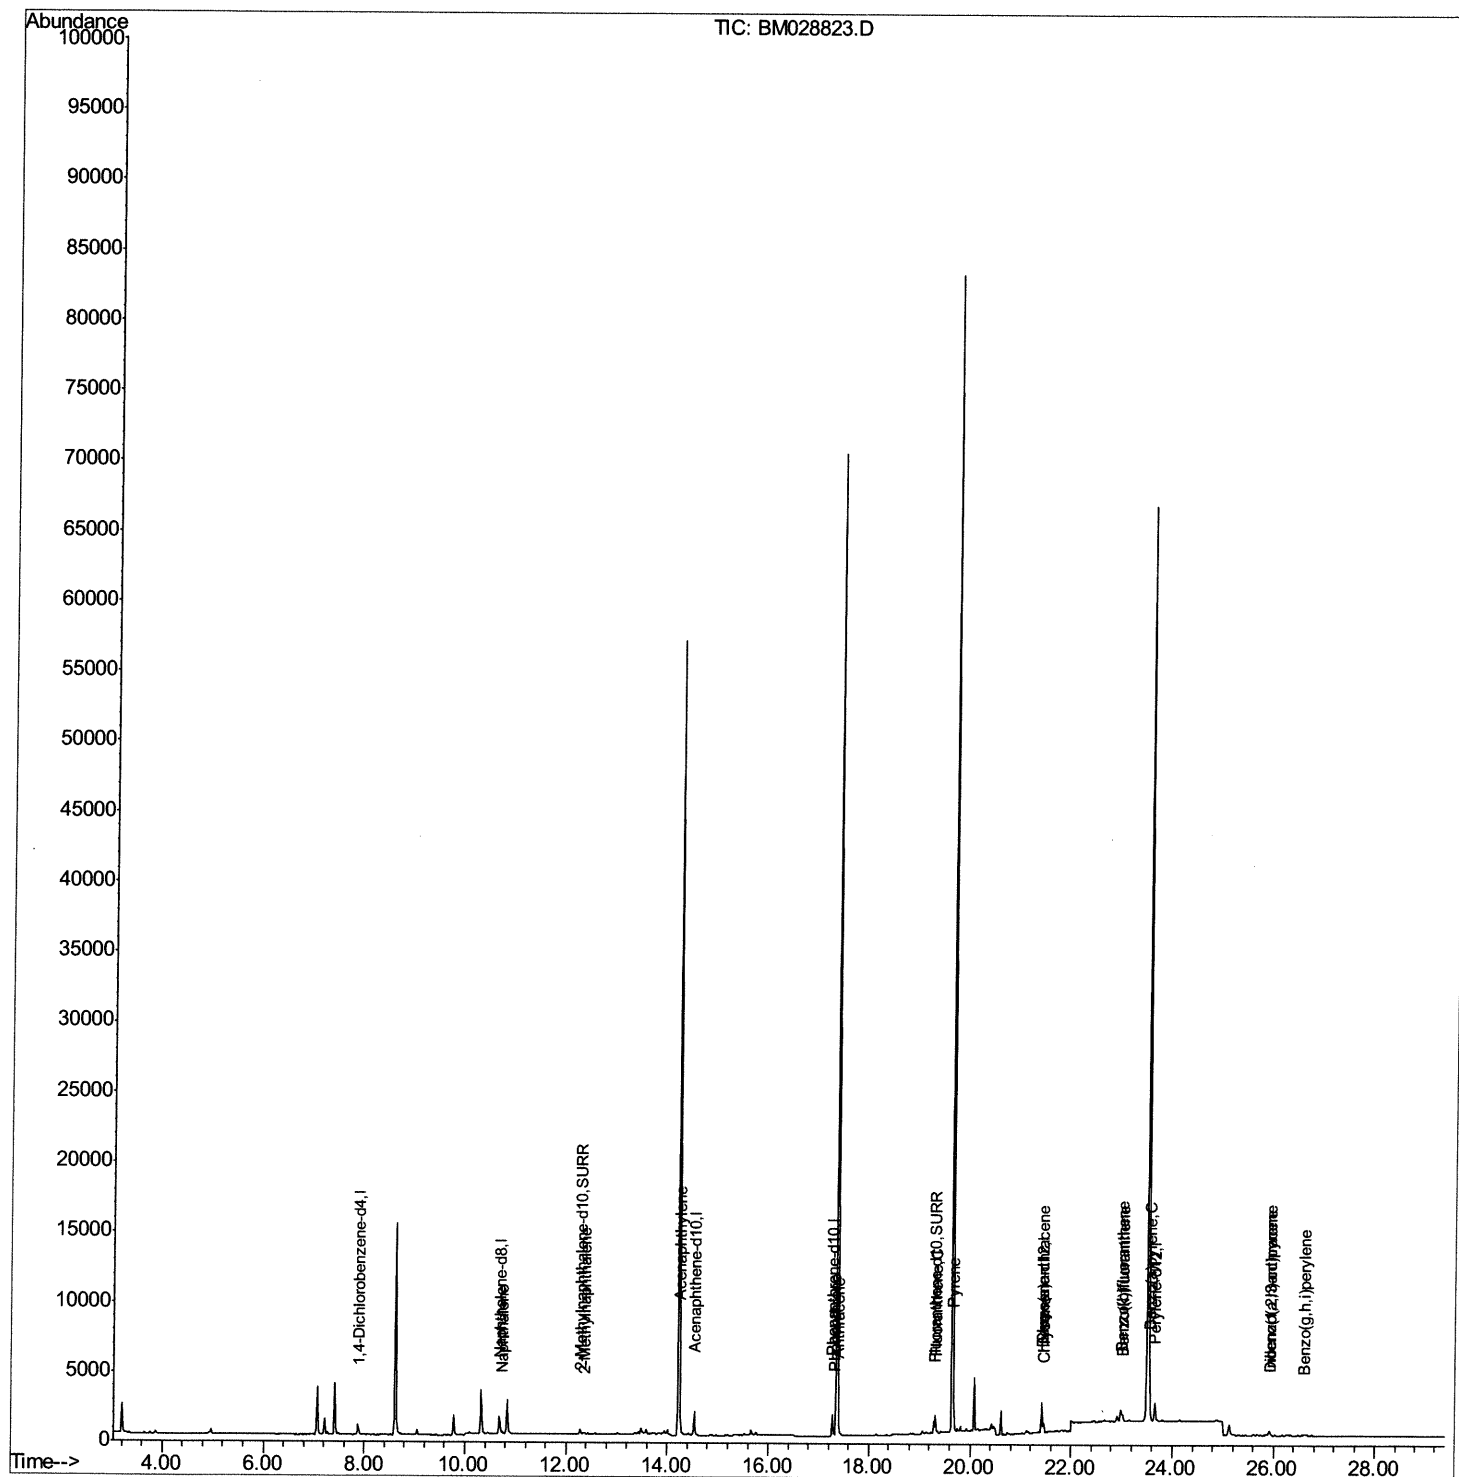

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028823.D
 Acq On : 19 Feb 2021 17:03
 Operator : CG/JU
 Sample : M1412-13
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGX8

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:07:59 PM

Quant Time: Feb 19 17:37:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 10:10:00 2021
 Response via : Initial Calibration

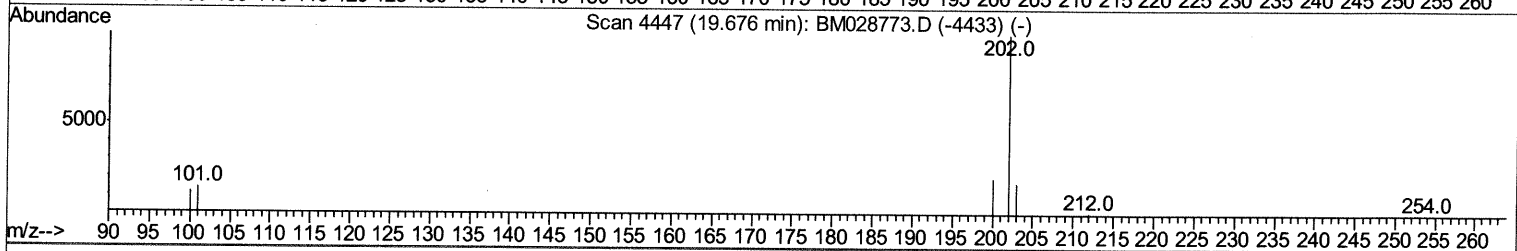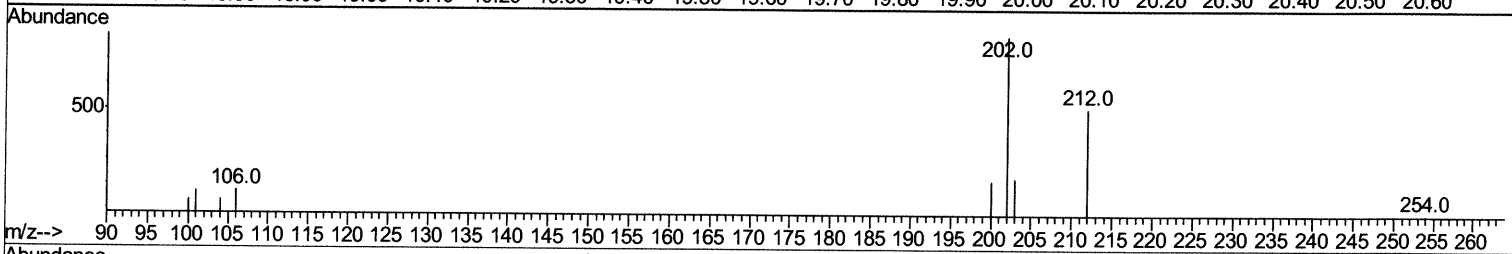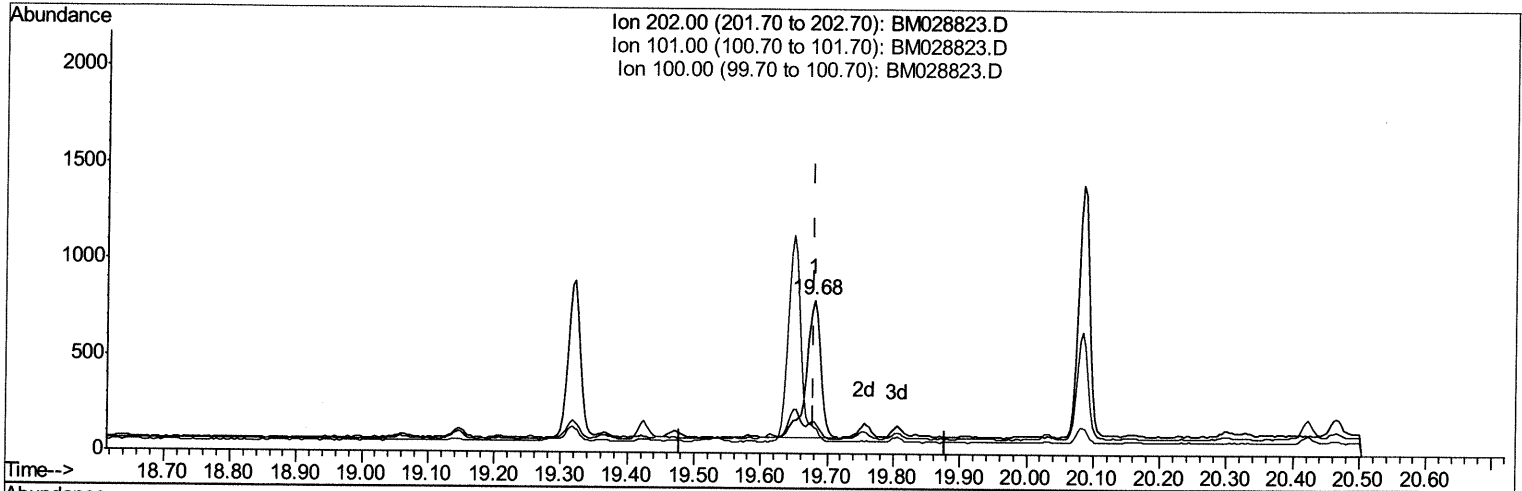

(17) Pyrene

19.680min (+0.001) 0.17ng/ul

response 1058

Ion	Exp%	Act%
202.00	100	100
101.00	15.90	21.05#
100.00	12.80	17.04#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028823.D
 Acq On : 19 Feb 2021 17:03
 Operator : CG/JU
 Sample : M1412-13
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGX8

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:07:59 PM

Quant Time: Feb 19 17:37:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 10:10:00 2021
 Response via : Initial Calibration

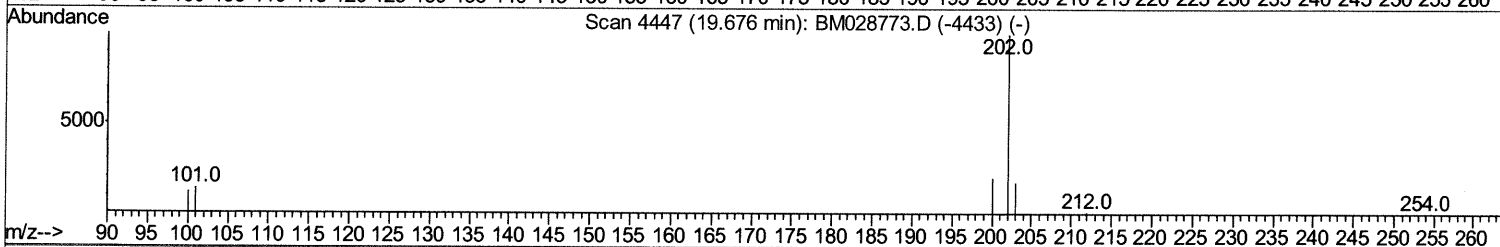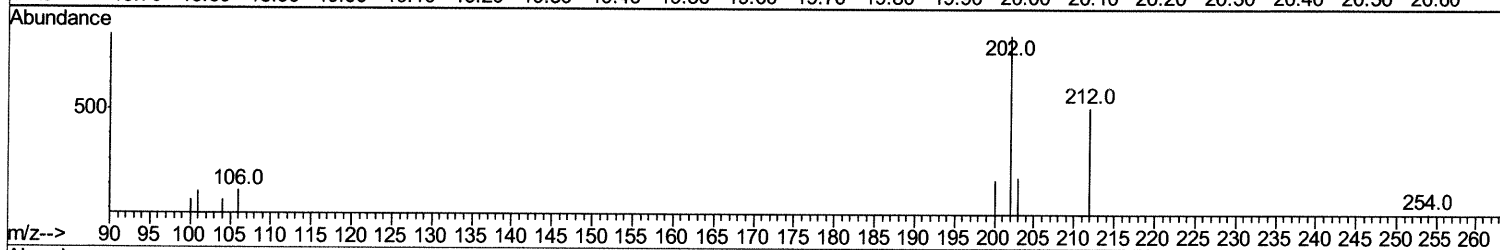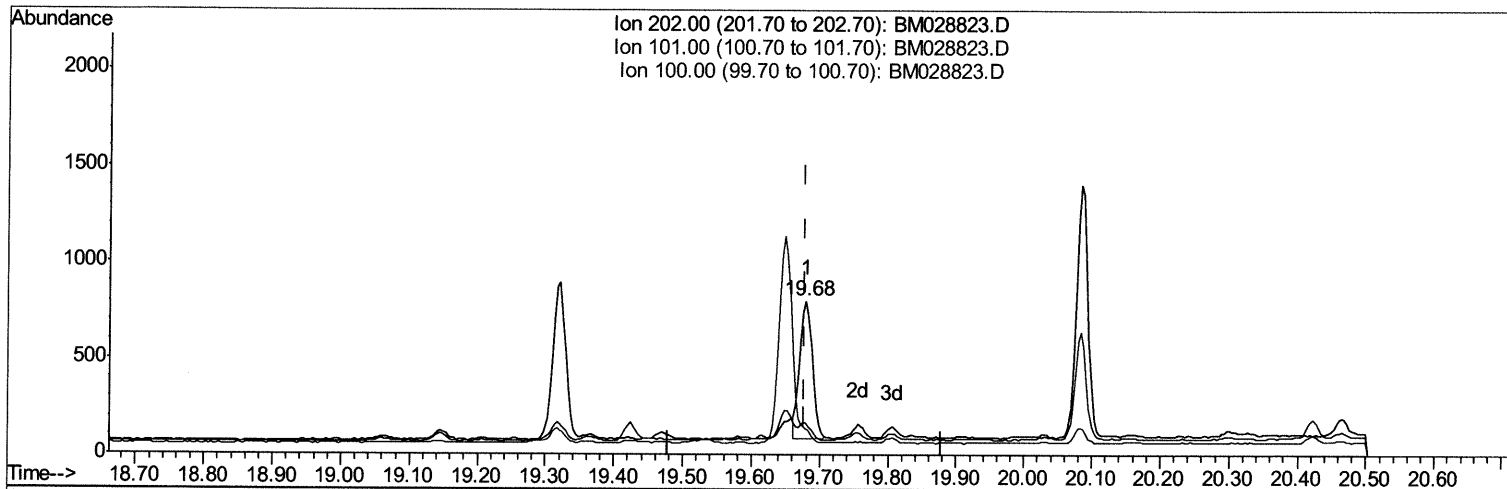

TIC: BM028823.D

(17) Pyrene

19.680min (+0.001) 0.15ng/ul m

response 921

Ion	Exp%	Act%
202.00	100	100
101.00	15.90	21.05#
100.00	12.80	17.04#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028823.D
Acq On : 19 Feb 2021 17:03
Operator : CG/JU
Sample : M1412-13
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGX8

Manual Integrations
APPROVED

mohammad
2/22/2021 2:07:59 PM

Quant Time: Feb 19 17:37:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 10:10:00 2021
Response via : Initial Calibration

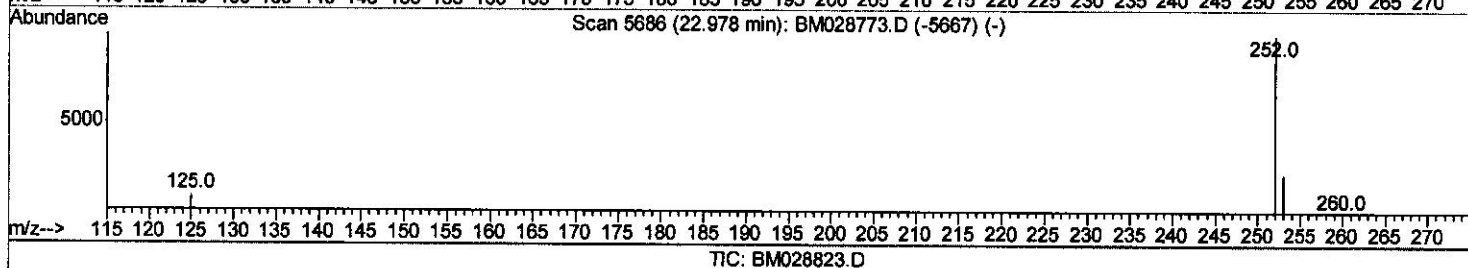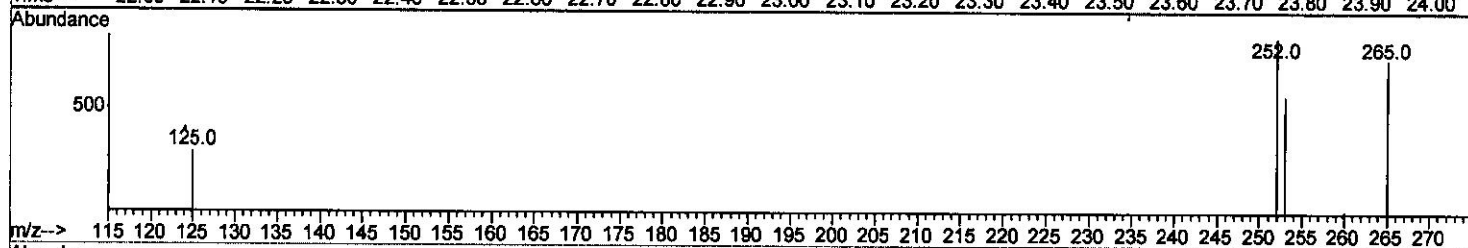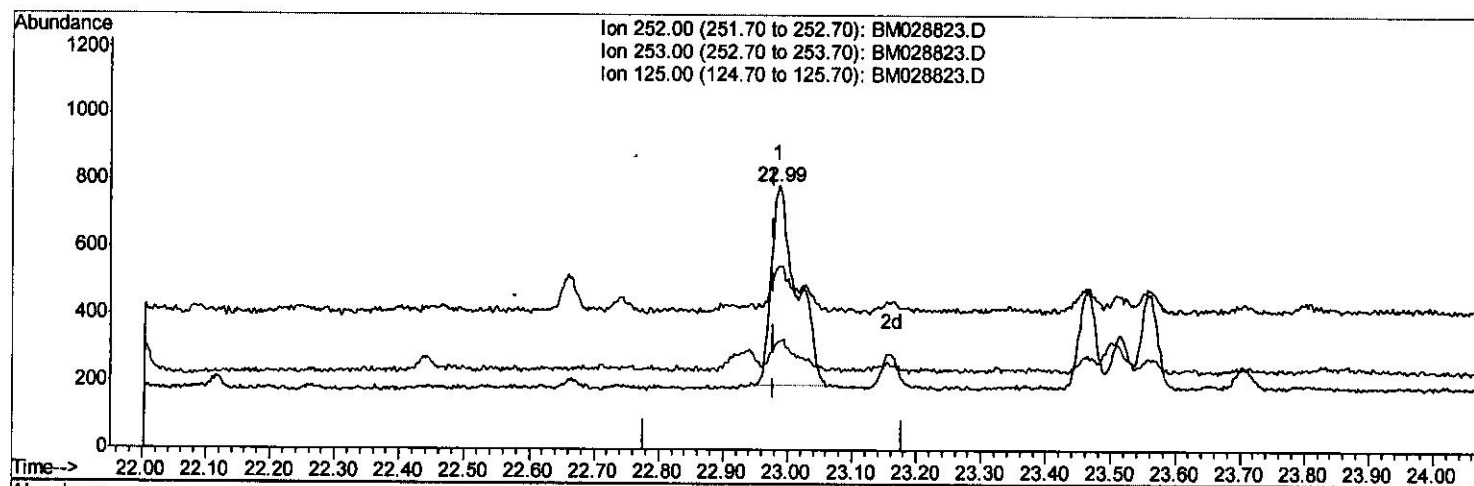

(21) Benzo(b)fluoranthene

22.987min (+0.009) 0.29ng/ui

response 1634

Ion	Exp%	Act%
252.00	100	100
253.00	33.50	69.76#
125.00	28.70	41.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028823.D
Acq On : 19 Feb 2021 17:03
Operator : CG/JU
Sample : M1412-13
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
Client Sampled :
DBGX8

Manual Integrations
APPROVED

mohammad
2/22/2021 2:07:59 PM

Quant Time: Feb 19 17:37:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 10:10:00 2021
Response via : Initial Calibration

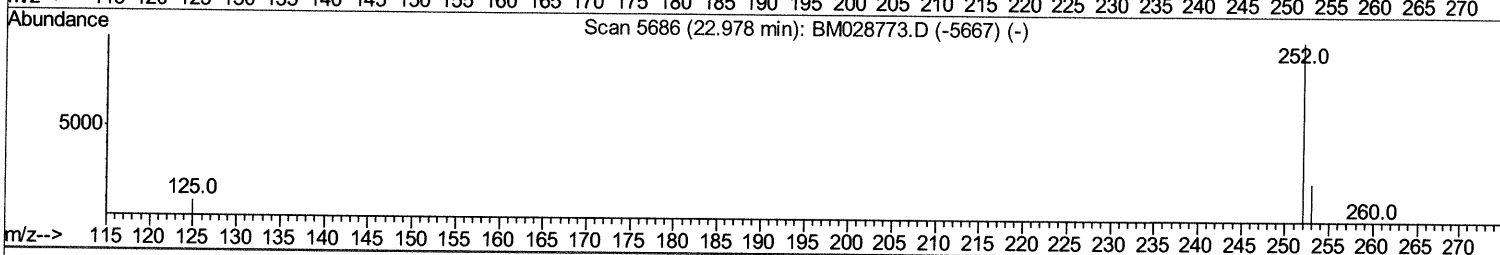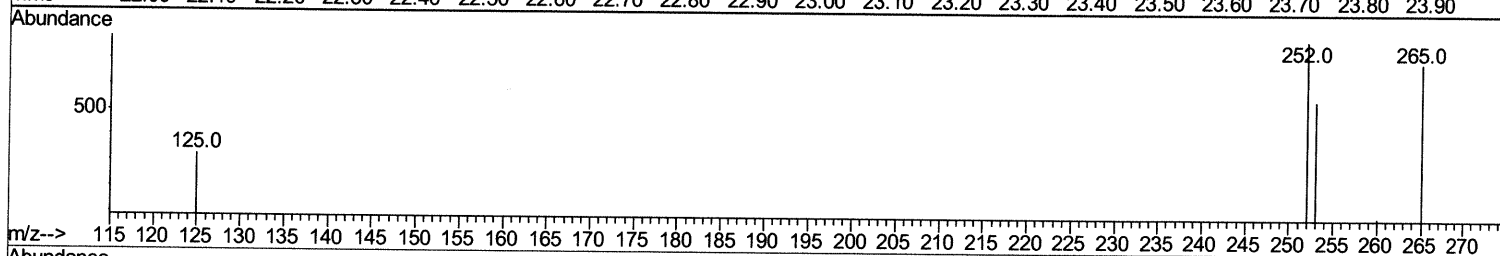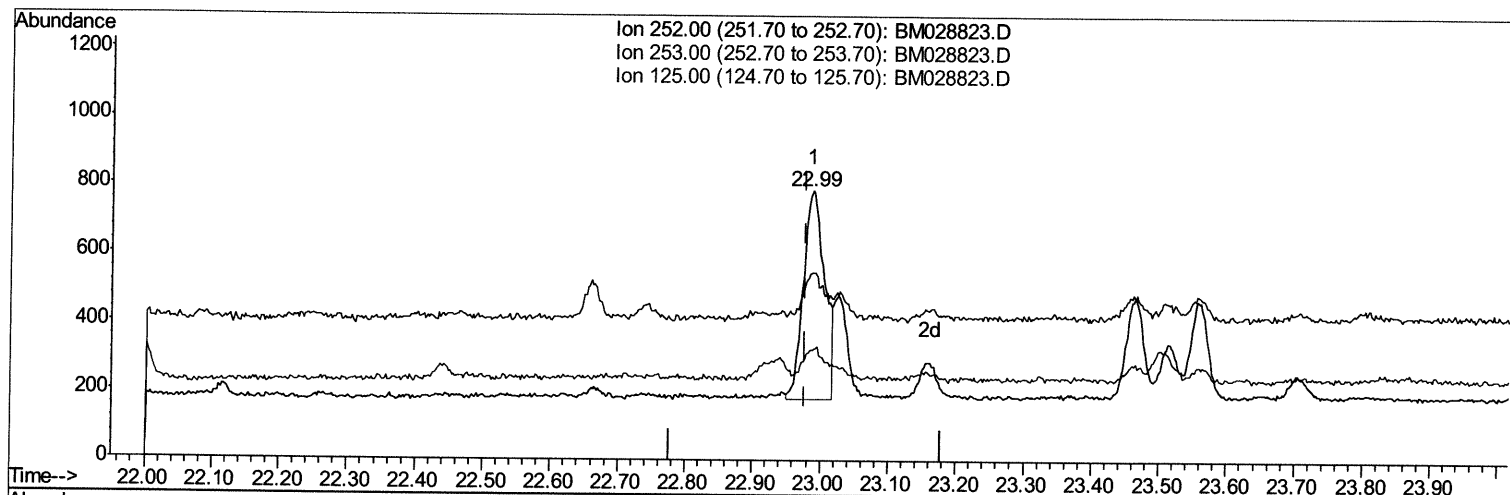

TIC: BM028823.D

(21) Benzo(b)fluoranthene

22.987min (+0.009) 0.23ng/ul m

response 1287

Ion	Exp%	Act%
252.00	100	100
253.00	33.50	69.76#
125.00	28.70	41.04
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028823.D
Acq On : 19 Feb 2021 17:03
Operator : CG/JU
Sample : M1412-13
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGX8

Manual Integrations
APPROVED

mohammad
2/22/2021 2:07:59 PM

Quant Time: Feb 19 17:37:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 10:10:00 2021
Response via : Initial Calibration

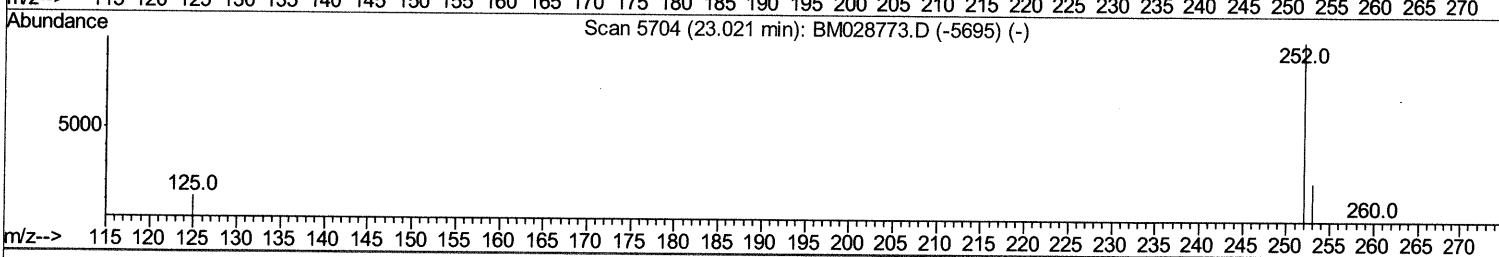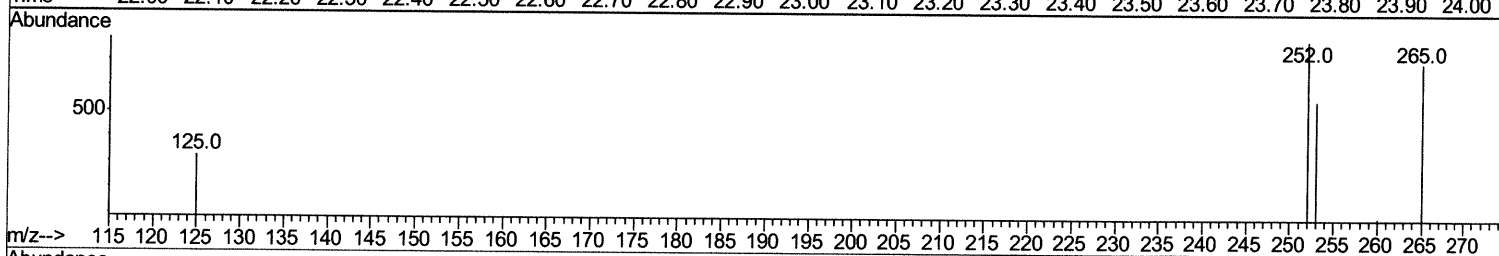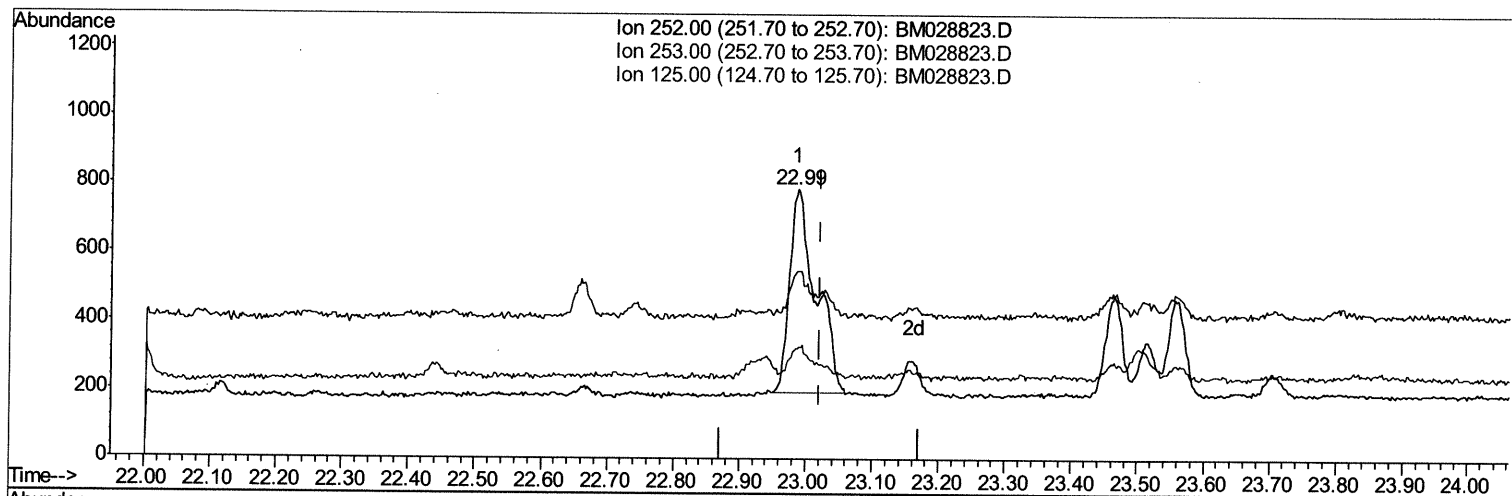

TIC: BM028823.D

(22) Benzo(k)fluoranthene

22.987min (-0.034) 0.29ng/ul

response 1634

Ion	Exp%	Act%
252.00	100	100
253.00	32.90	69.76#
125.00	28.60	41.04#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028823.D
 Acq On : 19 Feb 2021 17:03
 Operator : CG/JU
 Sample : M1412-13
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGX8

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:07:59 PM

Quant Time: Feb 19 17:37:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 10:10:00 2021
 Response via : Initial Calibration

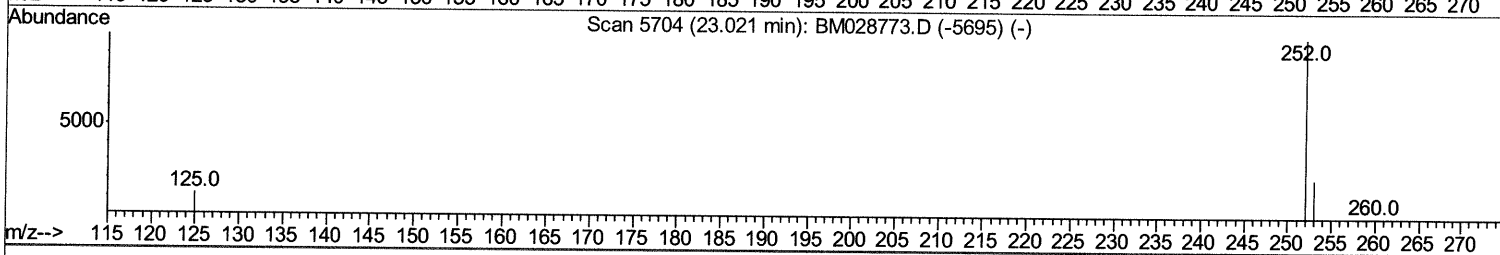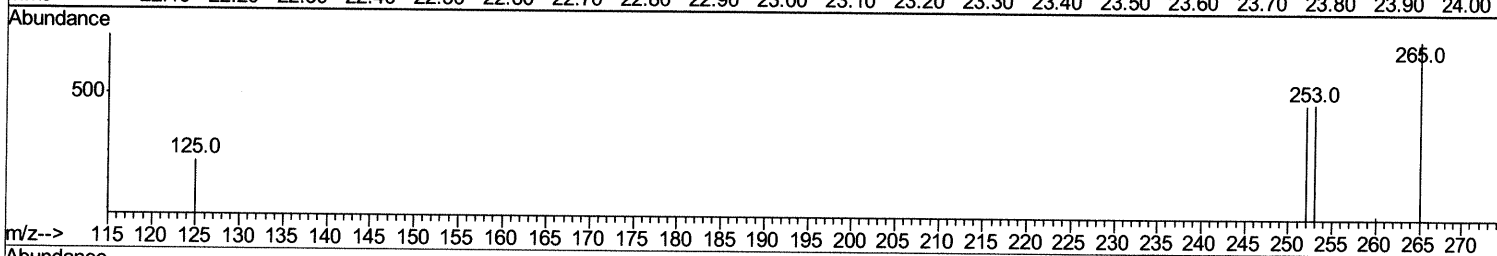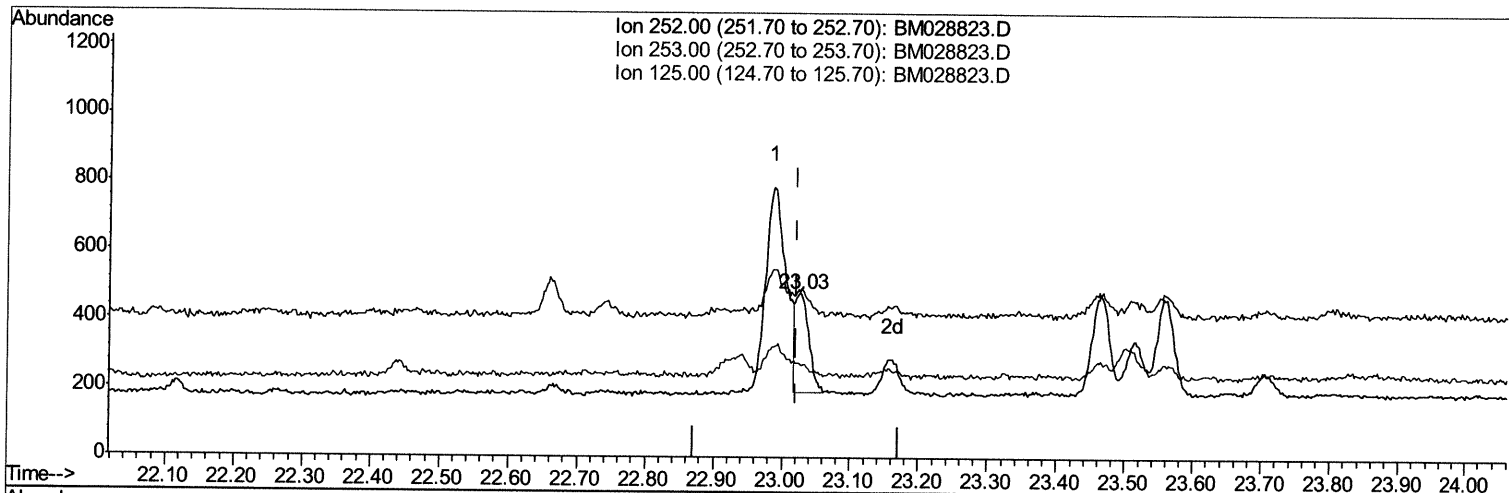

TIC: BM028823.D

(22) Benzo(k)fluoranthene

23.026min (+0.004) 0.07ng/ul m

response 402

Ion	Exp%	Act%
252.00	100	100
253.00	32.90	100.42#
125.00	28.60	56.69#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028823.D
 Acq On : 19 Feb 2021 17:03
 Operator : CG/JU
 Sample : M1412-13
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGX8

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:07:59 PM

Quant Time: Feb 19 17:39:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 10:10:00 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	400	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	1639	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	921	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.27	188	1790	0.40	ng/ul	0.00
16) Chrysene-d12	21.42	240	1746	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	1656	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	466	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	946	0.20	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.74	128	149	0.037	ng/ul#	28
5) 2-Methylnaphthalene	12.36	142	65	0.024	ng/ul	99
7) Acenaphthylene	14.26	152	149	0.040	ng/ul#	34
12) Phenanthrene	17.32	178	369	0.074	ng/ul#	70
13) Anthracene	17.41	178	169	0.035	ng/ul#	40
15) Fluoranthene	19.32	202	1082	0.190	ng/ul	94
17) Pyrene	19.68	202	921m	0.145	ng/ul	59
18) Benzo(a)anthracene	21.41	228	448	0.075	ng/ul#	59
19) Chrysene	21.46	228	746	0.126	ng/ul#	67
21) Benzo(b)fluoranthene	22.99	252	1287m	0.227	ng/ul	22
22) Benzo(k)fluoranthene	23.03	252	402m	0.071	ng/ul	100
23) Benzo(a)pyrene	23.56	252	497	0.098	ng/ul#	1
24) Indeno(1,2,3-cd)pyrene	25.91	276	461	0.070	ng/ul#	1
25) Dibenzo(a,h)anthracene	25.91	278	135	0.024	ng/ul#	1
26) Benzo(a,h,i)perylene	26.61	276	157	0.029	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed