


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028827.D
Acq On : 19 Feb 2021 19:30
Operator : CG/JU
Sample : M1412-02
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBG5

Manual Integrations
APPROVED

mohammad
2/22/2021 2:08:09 PM

Quant Time: Feb 20 01:32:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 20 01:10:53 2021
Response via : Initial Calibration

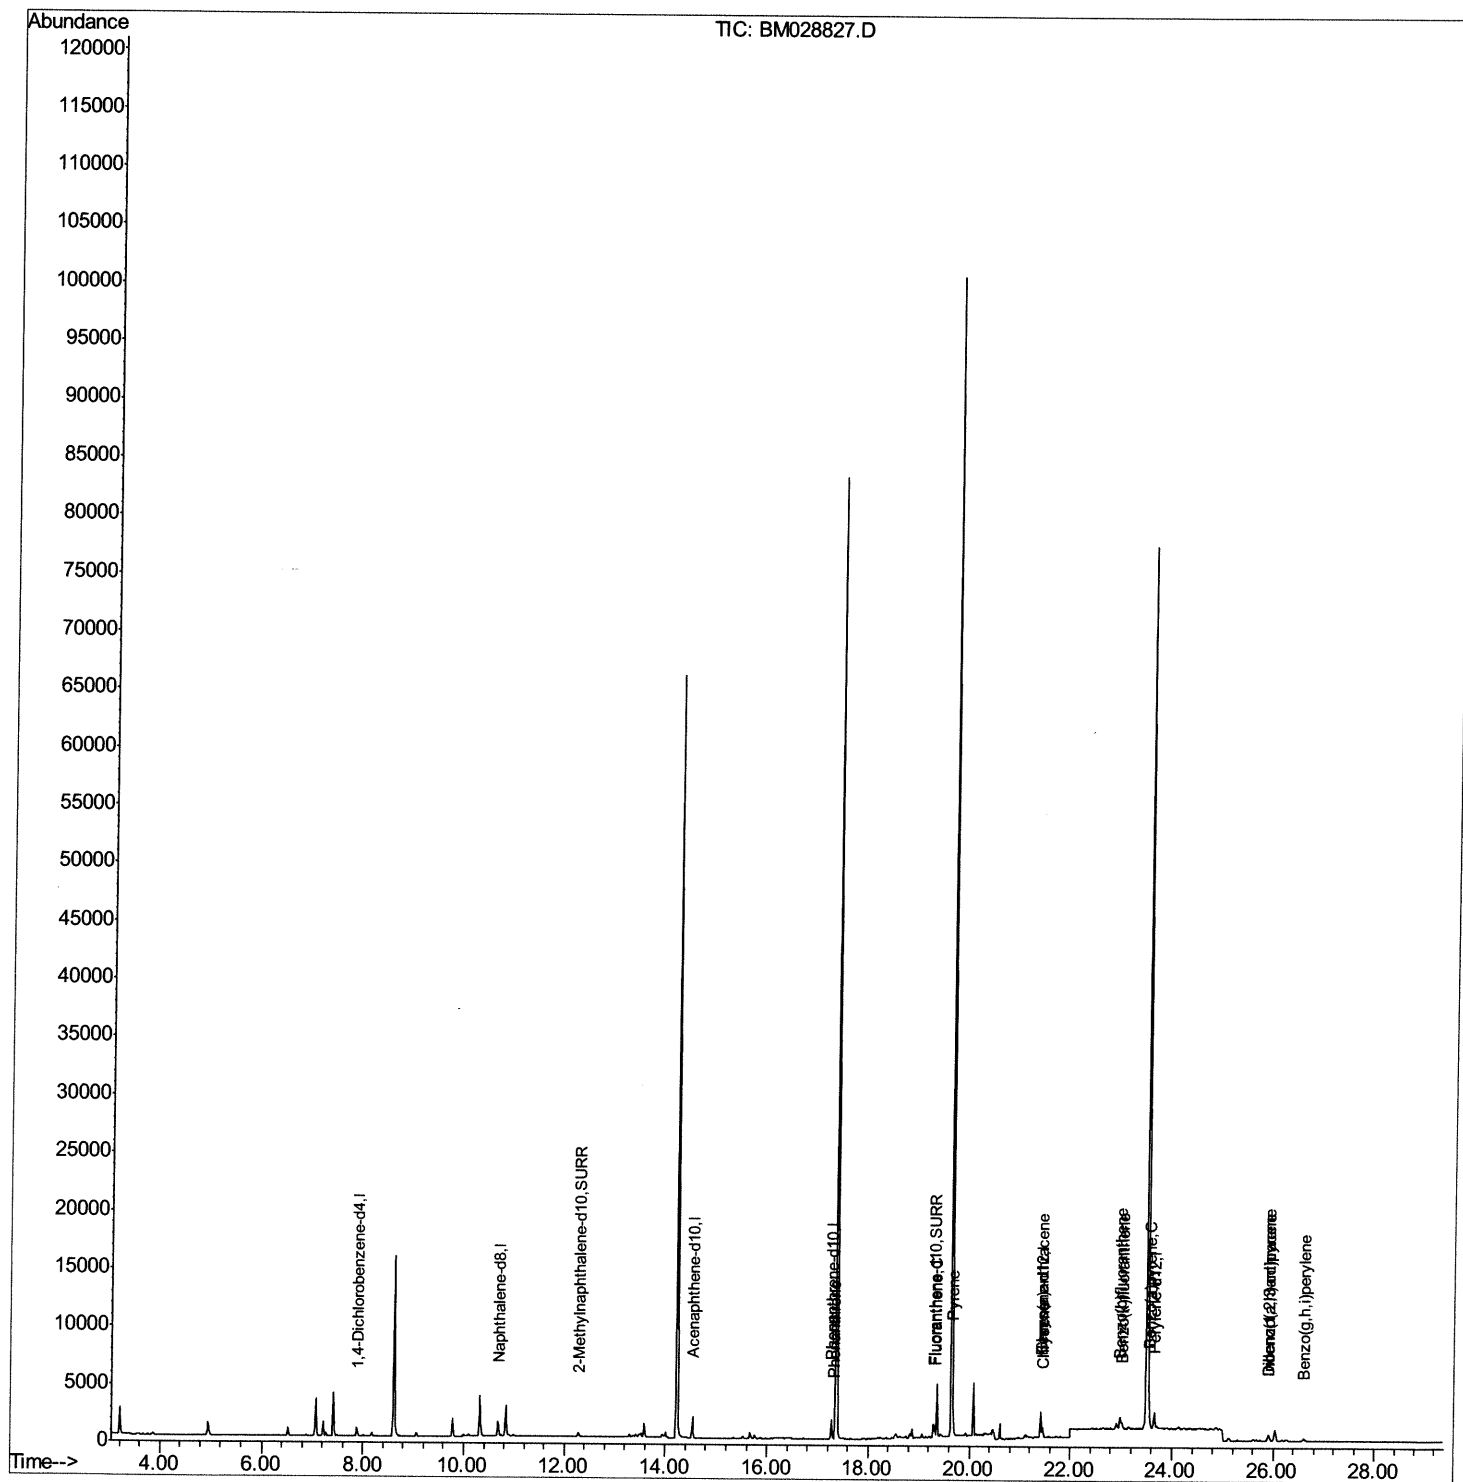

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028827.D
 Acq On : 19 Feb 2021 19:30
 Operator : CG/JU
 Sample : M1412-02
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBG5

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:08:09 PM

Quant Time: Feb 20 01:29:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 20 01:10:53 2021
 Response via : Initial Calibration

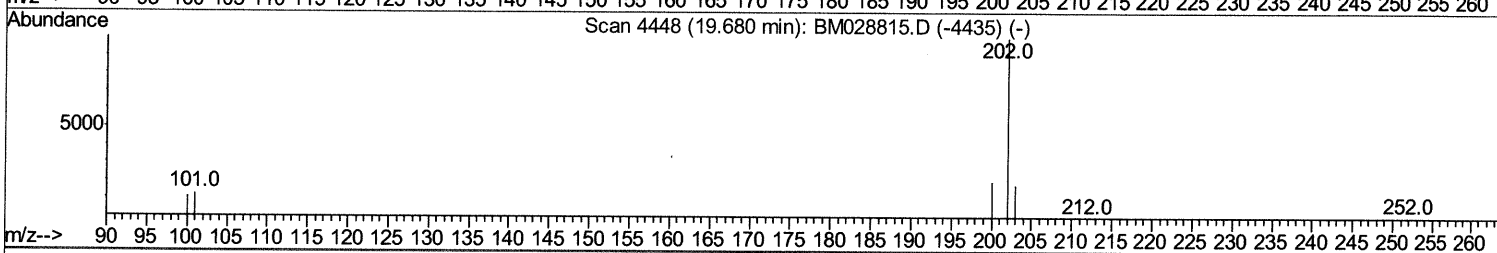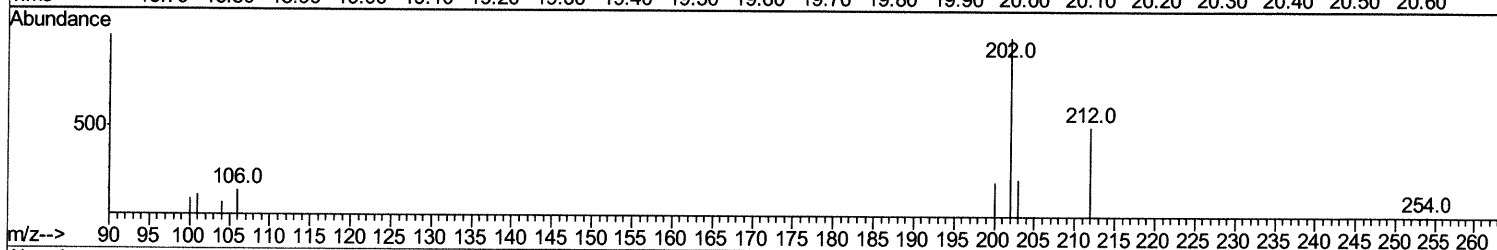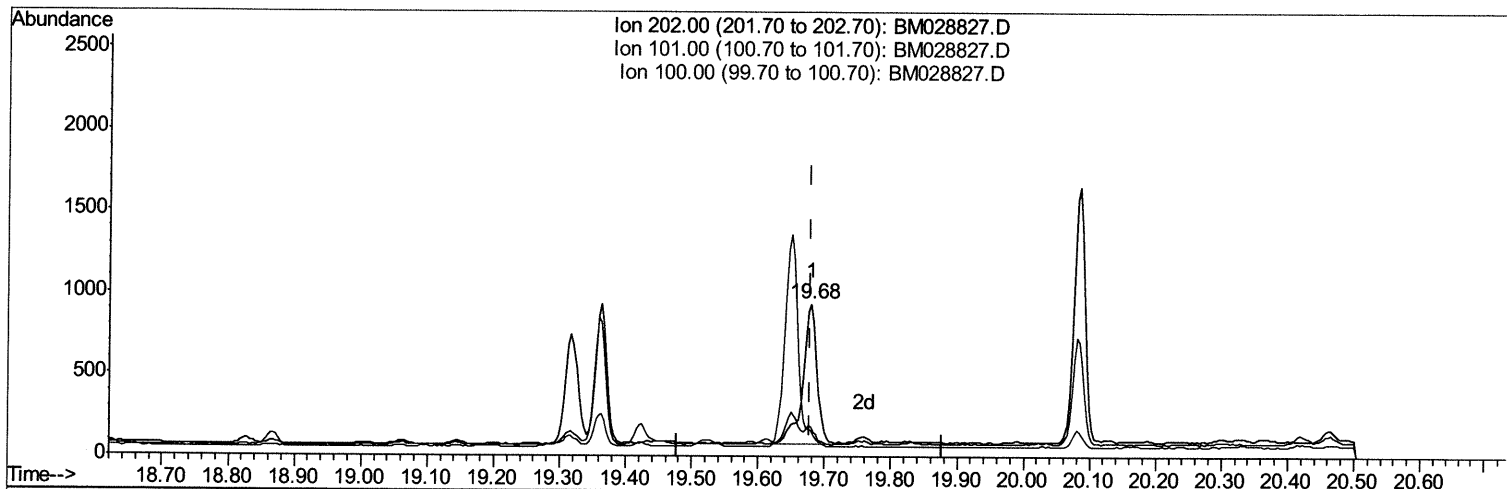

TIC: BM028827.D

(17) Pyrene

19.680min (+0.001) 0.19ng/ul

response 1279

Ion	Exp%	Act%
202.00	100	100
101.00	15.90	19.10#
100.00	12.80	16.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028827.D
Acq On : 19 Feb 2021 19:30
Operator : CG/JU
Sample : M1412-02
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGT5

Manual Integrations
APPROVED

mohammad
2/22/2021 2:08:09 PM

Quant Time: Feb 20 01:29:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 20 01:10:53 2021
Response via : Initial Calibration

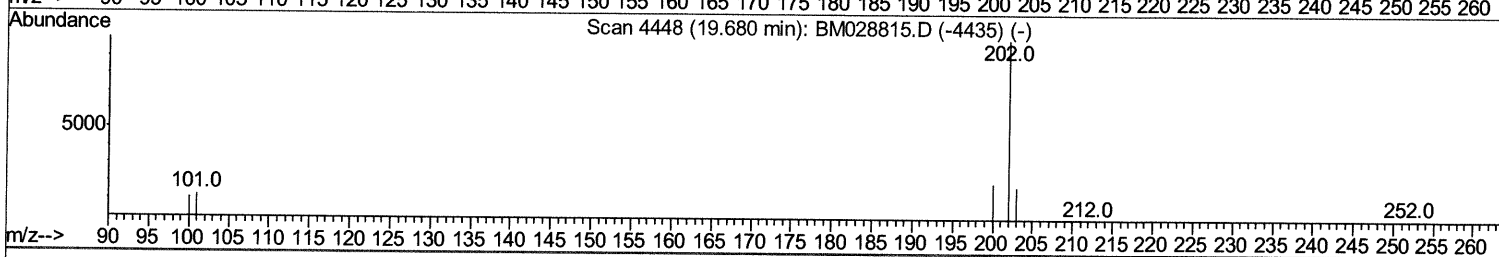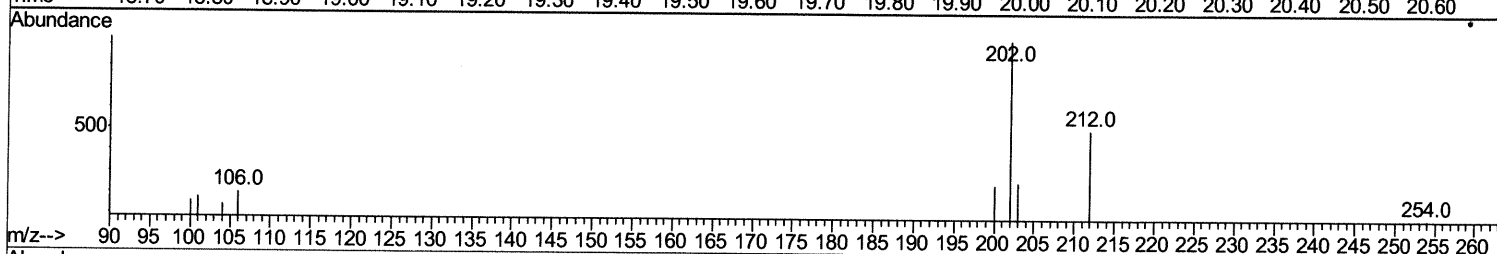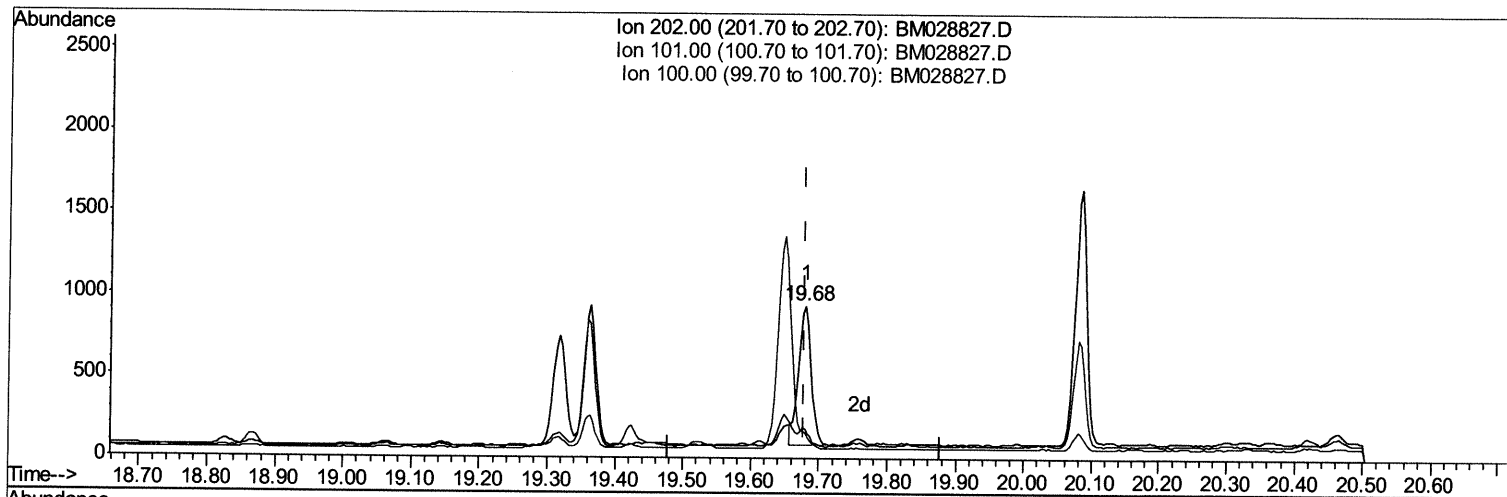

TIC: BM028827.D

(17) Pyrene

19.680min (+0.001) 0.17ng/ul m

response 1112

Ion	Exp%	Act%
202.00	100	100
101.00	15.90	19.10#
100.00	12.80	16.74#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028827.D
Acq On : 19 Feb 2021 19:30
Operator : CG/JU
Sample : M1412-02
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGT5

Manual Integrations
APPROVED

mohammad
2/22/2021 2:08:09 PM

Quant Time: Feb 20 01:29:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 20 01:10:53 2021
Response via : Initial Calibration

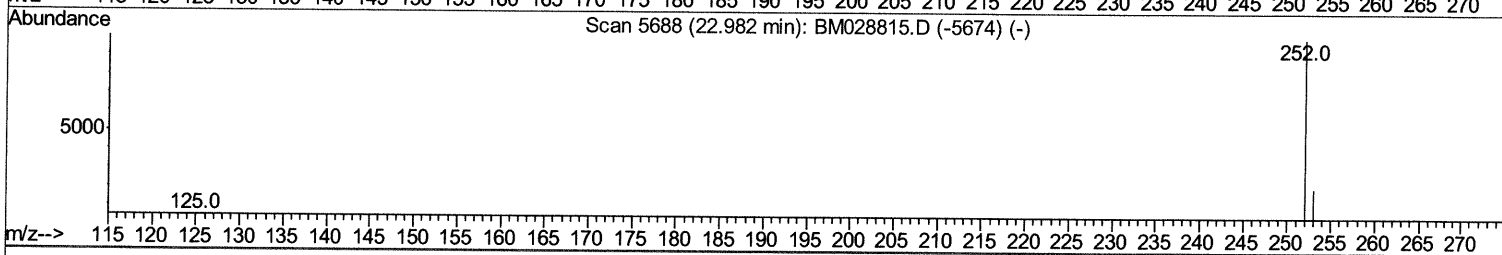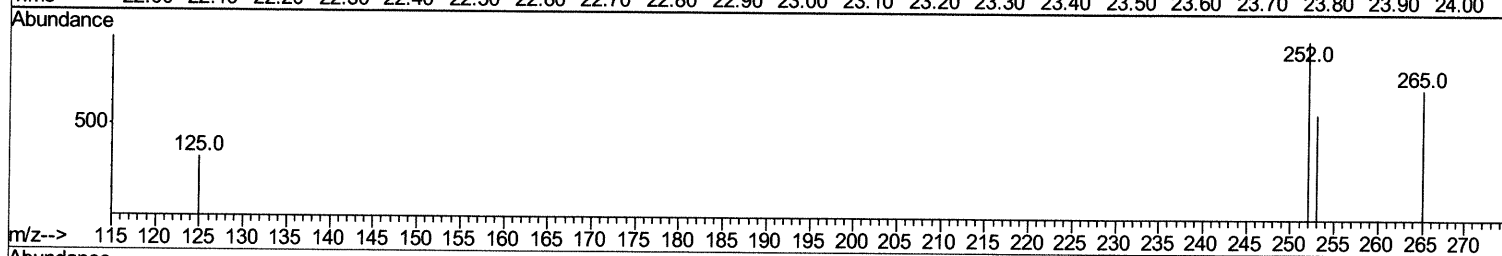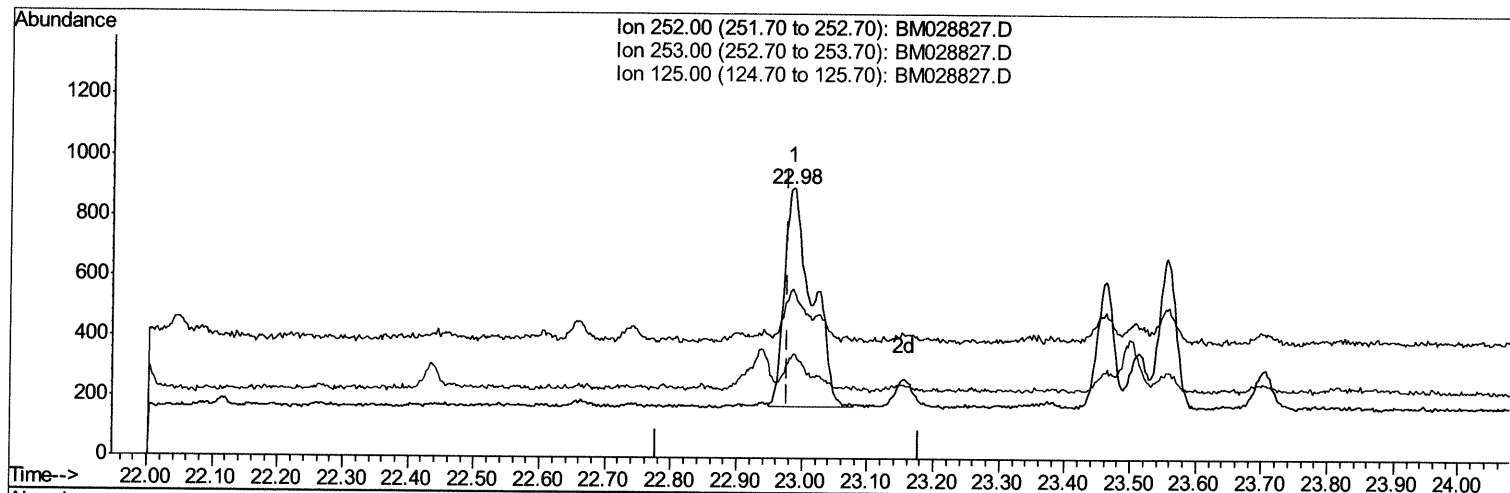

TIC: BM028827.D

(21) Benzo(b)fluoranthene

22.985min (+0.007) 0.35ng/ul

response 2132

Ion	Exp%	Act%
252.00	100	100
253.00	33.50	62.83
125.00	28.70	38.50
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028827.D
 Acq On : 19 Feb 2021 19:30
 Operator : CG/JU
 Sample : M1412-02
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBG5

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:08:09 PM

Quant Time: Feb 20 01:29:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 20 01:10:53 2021
 Response via : Initial Calibration

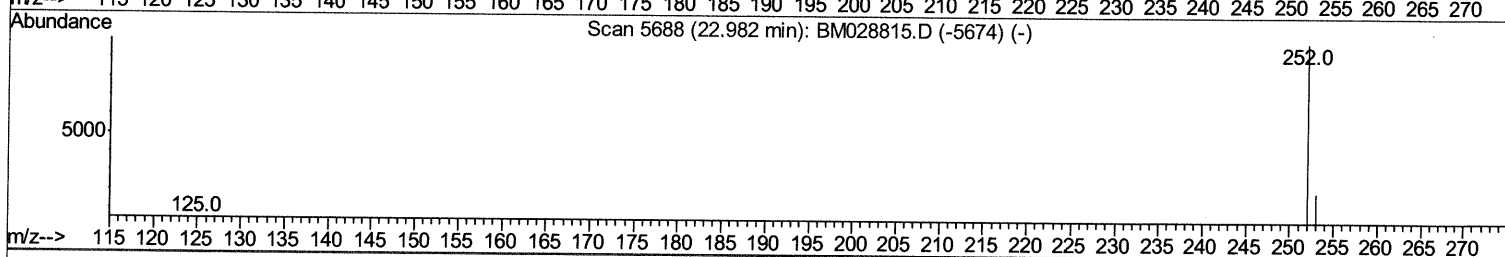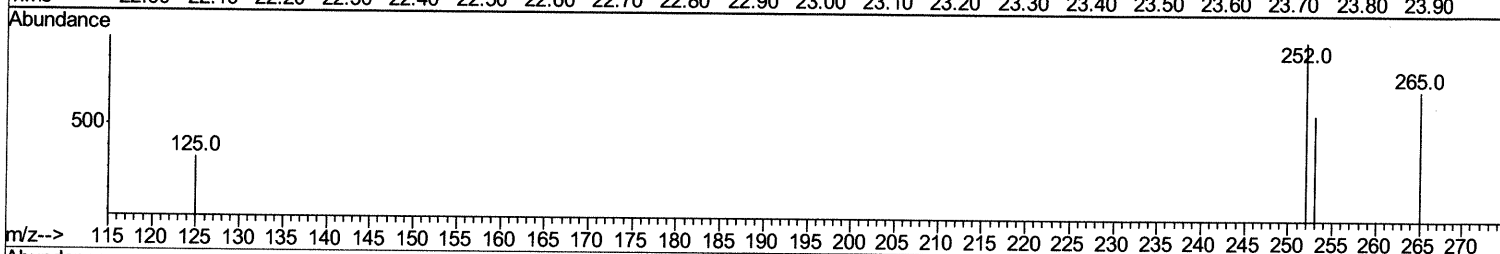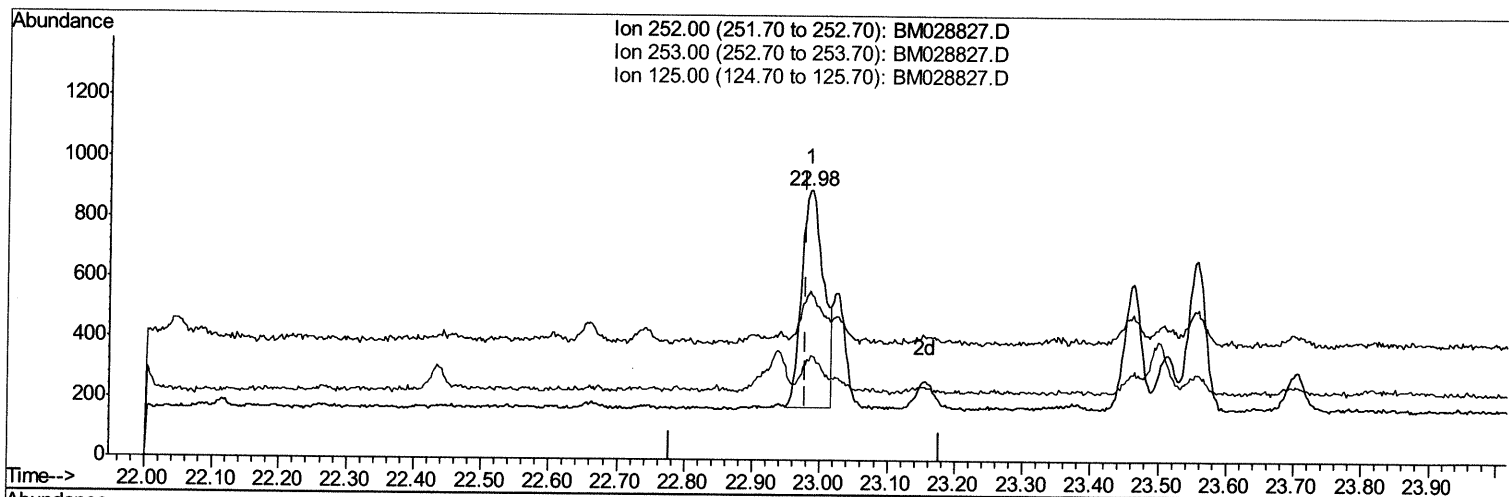

(21) Benzo(b)fluoranthene

22.985min (+0.007) 0.27ng/ul m

response 1614

Ion	Exp%	Act%
252.00	100	100
253.00	33.50	62.83
125.00	28.70	38.50
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028827.D
Acq On : 19 Feb 2021 19:30
Operator : CG/JU
Sample : M1412-02
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBG5

Manual Integrations
APPROVED

mohammad
2/22/2021 2:08:09 PM

Quant Time: Feb 20 01:29:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 20 01:10:53 2021
Response via : Initial Calibration

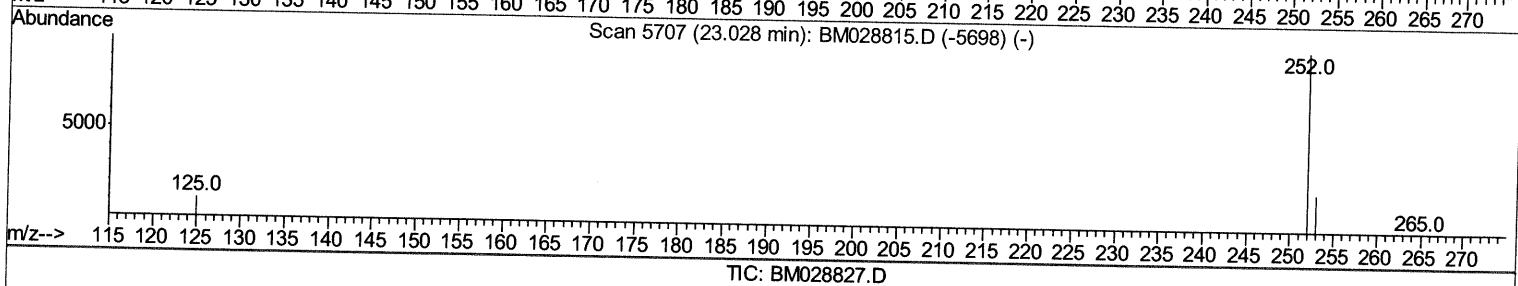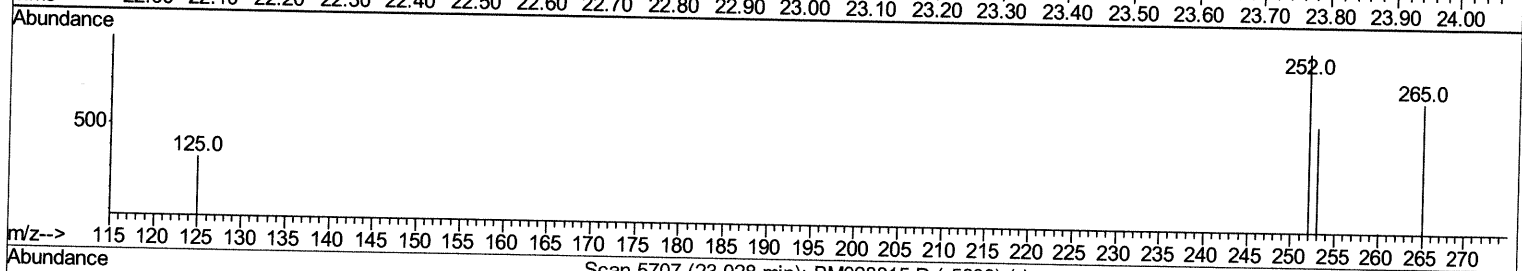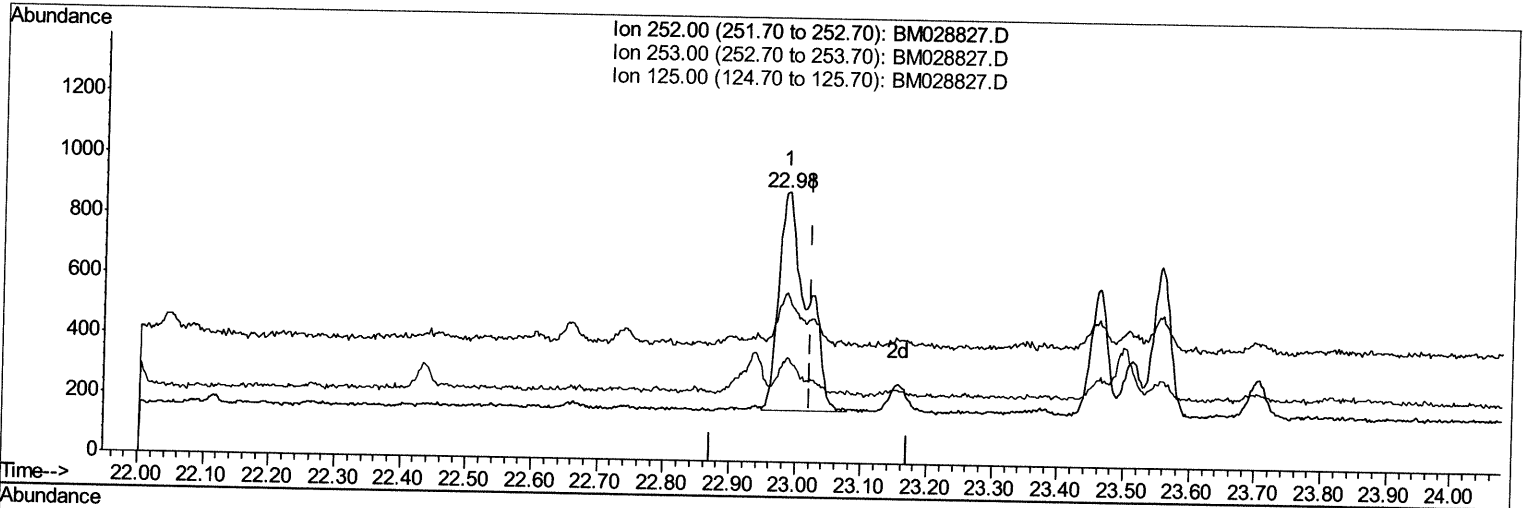

(22) Benzo(k)fluoranthene

22.985min (-0.037) 0.35ng/ul

response 2132

Ion	Exp%	Act%
252.00	100	100
253.00	32.90	62.83#
125.00	28.60	38.50#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
Data File : BM028827.D
Acq On : 19 Feb 2021 19:30
Operator : CG/JU
Sample : M1412-02
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBG5

Manual Integrations
APPROVED

mohammad
2/22/2021 2:08:09 PM

Quant Time: Feb 20 01:29:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 20 01:10:53 2021
Response via : Initial Calibration

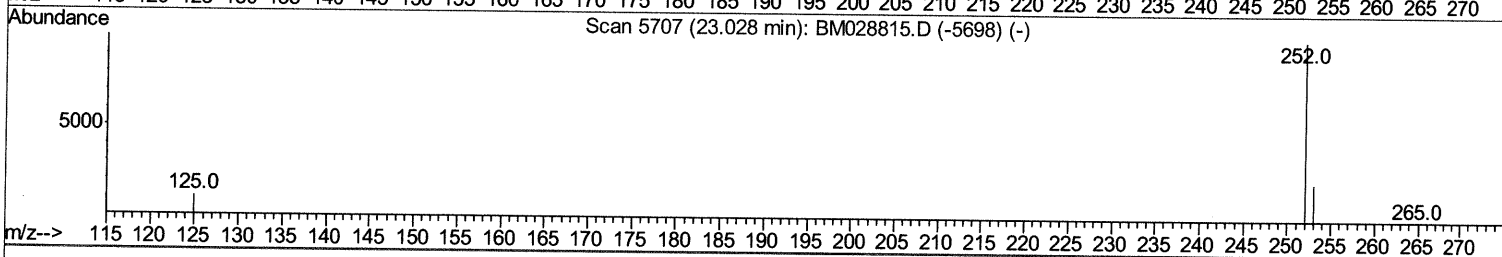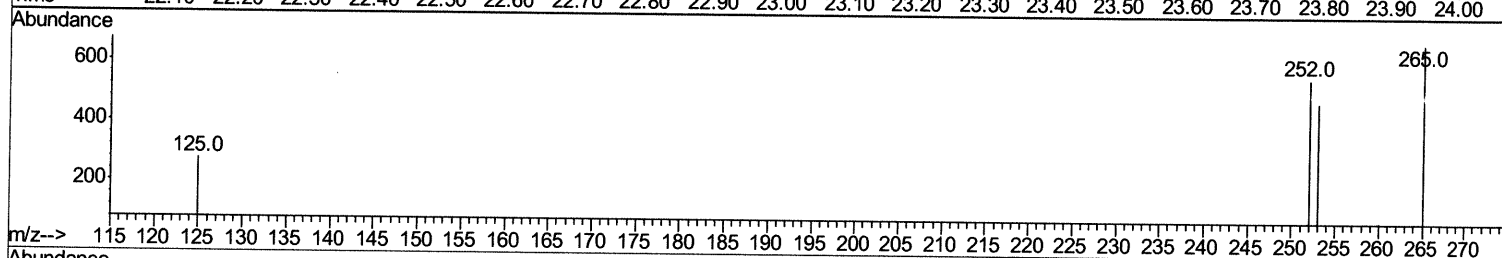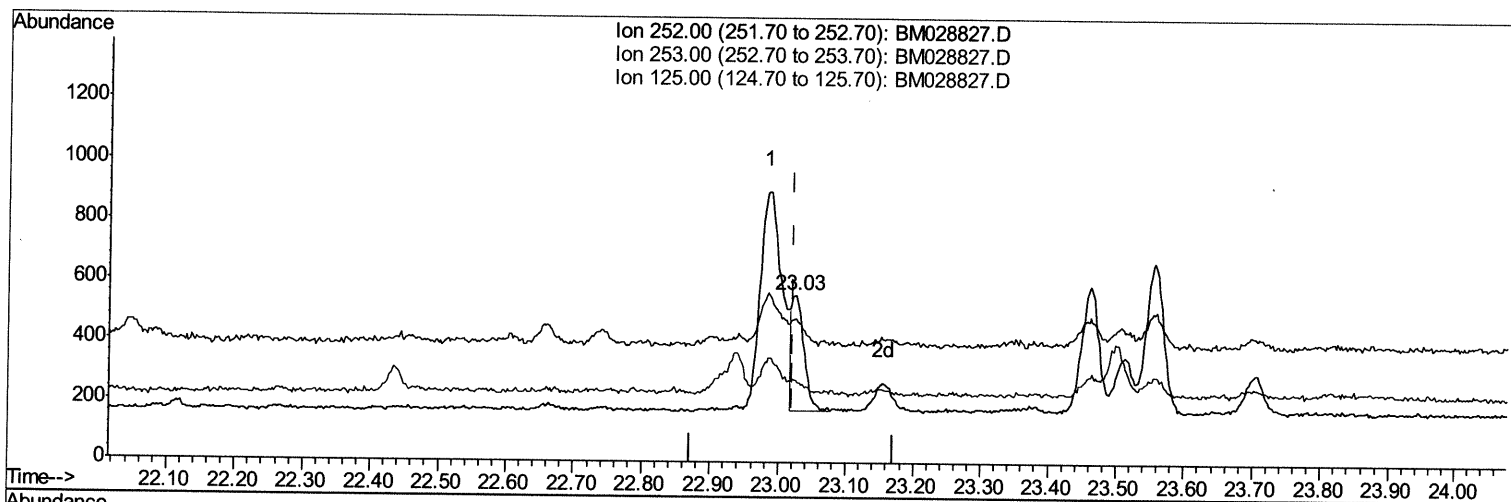

TIC: BM028827.D

(22) Benzo(k)fluoranthene

23.026min (+0.004) 0.08ng/ul m

response 501

Ion	Exp%	Act%
252.00	100	100
253.00	32.90	85.95#
125.00	28.60	49.19#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021821\
 Data File : BM028827.D
 Acq On : 19 Feb 2021 19:30
 Operator : CG/JU
 Sample : M1412-02
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGT5

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:08:09 PM

Quant Time: Feb 20 01:32:51 2021

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Feb 20 01:10:53 2021

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	411	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	1742	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	1039	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.27	188	2003	0.40	ng/ul	0.00
16) Chrysene-d12	21.42	240	1853	0.40	ng/ul	0.00
20) Perylene-d12	23.65	264	1773	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.28	152	508	0.21	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	1153	0.22	ng/ul	0.00

Target Compounds

					Ovalue	
12) Phenanthrene	17.31	178	181	0.032	ng/ul#	50
15) Fluoranthene	19.32	202	885	0.139	ng/ul	88
17) Pyrene	19.68	202	1112m	0.165	ng/ul	74 2/22/21
18) Benzo(a)anthracene	21.41	228	601	0.095	ng/ul#	73
19) Chrysene	21.46	228	869	0.138	ng/ul#	75
21) Benzo(b)fluoranthene	22.98	252	1614m	0.266	ng/ul	74 2/22/21
22) Benzo(k)fluoranthene	23.03	252	501m	0.083	ng/ul	74 2/22/21
23) Benzo(a)pyrene	23.56	252	898	0.166	ng/ul#	60
24) Indeno(1,2,3-cd)pyrene	25.91	276	782	0.111	ng/ul#	100
25) Dibenzo(a,h)anthracene	25.92	278	197	0.033	ng/ul#	1
26) Benzo(g,h,i)perylene	26.61	276	337	0.058	ng/ul#	33

(#) = qualifier out of range (m) = manual integration (+) = signals summed