

Data Path : Z:\HPCHEM1\BNA_M\Data\BM021915\
 Data File : BM000551.D
 Acq On : 19 Feb 2015 12:13
 Operator : TP/IZ
 Sample : G1291-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 19 13:32:41 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM021815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 19 10:41:02 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	2802	0.40	ng/ul	0.00
2) Naphthalene-d8	10.47	136	9996	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.32	164	6031	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.07	188	12453	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	8159	0.40	ng/ul	0.00
20) Perylene-d12	23.48	264	6238	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.06	152	3768	0.28	ng/ul	-0.01
14) Fluoranthene-d10	19.10	212	8770	0.33	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.51	128	14189	0.57	ng/ul	99
5) 2-Methylnaphthalene	12.13	142	10094	0.57	ng/ul	100
9) Fluorene	15.39	166	16780	0.71	ng/ul	96
11) Pentachlorophenol	16.73	266	6020	1.71	ng/ul	96
12) Phenanthrene	17.10	178	29028	0.83	ng/ul#	91
15) Fluoranthene	19.14	202	25250	0.63	ng/ul	98
18) Benzo(a)anthracene	21.25	228	22386	0.87	ng/ul	100
22) Benzo(k)fluoranthene	22.86	252	16594	0.72	ng/ul#	88
24) Indeno(1,2,3-cd)pyrene	25.70	276	13092	0.67	ng/ul	98
26) Benzo(g,h,i)perylene	26.39	276	19624	1.16	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM021915\
Data File : BM000551.D
Acq On : 19 Feb 2015 12:13
Operator : TP/IZ
Sample : G1291-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 19 13:32:41 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM021815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 19 10:41:02 2015
Response via : Initial Calibration




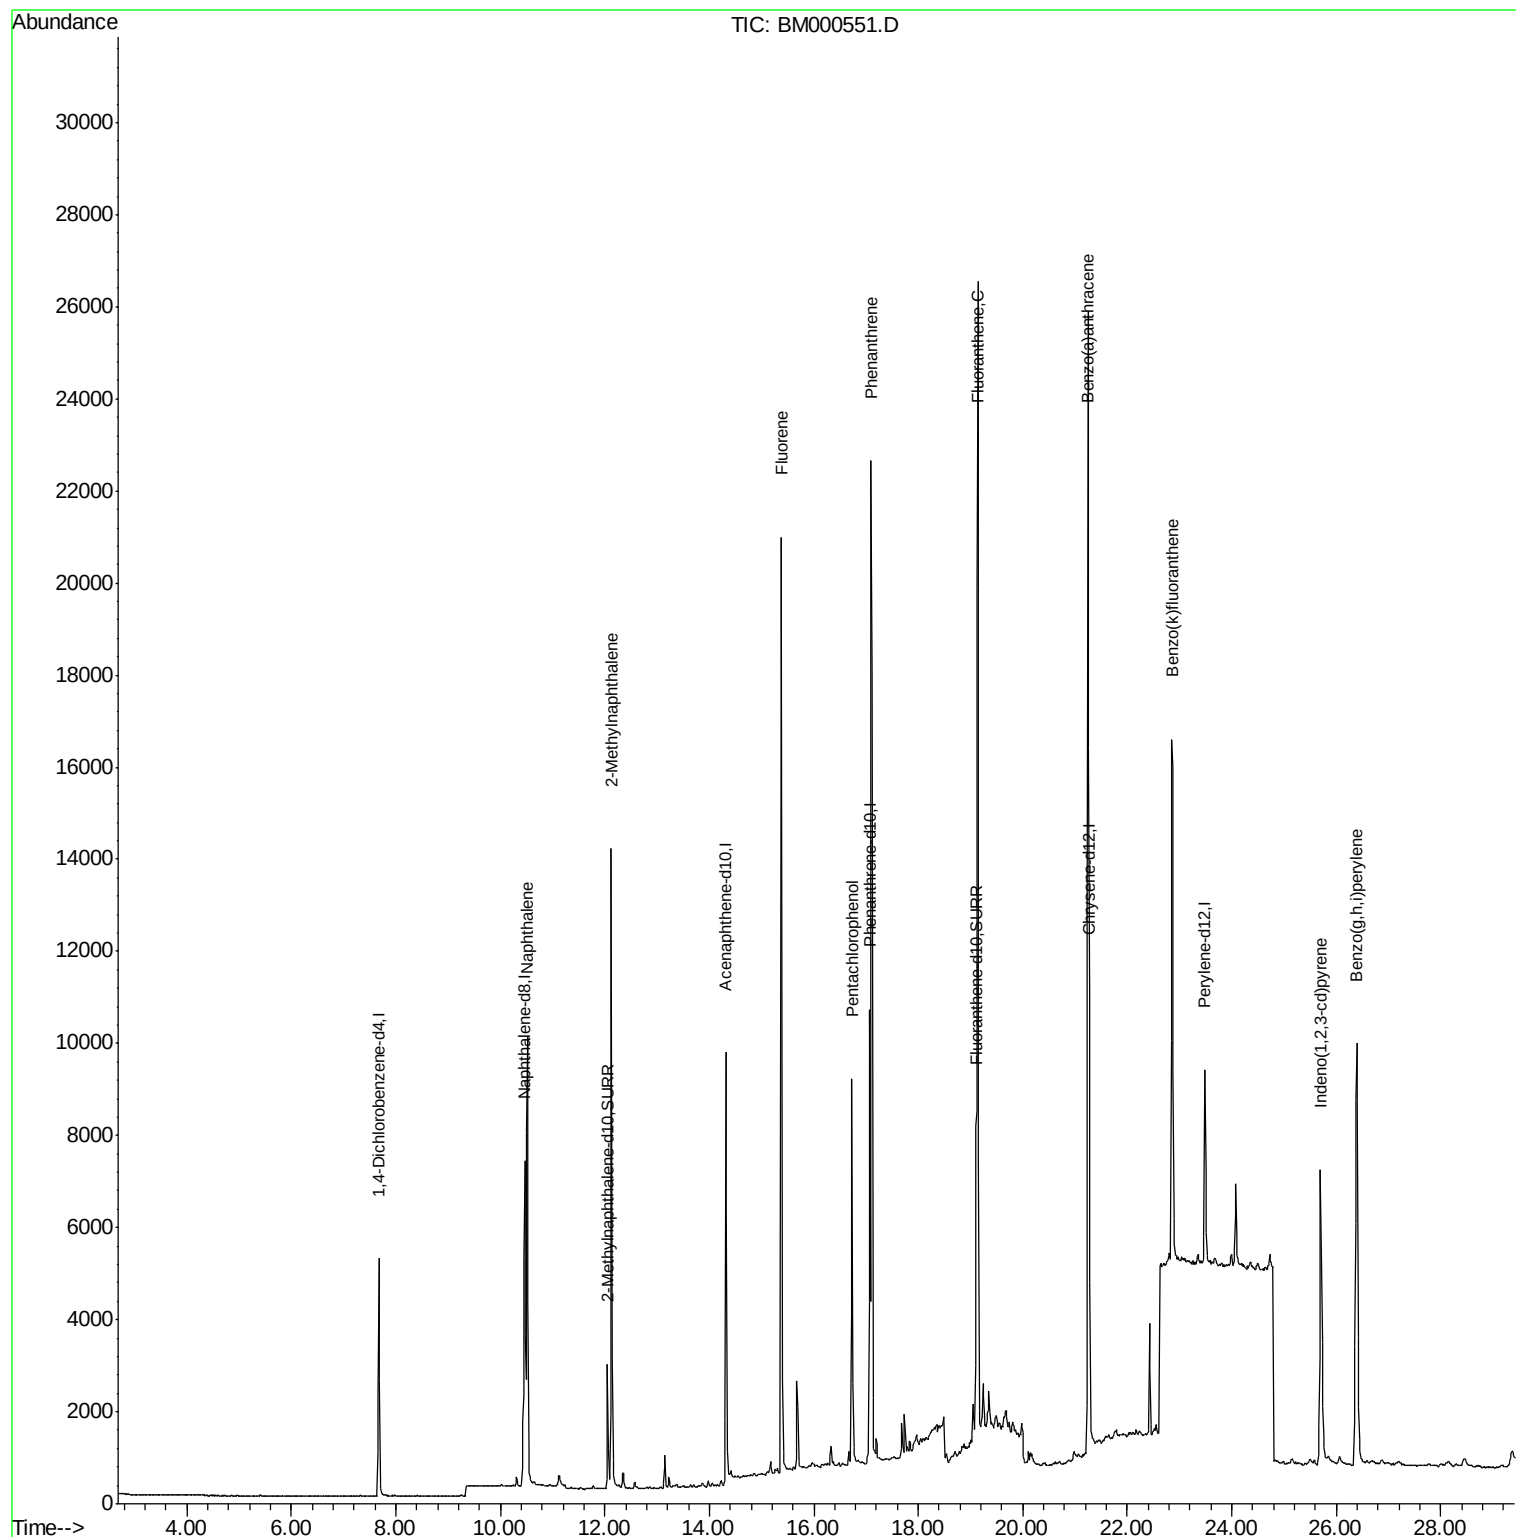


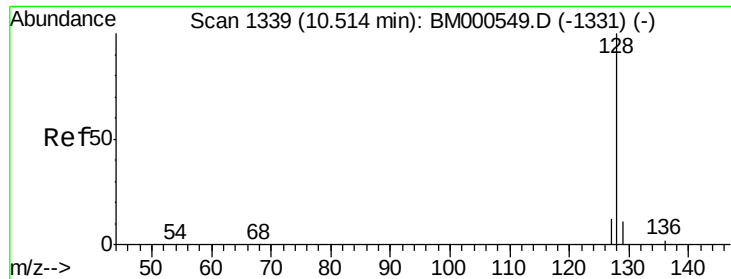

#3
Naphthalene
Concen: 0.57 ng/ul
RT: 10.51 min Scan# 1339
Delta R.T. -0.00 min
Lab File: BM000551.D
Acq: 19 Feb 2015 12:13




Instrument :
BNA_M
ClientSampled :


Tgt Ion:128 Resp: 14189
Ion Ratio Lower Upper
128 100
129 11.9 9.0 13.6
127 12.6 10.6 15.8

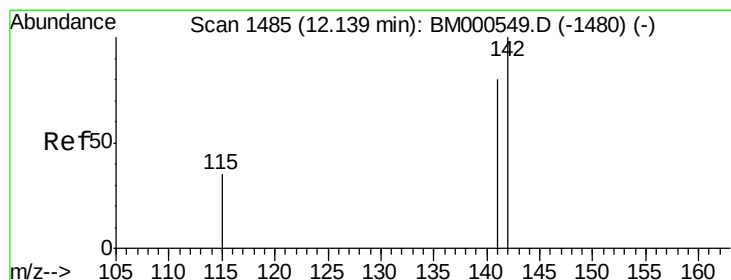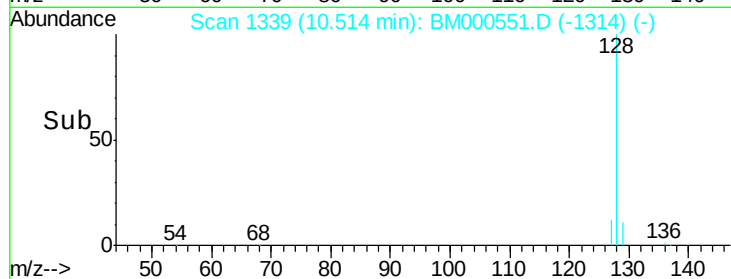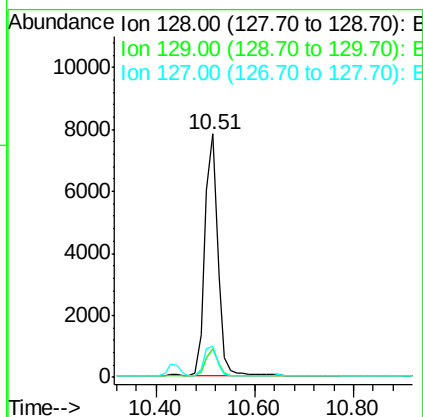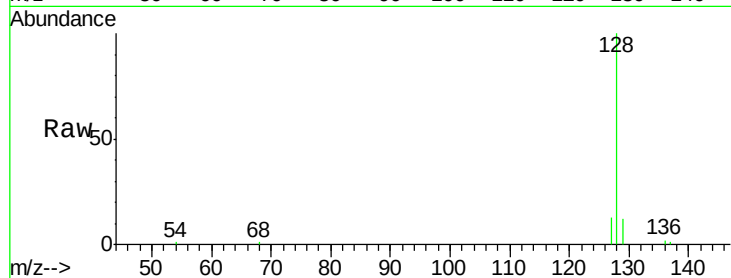

#5
2-Methylnaphthalene
Concen: 0.57 ng/ul
RT: 12.13 min Scan# 1484
Delta R.T. -0.01 min
Lab File: BM000551.D
Acq: 19 Feb 2015 12:13

Tgt Ion:142 Resp: 10094
Ion Ratio Lower Upper
142 100
141 88.1 70.4 105.6


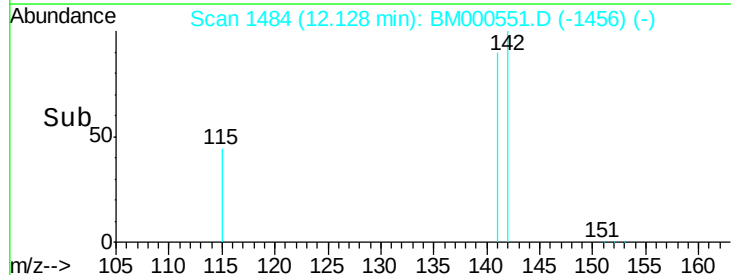
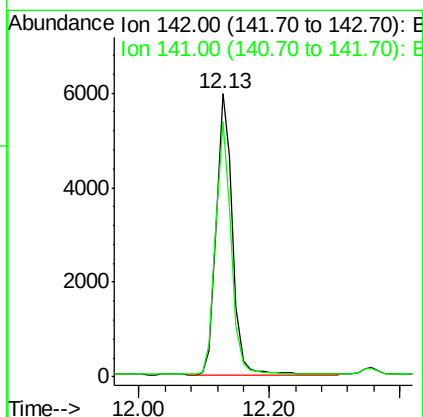
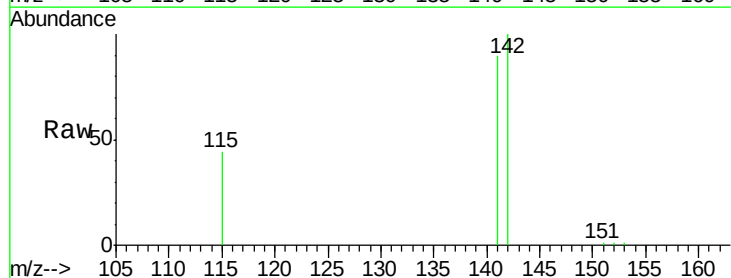


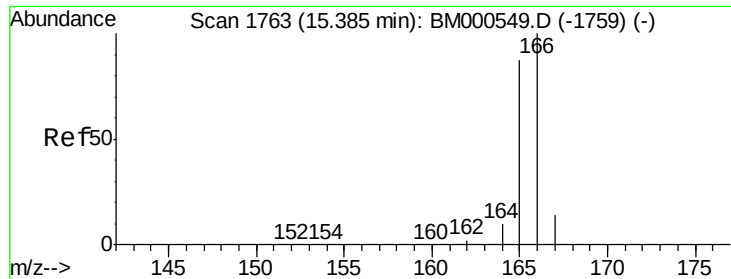

#9
 Fluorene
 Concen: 0.71 ng/ul
 RT: 15.39 min Scan# 1763
 Delta R.T. -0.00 min
 Lab File: BM000551.D
 Acq: 19 Feb 2015 12:13




Instrument :
 BNA_M
 ClientSampleId :


Tgt Ion:166 Resp: 16780
 Ion Ratio Lower Upper
 166 100
 165 86.4 72.3 108.5
 167 15.2 11.9 17.9

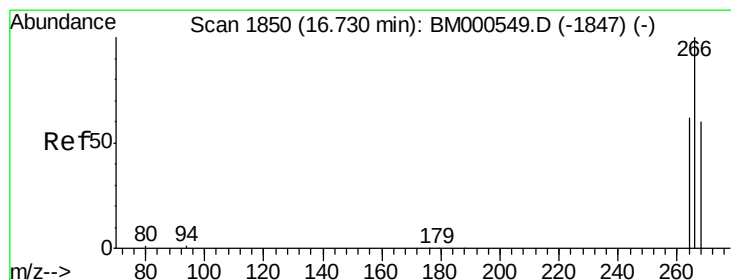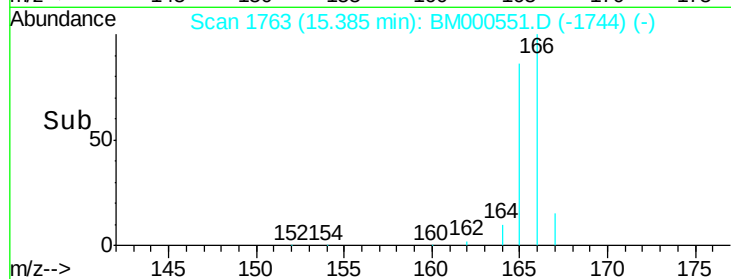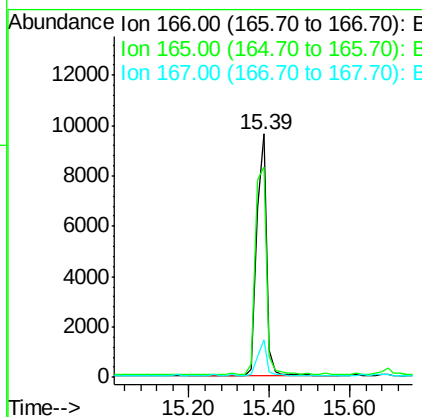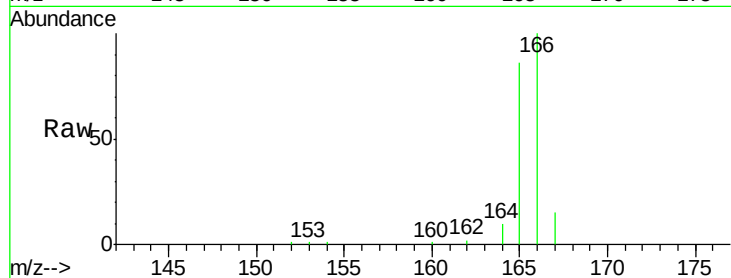

#11
 Pentachlorophenol
 Concen: 1.71 ng/ul
 RT: 16.73 min Scan# 1850
 Delta R.T. -0.00 min
 Lab File: BM000551.D
 Acq: 19 Feb 2015 12:13

Tgt Ion:266 Resp: 6020
 Ion Ratio Lower Upper
 266 100
 264 62.1 51.8 77.6
 268 64.6 55.4 83.0

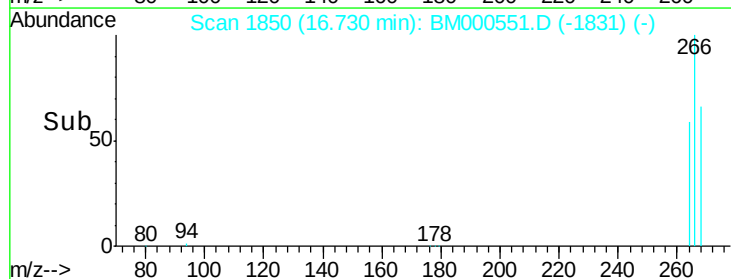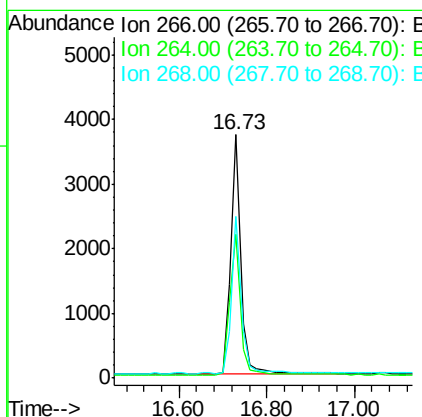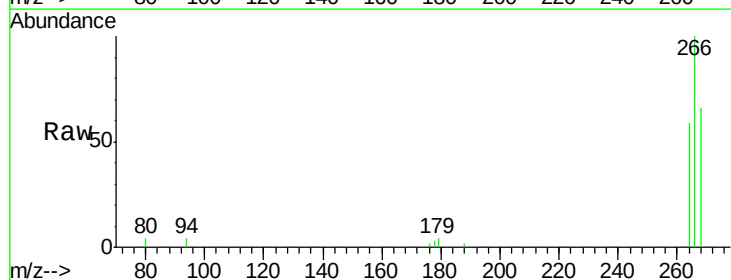

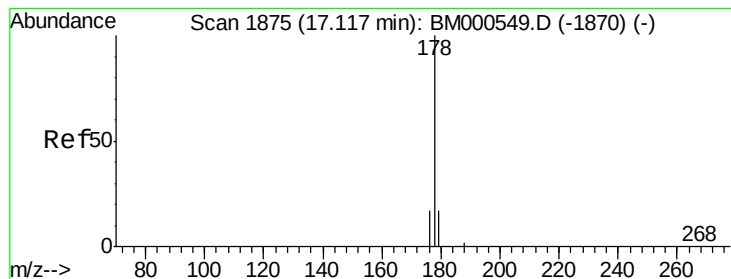

#12

Phenanthrene

Concen: 0.83 ng/ul

RT: 17.10 min Scan# 1874

Delta R.T. -0.02 min

Lab File: BM000551.D

Acq: 19 Feb 2015 12:13

Instrument :

BNA_M

ClientSampleId :


Tgt Ion:178 Resp: 29028

Ion Ratio Lower Upper

178 100

176 22.1 14.1 21.1#




179 14.3 14.4 21.6#

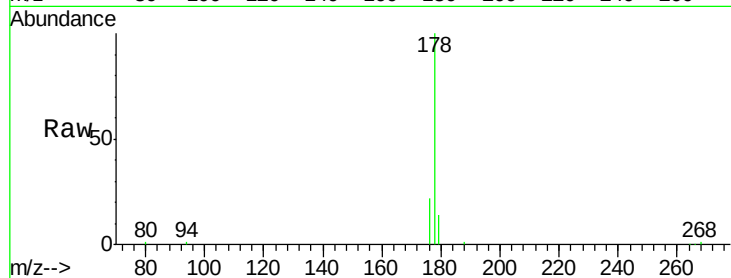

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

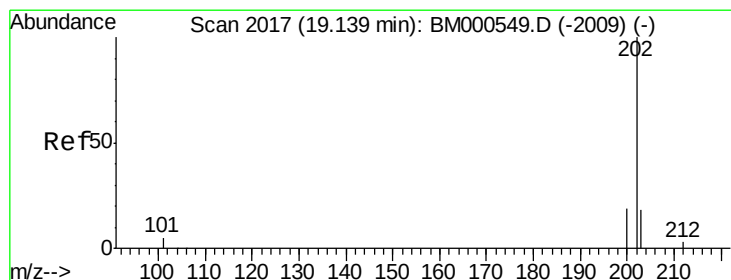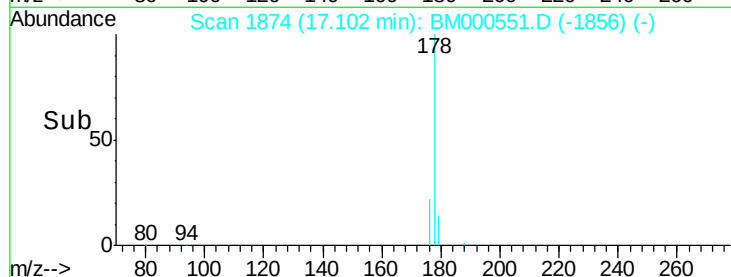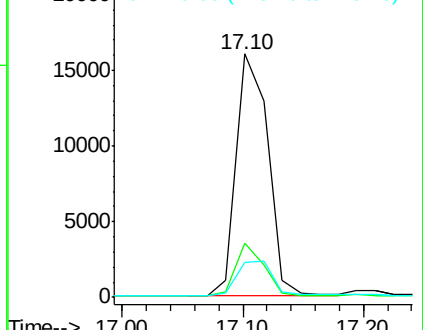

#15

Fluoranthene

Concen: 0.63 ng/ul

RT: 19.14 min Scan# 2017

Delta R.T. -0.00 min

Lab File: BM000551.D

Acq: 19 Feb 2015 12:13


Tgt Ion:202 Resp: 25250

Ion Ratio Lower Upper

202 100

101 5.8 0.0 25.4



203 19.8 0.0 38.6

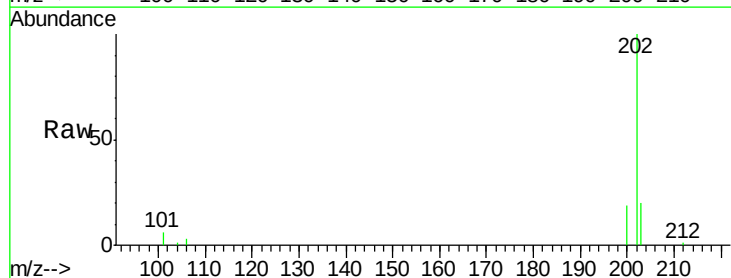


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

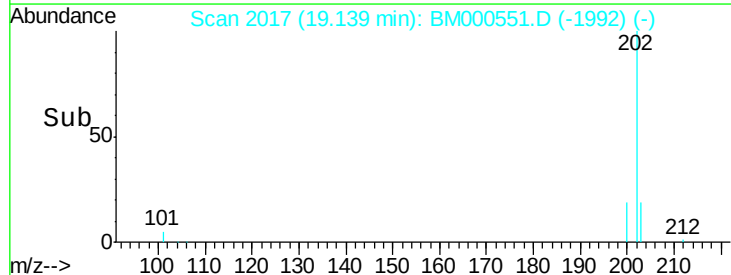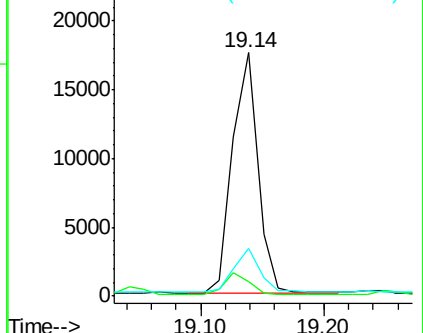

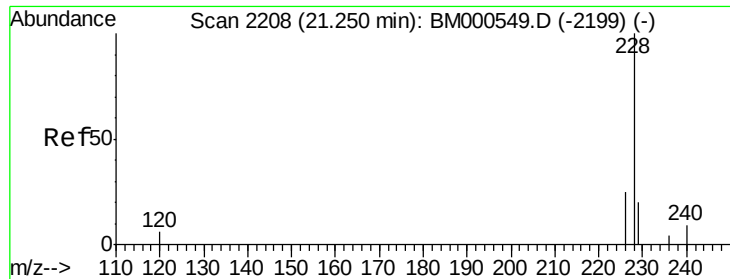

#18

Benzo(a)anthracene

Concen: 0.87 ng/ul

RT: 21.25 min Scan# 2208

Delta R.T. -0.00 min

Lab File: BM000551.D

Acq: 19 Feb 2015 12:13

Instrument :

BNA_M

ClientSampleId :


Tgt Ion:228 Resp: 22386

Ion Ratio Lower Upper

228 100

226 26.6 21.2 31.8




229 20.2 16.4 24.6

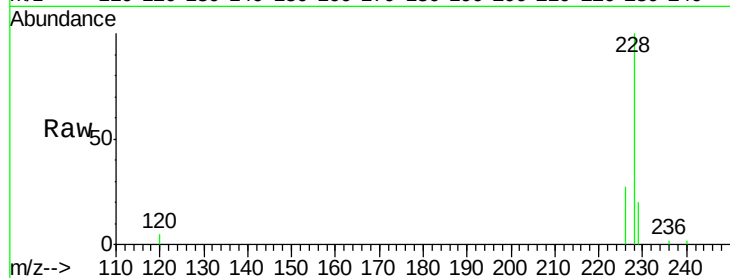

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

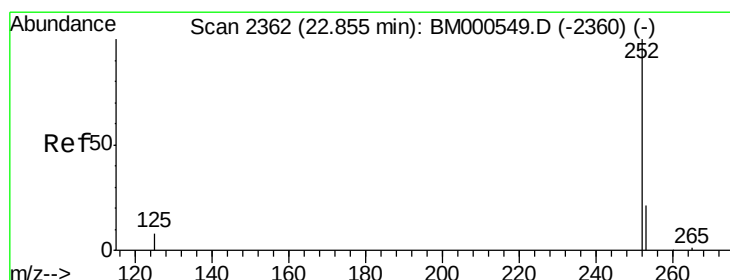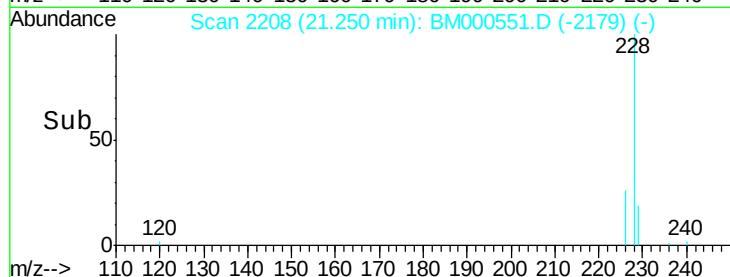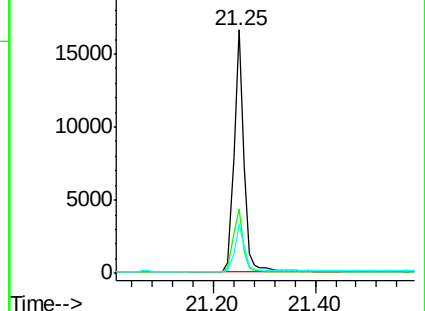

#22

Benzo(k)fluoranthene

Concen: 0.72 ng/ul

RT: 22.86 min Scan# 2362

Delta R.T. -0.00 min

Lab File: BM000551.D

Acq: 19 Feb 2015 12:13


Tgt Ion:252 Resp: 16594

Ion Ratio Lower Upper

252 100

253 29.0 29.2 43.8#



125 17.0 10.8 16.2#

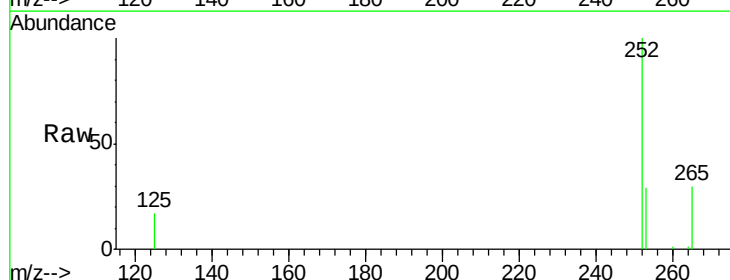


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

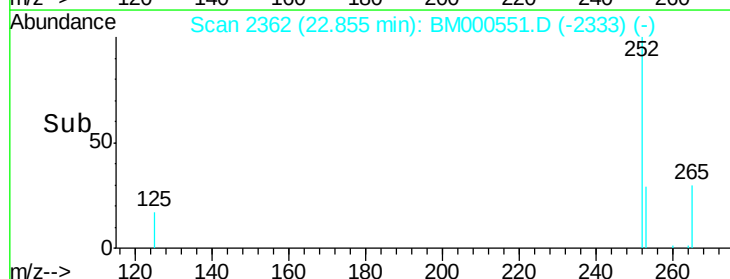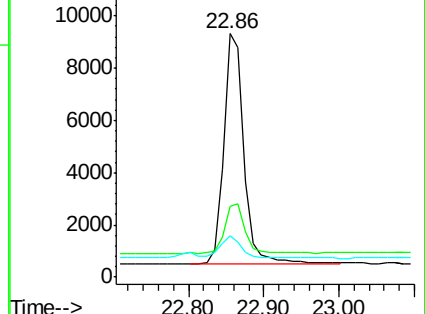

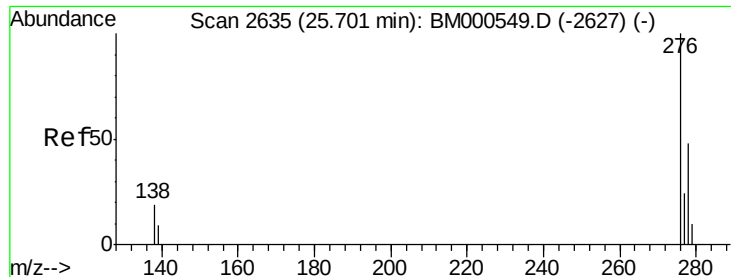

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.67 ng/ul

RT: 25.70 min Scan# 2635

Delta R.T. -0.01 min


Lab File: BM000551.D

Acq: 19 Feb 2015 12:13

Instrument :

BNA_M

ClientSampleId :

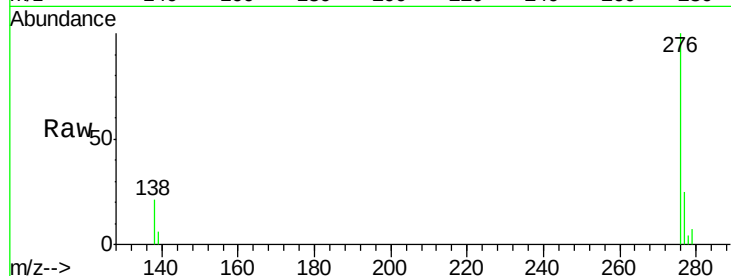




Tgt Ion:276 Resp: 13092

Ion Ratio Lower Upper

276 100

138 18.0 14.9 22.3

277 23.9 19.9 29.9

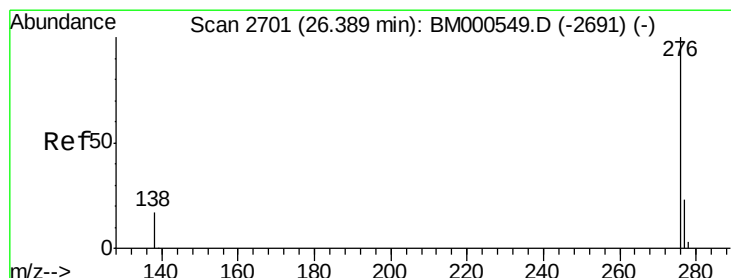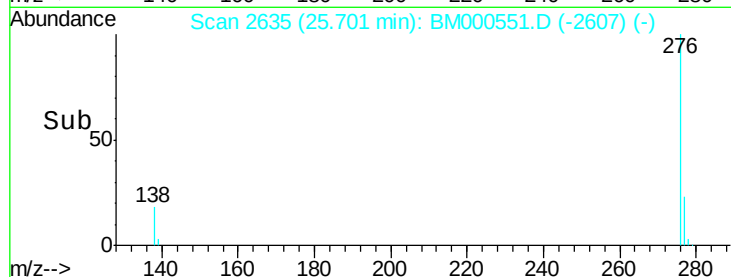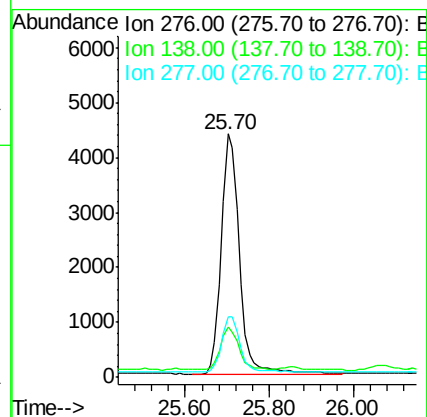

#26

Benzo(g,h,i)perylene

Concen: 1.16 ng/ul

RT: 26.39 min Scan# 2701

Delta R.T. -0.00 min

Lab File: BM000551.D

Acq: 19 Feb 2015 12:13

Tgt Ion:276 Resp: 19624

Ion Ratio Lower Upper

276 100

277 24.8 21.4 32.2

138 19.2 16.5 24.7

