


Data Path : Z:\HPCHEM1\BNA_M\Data\BM021915\
Data File : BM000548.D
Acq On : 19 Feb 2015 08:51
Operator : TP/IZ
Sample : DFTPP26
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP26

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM021815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 19 17:40:46 2015

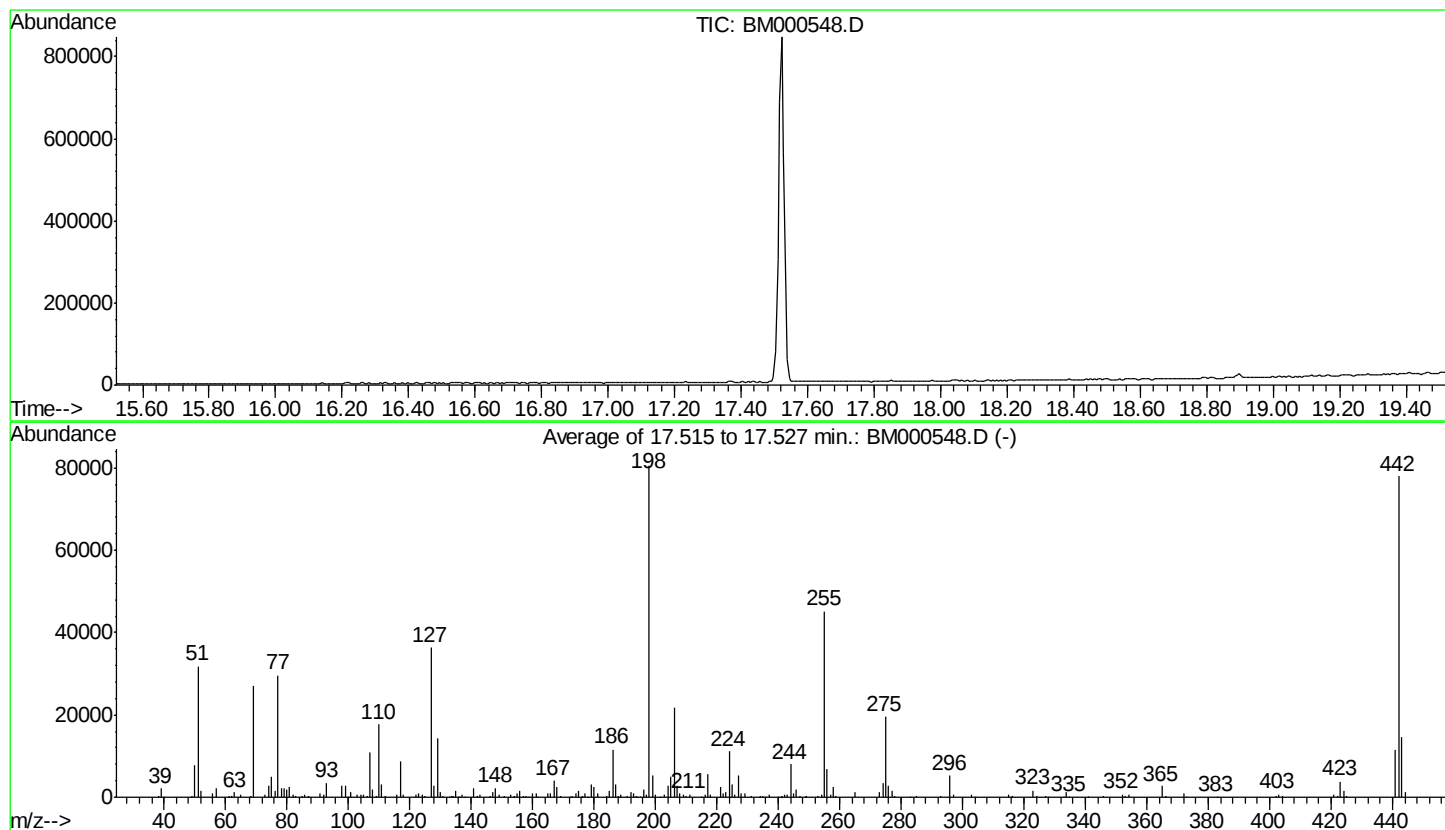

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	31808	PASS
68	69	0.00	2	1.6	442	PASS
69	198	0.00	100	33.4	26946	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.0	36269	PASS
197	198	0.00	2	0.8	629	PASS
198	198	100	100	100.0	80560	PASS
199	198	5	9	6.5	5266	PASS
275	198	10	60	24.3	19556	PASS
365	198	1	100	3.4	2713	PASS
441	443	0.01	100	78.6	11441	PASS
442	198	50	100	96.8	78005	PASS
443	442	15	24	18.7	14562	PASS

m/z	Abundance
38.10	351.0
39.10	2460.0
40.00	646.0
44.00	2104.0
49.10	498.0
50.10	9645.0
51.10	36784.0
52.10	2071.0
56.00	1191.0
57.00	2251.0
61.10	444.0
62.00	436.0
63.10	1066.0
65.20	592.0
68.20	609.0
69.00	29720.0
73.10	879.0
74.00	3163.0
75.10	4955.0
76.10	1589.0
77.10	33048.0
78.10	2907.0
79.00	2349.0
80.10	2237.0
81.00	2876.0
81.90	883.0
83.10	655.0
85.00	352.0
85.90	868.0
87.00	531.0
91.00	719.0
91.90	778.0
93.00	3409.0
98.00	3112.0
99.00	3648.0
101.10	1629.0
103.00	668.0
103.90	836.0
105.10	944.0
106.10	505.0
107.10	11876.0
108.00	2265.0
109.10	429.0
110.00	18680.0
111.00	3573.0
111.90	395.0
116.10	901.0
117.00	10054.0
118.00	834.0
121.90	888.0
123.00	1085.0
124.00	709.0
125.00	491.0
127.00	37376.0
128.00	2872.0
129.00	14582.0
130.00	1458.0
131.00	541.0
134.10	403.0
135.00	1501.0
135.90	316.0
137.00	916.0
137.90	319.0
141.00	2600.0
141.90	543.0
143.10	687.0
146.10	312.0
147.00	1429.0
148.00	2776.0
149.00	698.0
151.00	464.0
153.00	707.0
153.80	419.0
154.20	394.0
154.90	920.0
156.00	2013.0
157.00	552.0
160.00	912.0
161.10	766.0
165.00	780.0
166.00	864.0
167.00	4370.0
168.10	2507.0
169.10	396.0
172.10	376.0
173.00	451.0
174.00	941.0
175.10	1563.0
176.00	456.0
177.00	778.0
179.00	3481.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

180.00	2668.0
181.10	1098.0
184.00	327.0
185.00	1687.0
186.10	10898.0
187.00	2962.0
188.00	457.0
188.90	639.0
191.10	470.0
191.90	1212.0
193.00	1091.0
193.90	387.0
196.00	1860.0
197.10	562.0
198.00	78792.0
199.00	5591.0
199.90	473.0
201.60	405.0
202.90	399.0
204.00	2839.0
205.10	4927.0
206.10	21552.0
207.10	5093.0
208.00	1126.0
209.10	597.0
210.00	447.0
211.20	592.0
216.10	659.0
217.00	5748.0
218.00	732.0
221.10	2405.0
222.00	980.0
223.10	1604.0
224.10	10201.0
225.00	2724.0
226.00	646.0
227.00	5547.0
228.00	1144.0
229.00	1242.0
231.10	427.0
234.90	354.0
237.00	702.0
241.20	318.0
242.10	441.0
243.20	534.0
244.10	7054.0
245.10	896.0
246.00	1431.0
247.00	336.0
248.90	444.0
253.00	363.0
254.10	630.0
255.00	41312.0
256.00	6197.0
257.00	819.0
258.00	2465.0
258.90	531.0
265.00	985.0
273.10	870.0
274.00	2743.0
275.00	18728.0
276.00	2834.0
277.00	1299.0
281.10	494.0
292.90	395.0
296.00	4868.0
297.10	549.0
303.10	442.0
315.00	624.0
315.90	463.0
323.10	1346.0
333.00	391.0
333.90	946.0
340.80	312.0
352.10	577.0
352.90	544.0
353.90	507.0
365.00	2305.0
365.80	309.0
372.00	775.0
382.90	368.0
402.90	558.0
421.10	469.0
422.10	398.0
423.00	3011.0
424.10	1647.0
425.00	363.0
441.10	8390.0
442.10	59304.0
443.00	10848.0
444.10	1149.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

m/z	Abundance
38.10	616.0
39.10	2541.0
40.00	502.0
44.00	2532.0
49.10	356.0
50.10	8694.0
51.10	36472.0
52.00	1441.0
56.00	1086.0
57.00	2399.0
61.10	479.0
62.10	502.0
63.00	1542.0
65.00	873.0
68.10	388.0
69.00	31696.0
73.10	1312.0
74.10	3470.0
75.00	6273.0
76.10	1914.0
77.10	35472.0
78.10	2858.0
79.00	2463.0
79.90	2122.0
81.00	2549.0
81.90	352.0
82.10	373.0
83.00	704.0
85.00	707.0
86.00	866.0
87.20	443.0
91.00	1092.0
92.00	899.0
93.00	4556.0
98.00	3315.0
99.00	2875.0
99.90	391.0
101.00	1530.0
102.90	575.0
104.00	738.0
105.00	769.0
106.10	484.0
107.00	12727.0
108.10	2163.0
109.00	408.0
110.00	21216.0
111.00	3635.0
112.10	455.0
115.90	943.0
117.00	10397.0
117.90	819.0
122.00	852.0
123.00	1267.0
124.00	559.0
124.80	459.0
127.00	44192.0
128.00	3153.0
129.00	18656.0
130.00	1334.0
130.90	334.0
132.90	304.0
133.80	571.0
135.00	1876.0
136.10	424.0
137.10	817.0
141.00	2231.0
142.10	1182.0
143.10	474.0
147.10	1633.0
148.00	2525.0
149.00	630.0
150.90	439.0
153.10	605.0
154.00	820.0
155.00	1204.0
156.00	1735.0
158.10	472.0
158.90	339.0
159.90	952.0
161.00	1083.0
161.80	448.0
165.00	1052.0
165.90	1169.0
167.10	4870.0
167.90	2920.0
169.10	375.0
172.90	598.0
174.00	954.0
175.10	1822.0
176.30	386.0
177.00	1271.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

177.90	320.0
179.00	3859.0
180.00	2903.0
181.10	1371.0
184.10	385.0
185.00	1904.0
186.00	14037.0
187.10	4230.0
188.20	486.0
188.90	806.0
191.00	617.0
191.90	1524.0
193.00	1570.0
193.90	440.0
195.10	386.0
196.10	1976.0
197.10	688.0
198.00	98104.0
199.00	5786.0
200.00	595.0
202.90	753.0
204.00	3748.0
205.00	6229.0
206.10	26384.0
207.10	6174.0
207.90	1259.0
209.00	686.0
210.10	436.0
211.00	946.0
214.90	428.0
216.10	442.0
217.00	6370.0
218.10	930.0
221.00	3150.0
222.00	910.0
223.00	1487.0
224.10	13359.0
225.10	4587.0
226.00	574.0
227.00	6416.0
228.00	1041.0
229.00	1069.0
231.10	588.0
234.00	495.0
235.00	302.0
236.00	315.0
237.00	901.0
240.00	302.0
240.90	438.0
241.20	438.0
242.10	656.0
243.00	558.0
244.10	10427.0
245.00	1163.0
246.00	2330.0
247.00	424.0
249.10	377.0
253.00	330.0
254.10	671.0
255.10	55536.0
256.00	8150.0
256.90	715.0
258.00	2427.0
258.80	669.0
265.00	1387.0
273.10	1527.0
274.00	4615.0
275.00	24016.0
276.00	3568.0
277.00	2593.0
278.00	556.0
281.00	606.0
283.00	401.0
284.90	587.0
293.00	343.0
296.00	5692.0
296.90	907.0
303.00	814.0
304.00	336.0
314.90	953.0
316.10	525.0
323.00	1923.0
324.10	419.0
327.00	468.0
328.00	366.0
334.00	1540.0
334.80	371.0
341.00	422.0
346.00	637.0
352.00	934.0
352.90	501.0
354.00	685.0
365.00	3438.0
366.10	567.0
372.00	1050.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

373.10	485.0
402.10	410.0
403.00	1057.0
404.00	551.0
420.90	680.0
422.00	551.0
423.10	4343.0
424.10	1755.0
424.90	503.0
441.00	13598.0
442.10	94120.0
443.10	17104.0
444.10	1541.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

m/z	Abundance
39.10	1390.0
40.00	374.0
44.00	2543.0
50.10	5363.0
51.10	22168.0
52.10	1032.0
56.00	571.0
57.00	1614.0
60.90	389.0
63.00	1048.0
65.00	410.0
68.00	330.0
69.00	19424.0
73.10	1021.0
74.00	2001.0
75.00	3431.0
76.00	1240.0
77.10	20240.0
78.00	1131.0
79.00	1443.0
79.90	1291.0
81.00	1816.0
81.90	376.0
85.90	431.0
90.90	662.0
92.00	595.0
93.10	2630.0
98.00	2225.0
99.00	2277.0
100.90	864.0
103.00	327.0
103.90	633.0
104.90	596.0
107.00	7698.0
108.00	1155.0
110.00	13183.0
111.00	1925.0
112.00	362.0
117.00	5469.0
118.10	522.0
121.80	465.0
123.10	569.0
124.00	433.0
127.00	27240.0
128.00	2469.0
129.00	9837.0
130.00	1063.0
134.10	490.0
134.90	994.0
137.10	499.0
141.00	1387.0
141.90	414.0
143.10	404.0
146.00	330.0
147.00	987.0
148.10	1460.0
149.10	586.0
153.10	468.0
155.10	673.0
156.00	1337.0
158.00	350.0
160.00	693.0
161.00	746.0
165.10	548.0
166.10	572.0
167.00	2739.0
168.00	1778.0
169.10	324.0
174.00	558.0
175.10	1275.0
176.10	383.0
176.90	967.0
179.00	2203.0
180.00	1688.0
181.00	719.0
184.90	848.0
186.00	9850.0
187.00	2441.0
188.00	438.0
188.90	670.0
191.10	506.0
192.00	1082.0
193.00	1025.0
194.10	309.0
196.10	1486.0
197.10	638.0
198.00	64784.0
199.00	4423.0
200.00	442.0
203.00	300.0
204.00	2050.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

205.00	3980.0
206.10	17856.0
207.00	4222.0
208.10	1475.0
209.10	511.0
210.00	332.0
211.00	646.0
216.10	412.0
217.10	4642.0
218.10	359.0
221.00	2082.0
222.10	501.0
223.00	912.0
224.00	9785.0
225.10	2366.0
226.10	348.0
227.00	4148.0
227.90	648.0
229.00	834.0
231.00	352.0
234.00	314.0
236.80	362.0
237.20	375.0
242.10	517.0
243.10	756.0
244.10	6560.0
245.00	1028.0
245.90	1643.0
246.90	368.0
249.10	476.0
254.00	440.0
255.00	38648.0
256.00	5881.0
257.00	537.0
258.00	2278.0
265.00	1263.0
273.00	1606.0
274.00	2670.0
275.00	15926.0
276.00	2056.0
277.00	1227.0
281.10	475.0
284.90	404.0
293.10	346.0
296.00	5105.0
296.90	846.0
303.00	591.0
314.90	568.0
323.10	1486.0
324.00	338.0
327.00	351.0
333.90	945.0
346.10	508.0
352.00	620.0
352.90	349.0
354.10	734.0
365.00	2397.0
372.10	921.0
401.90	380.0
402.90	705.0
421.00	479.0
422.00	478.0
423.10	4270.0
424.00	1638.0
425.10	375.0
441.00	12337.0
442.00	80592.0
443.00	15736.0
444.00	1313.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

Scan 2515 (17.480 min): BM000548.D
DFTPP26

m/z	Abundance
39.90	411.0
44.00	2507.0
73.00	528.0
191.00	332.0
192.90	313.0
207.10	2474.0
208.00	314.0
281.10	602.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26