

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
 Data File : BM004286.D
 Acq On : 19 Feb 2016 14:55
 Operator : SJ/UM
 Sample : H1497-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-SS15A

Quant Time: Feb 19 23:34:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 19 23:29:57 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	21342	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	109233	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	72934	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	177601	20.00	ng/ul	0.00
78) Chrysene-d12	21.26	240	213235	20.00	ng/ul	0.00
86) Perylene-d12	23.48	264	206486	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	1925	4.54	ng/uL	0.00
5) Phenol-d5	6.82	99	49762	29.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	27746	29.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	44399	29.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	46833	32.07	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	23865	28.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	28231	30.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	46852	27.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	71446	35.45	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	194890	32.11	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	222345	30.15	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	30237	30.79	ng/ul	0.00
58) Fluorene-d10	15.29	176	165876	32.43	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	26456	24.46	ng/ul	0.00
71) Anthracene-d10	17.14	188	272147	31.34	ng/ul	0.00
79) Pyrene-d10	19.45	212	326351	28.83	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.34	264	348964	31.67	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.75	163	67471	10.64	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
Data File : BM004286.D
Acq On : 19 Feb 2016 14:55
Operator : SJ/UM
Sample : H1497-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-SS15A

Quant Time: Feb 19 23:34:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 19 23:29:57 2016
Response via : Initial Calibration

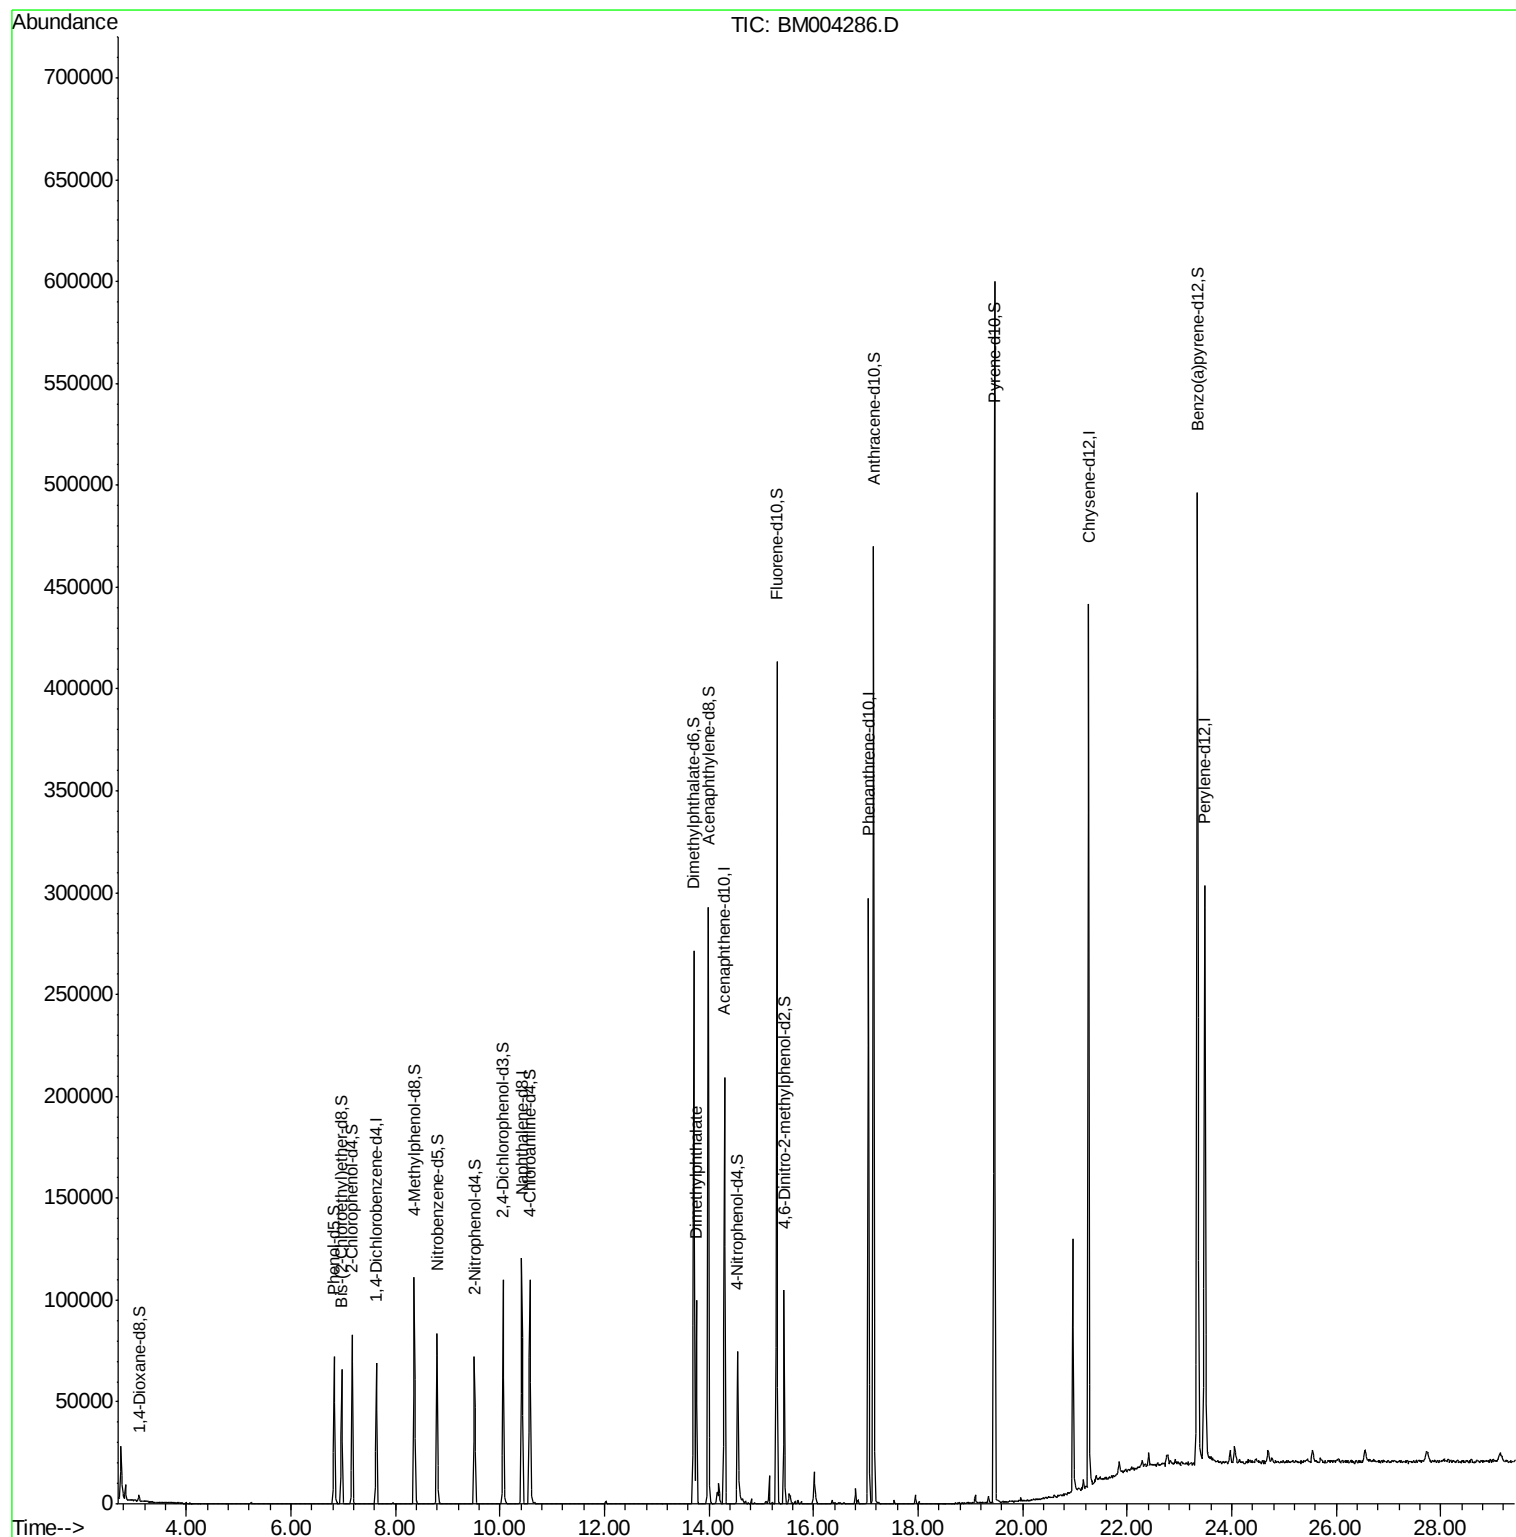

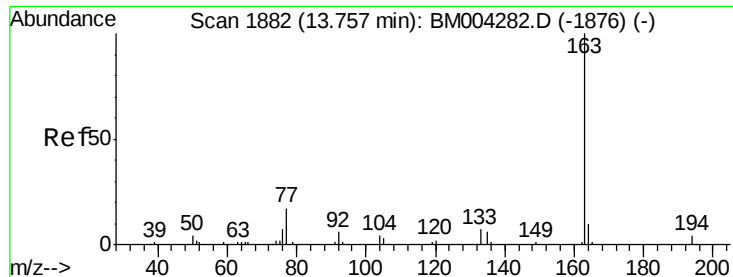

#45

Dimethylphthalate

Concen: 10.64 ng/ul

RT: 13.75 min Scan# 1881

Delta R.T. -0.01 min

Lab File: BM004286.D

Acq: 19 Feb 2016 14:55

Instrument :

BNA_M

ClientSampleId :

0311-SS15A

Tgt Ion:163 Resp: 67471

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 9.9 7.8 11.8

