

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
 Data File : BM004287.D
 Acq On : 19 Feb 2016 15:31
 Operator : SJ/UM
 Sample : H1497-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-SS15B

Quant Time: Feb 19 23:34:20 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 19 23:29:57 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	22141	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	111067	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	73357	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	178474	20.00	ng/ul	0.00
78) Chrysene-d12	21.26	240	214821	20.00	ng/ul	0.00
86) Perylene-d12	23.48	264	207483	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	1990	4.53	ng/uL	0.00
5) Phenol-d5	6.82	99	49196	27.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	27747	28.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	43978	27.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	47244	31.19	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	23602	27.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	27420	28.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	46079	26.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	71292	34.79	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	194400	31.85	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	219411	29.58	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	28951	29.31	ng/ul	0.00
58) Fluorene-d10	15.29	176	163307	31.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	25102	23.10	ng/ul	0.00
71) Anthracene-d10	17.14	188	271194	31.08	ng/ul	0.00
79) Pyrene-d10	19.45	212	319611	28.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.34	264	337896	30.52	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.75	163	65551	10.28	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
Data File : BM004287.D
Acq On : 19 Feb 2016 15:31
Operator : SJ/UM
Sample : H1497-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-SS15B

Quant Time: Feb 19 23:34:20 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 19 23:29:57 2016
Response via : Initial Calibration

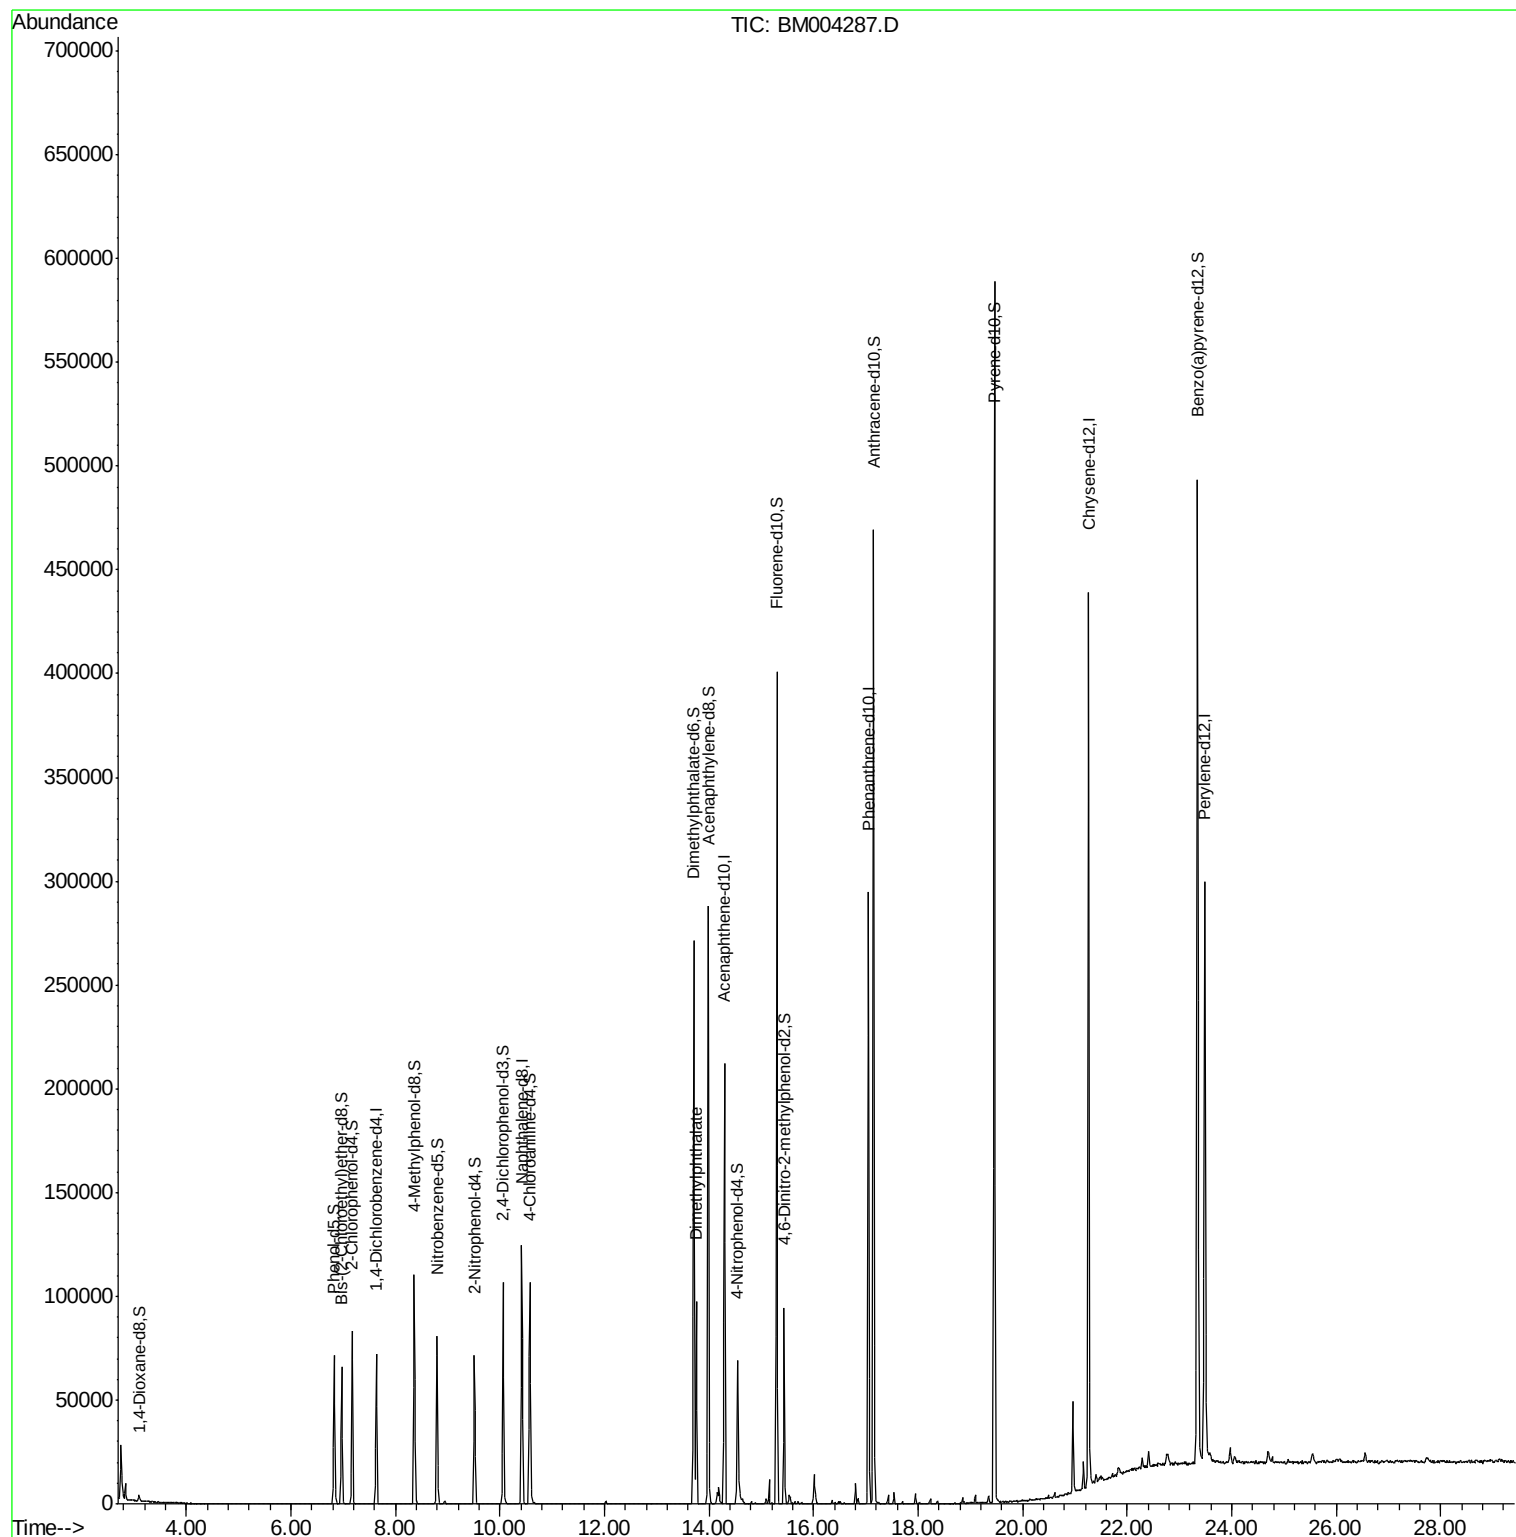

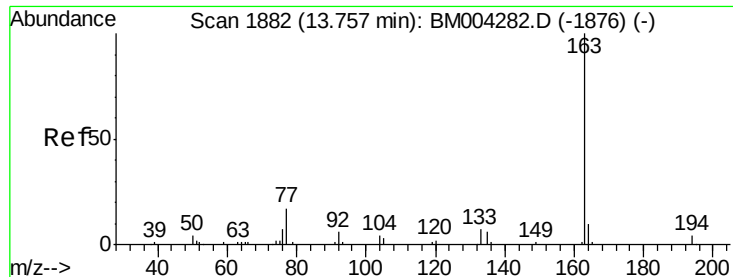

#45

Dimethylphthalate

Concen: 10.28 ng/ul

RT: 13.75 min Scan# 1881

Delta R.T. -0.01 min

Lab File: BM004287.D

Acq: 19 Feb 2016 15:31

Instrument :

BNA_M

ClientSampleId :

0311-SS15B


Tgt Ion:163 Resp: 65551

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 10.2 7.8 11.8

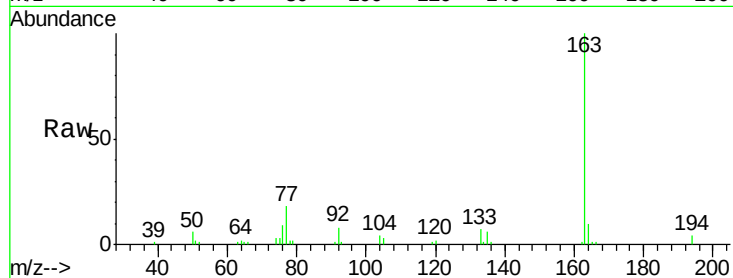

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

