

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
 Data File : BM004290.D
 Acq On : 19 Feb 2016 18:15
 Operator : SJ/UM
 Sample : H1497-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-SS32C

Quant Time: Feb 19 23:55:56 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 19 23:51:45 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	22568	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	110812	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	72328	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	177306	20.00	ng/ul	0.00
78) Chrysene-d12	21.26	240	210840	20.00	ng/ul	0.00
86) Perylene-d12	23.48	264	205765	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	2685	5.99	ng/uL	0.00
5) Phenol-d5	6.82	99	58507	32.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	33500	34.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	53241	33.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	55453	35.91	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	27960	32.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	32549	34.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	54024	31.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	82702	40.45	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	221920	36.87	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	253910	34.72	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	30611	31.44	ng/ul	0.00
58) Fluorene-d10	15.29	176	186541	36.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	27617	25.58	ng/ul	0.00
71) Anthracene-d10	17.14	188	305894	35.29	ng/ul	0.00
79) Pyrene-d10	19.45	212	361011	32.26	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.34	264	379730	34.58	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.75	163	71418	11.36	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
Data File : BM004290.D
Acq On : 19 Feb 2016 18:15
Operator : SJ/UM
Sample : H1497-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-SS32C

Quant Time: Feb 19 23:55:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 19 23:51:45 2016
Response via : Initial Calibration

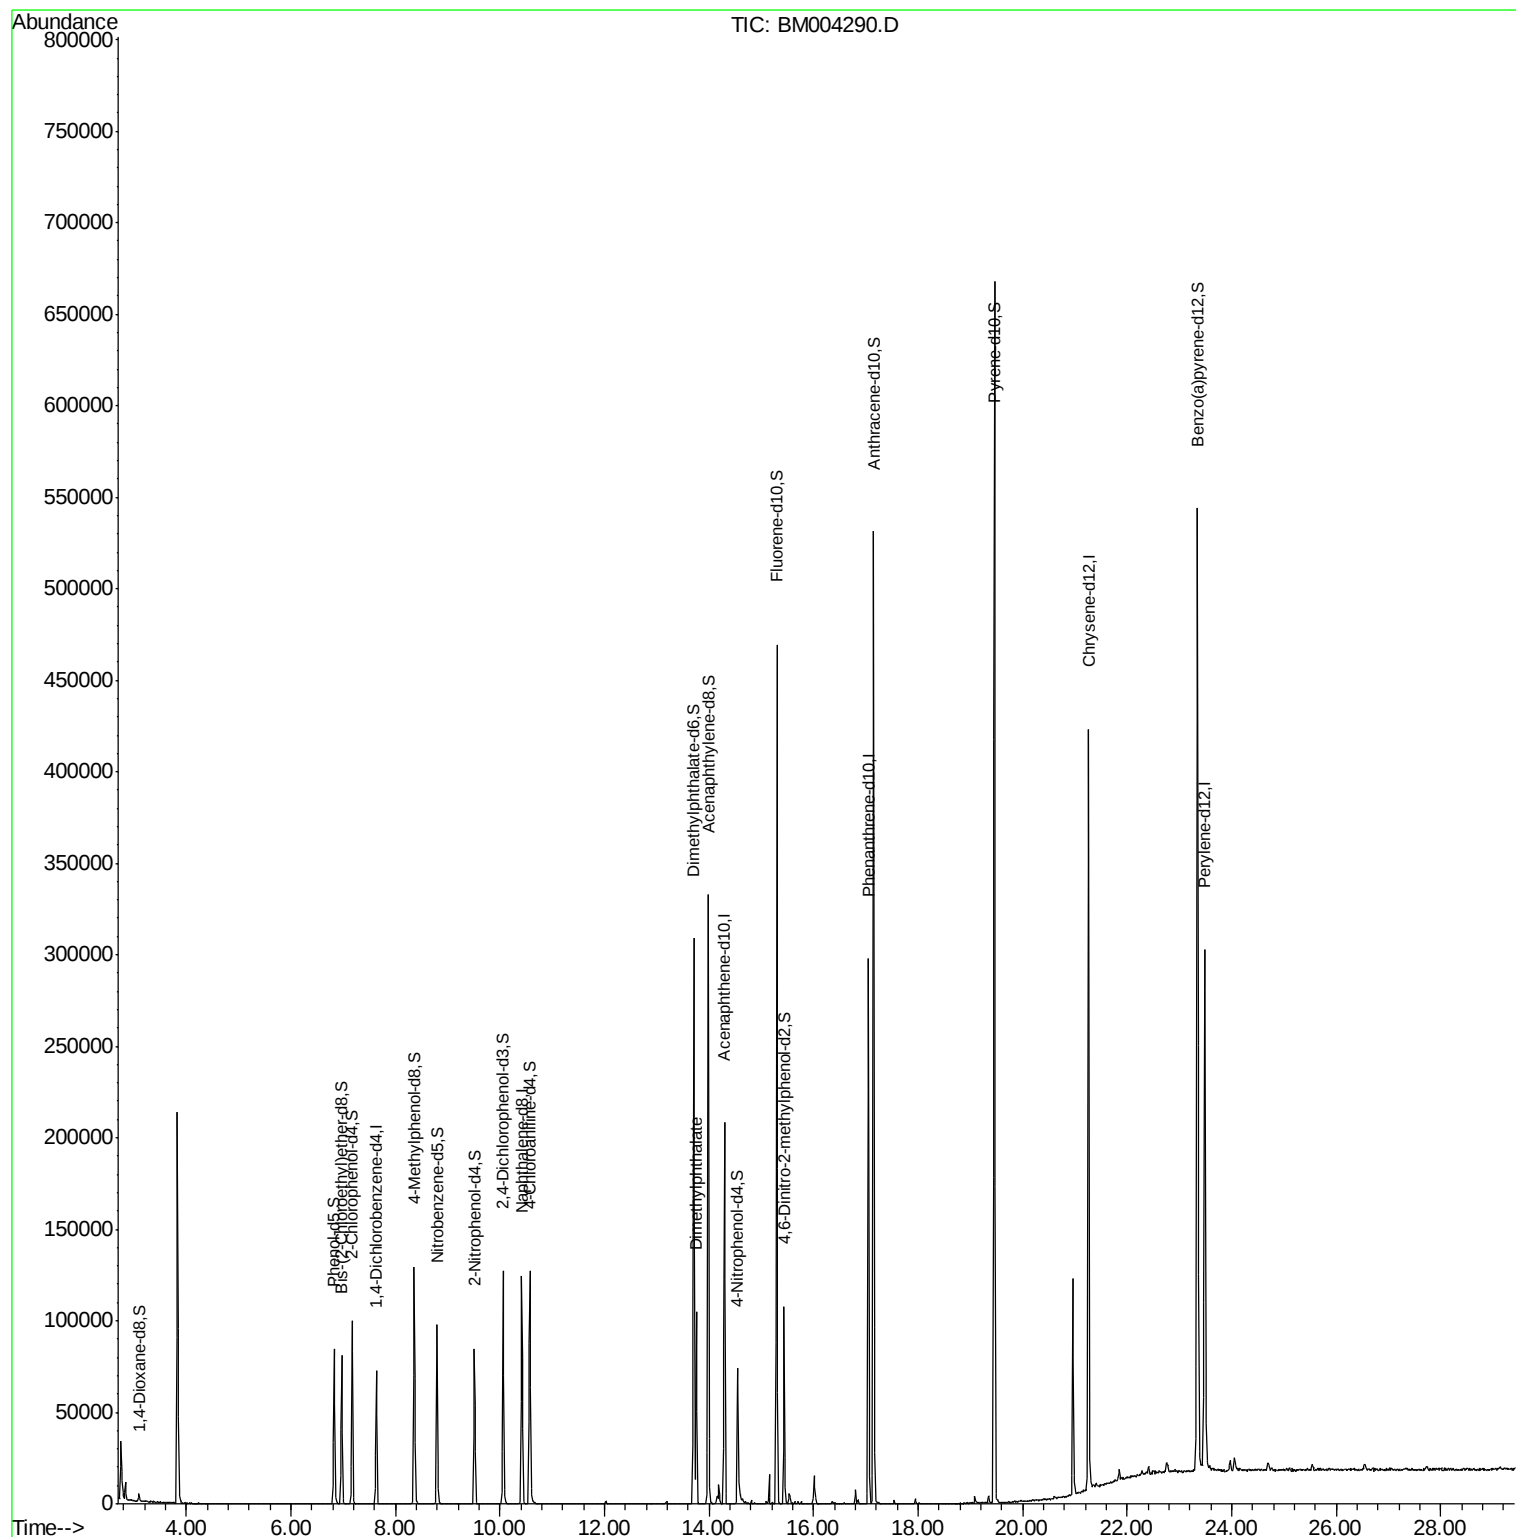

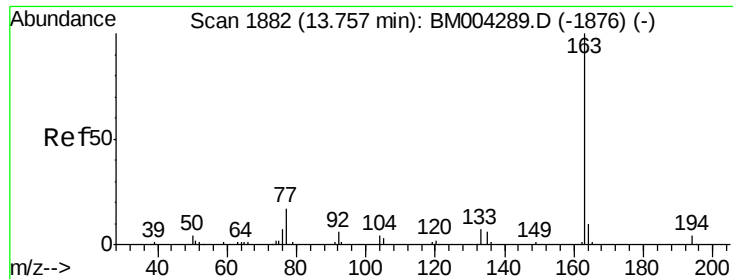

#45

Dimethylphthalate

Concen: 11.36 ng/ul

RT: 13.75 min Scan# 1881

Delta R.T. -0.01 min

Lab File: BM004290.D

Acq: 19 Feb 2016 18:15

Instrument :

BNA_M

ClientSampleId :

0311-SS32C



Tgt Ion:163 Resp: 71418

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.0 7.8 11.8

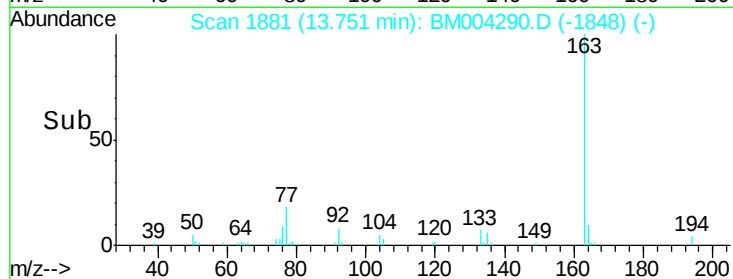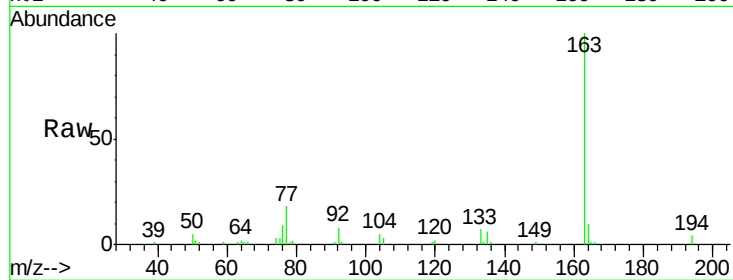

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

