

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
 Data File : BM004302.D
 Acq On : 20 Feb 2016 01:29
 Operator : SJ/UM
 Sample : H1497-22
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S08-0312

Quant Time: Feb 20 05:54:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 19 23:51:45 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	23486	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	121441	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	82442	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	201506	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	242404	20.00	ng/ul	0.00
86) Perylene-d12	23.48	264	236748	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	2129	4.57	ng/uL	0.00
5) Phenol-d5	6.82	99	54873	29.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	30724	30.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	48836	29.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	52901	32.92	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	26219	28.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	30424	29.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	52209	27.74	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	82477	36.81	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	216551	31.56	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	252693	30.32	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	33825	30.48	ng/ul	0.00
58) Fluorene-d10	15.29	176	187195	32.37	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	30130	24.55	ng/ul	0.00
71) Anthracene-d10	17.15	188	305131	30.97	ng/ul	0.00
79) Pyrene-d10	19.45	212	365021	28.37	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.34	264	389725	30.85	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.75	163	65914	9.20	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
Data File : BM004302.D
Acq On : 20 Feb 2016 01:29
Operator : SJ/UM
Sample : H1497-22
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S08-0312

Quant Time: Feb 20 05:54:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 19 23:51:45 2016
Response via : Initial Calibration

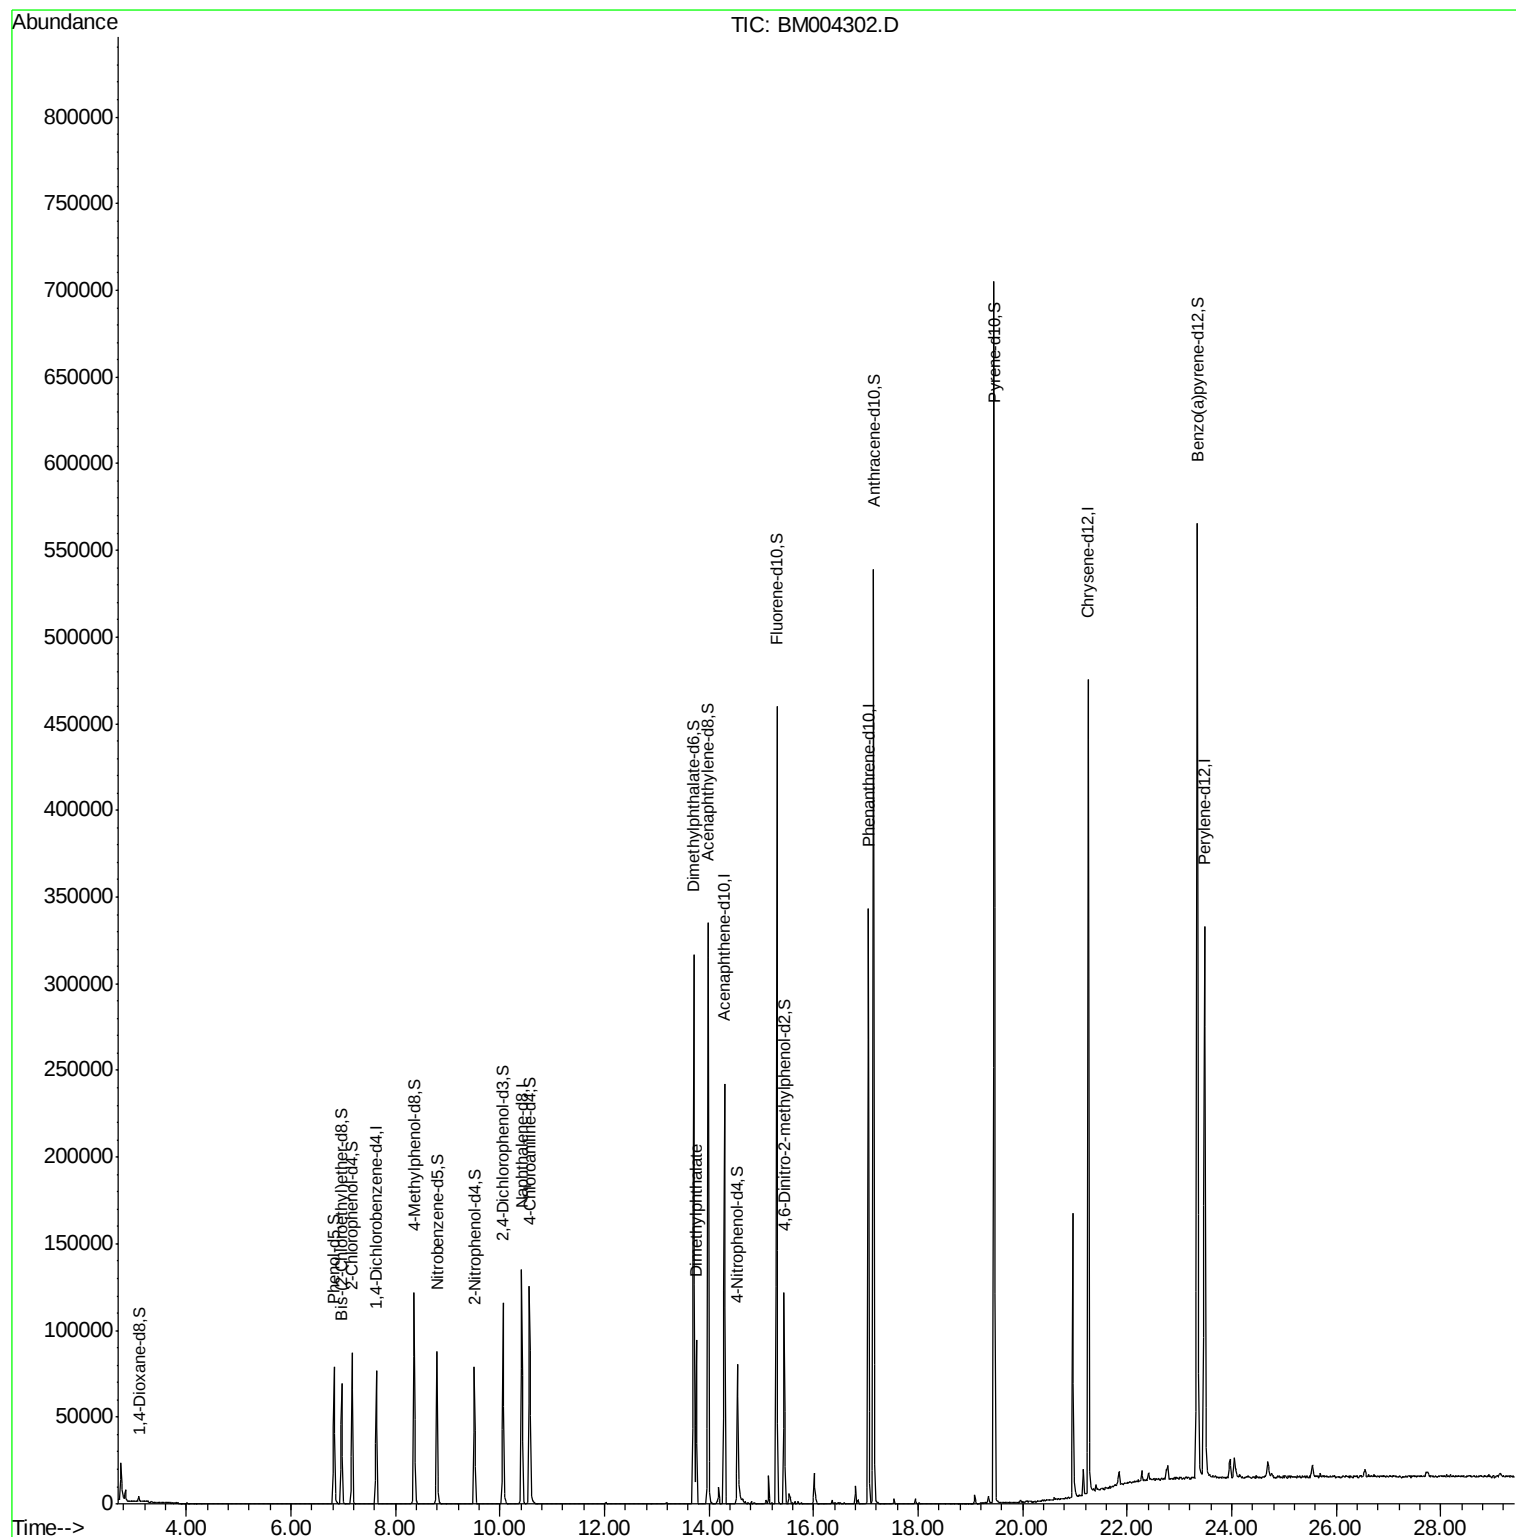

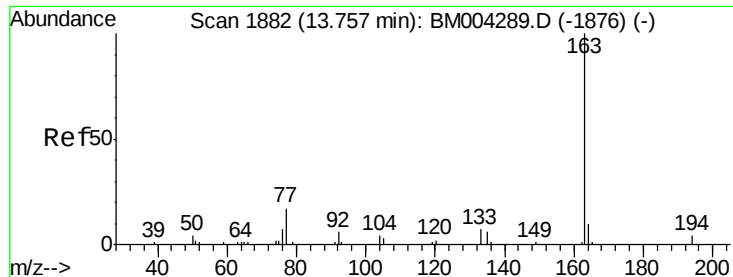

#45

Dimethylphthalate

Concen: 9.20 ng/ul

RT: 13.75 min Scan# 1881

Delta R.T. -0.01 min

Lab File: BM004302.D

Acq: 20 Feb 2016 01:29

Instrument :

BNA_M

ClientSampleId :

0311-S08-0312


Tgt Ion:163 Resp: 65914

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.2 7.8 11.8

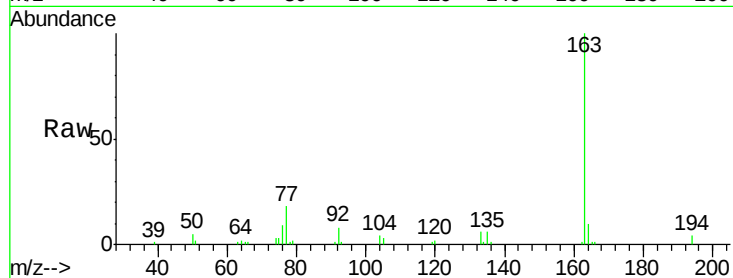

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

