

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
 Data File : BM004304.D
 Acq On : 20 Feb 2016 03:31
 Operator : SJ/UM
 Sample : H1497-12
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-SS34A

Quant Time: Feb 20 06:05:50 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 20 06:01:29 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	27807	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	146110	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	100736	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	245428	20.00	ng/ul	0.00
78) Chrysene-d12	21.26	240	286052	20.00	ng/ul	0.00
86) Perylene-d12	23.48	264	275236	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	1962	3.55	ng/uL	0.00
5) Phenol-d5	6.82	99	54439	24.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	30774	25.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	47538	24.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	53585	28.16	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	26743	23.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	31393	25.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	54221	23.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	86561	32.11	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	247985	29.58	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	278697	27.36	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	39433	29.08	ng/ul	0.00
58) Fluorene-d10	15.29	176	212891	30.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	37243	24.92	ng/ul	0.00
71) Anthracene-d10	17.15	188	362050	30.17	ng/ul	0.00
79) Pyrene-d10	19.46	212	428571	28.23	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.34	264	448200	30.52	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.75	163	96844	11.06	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
Data File : BM004304.D
Acq On : 20 Feb 2016 03:31
Operator : SJ/UM
Sample : H1497-12
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-SS34A

Quant Time: Feb 20 06:05:50 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 20 06:01:29 2016
Response via : Initial Calibration

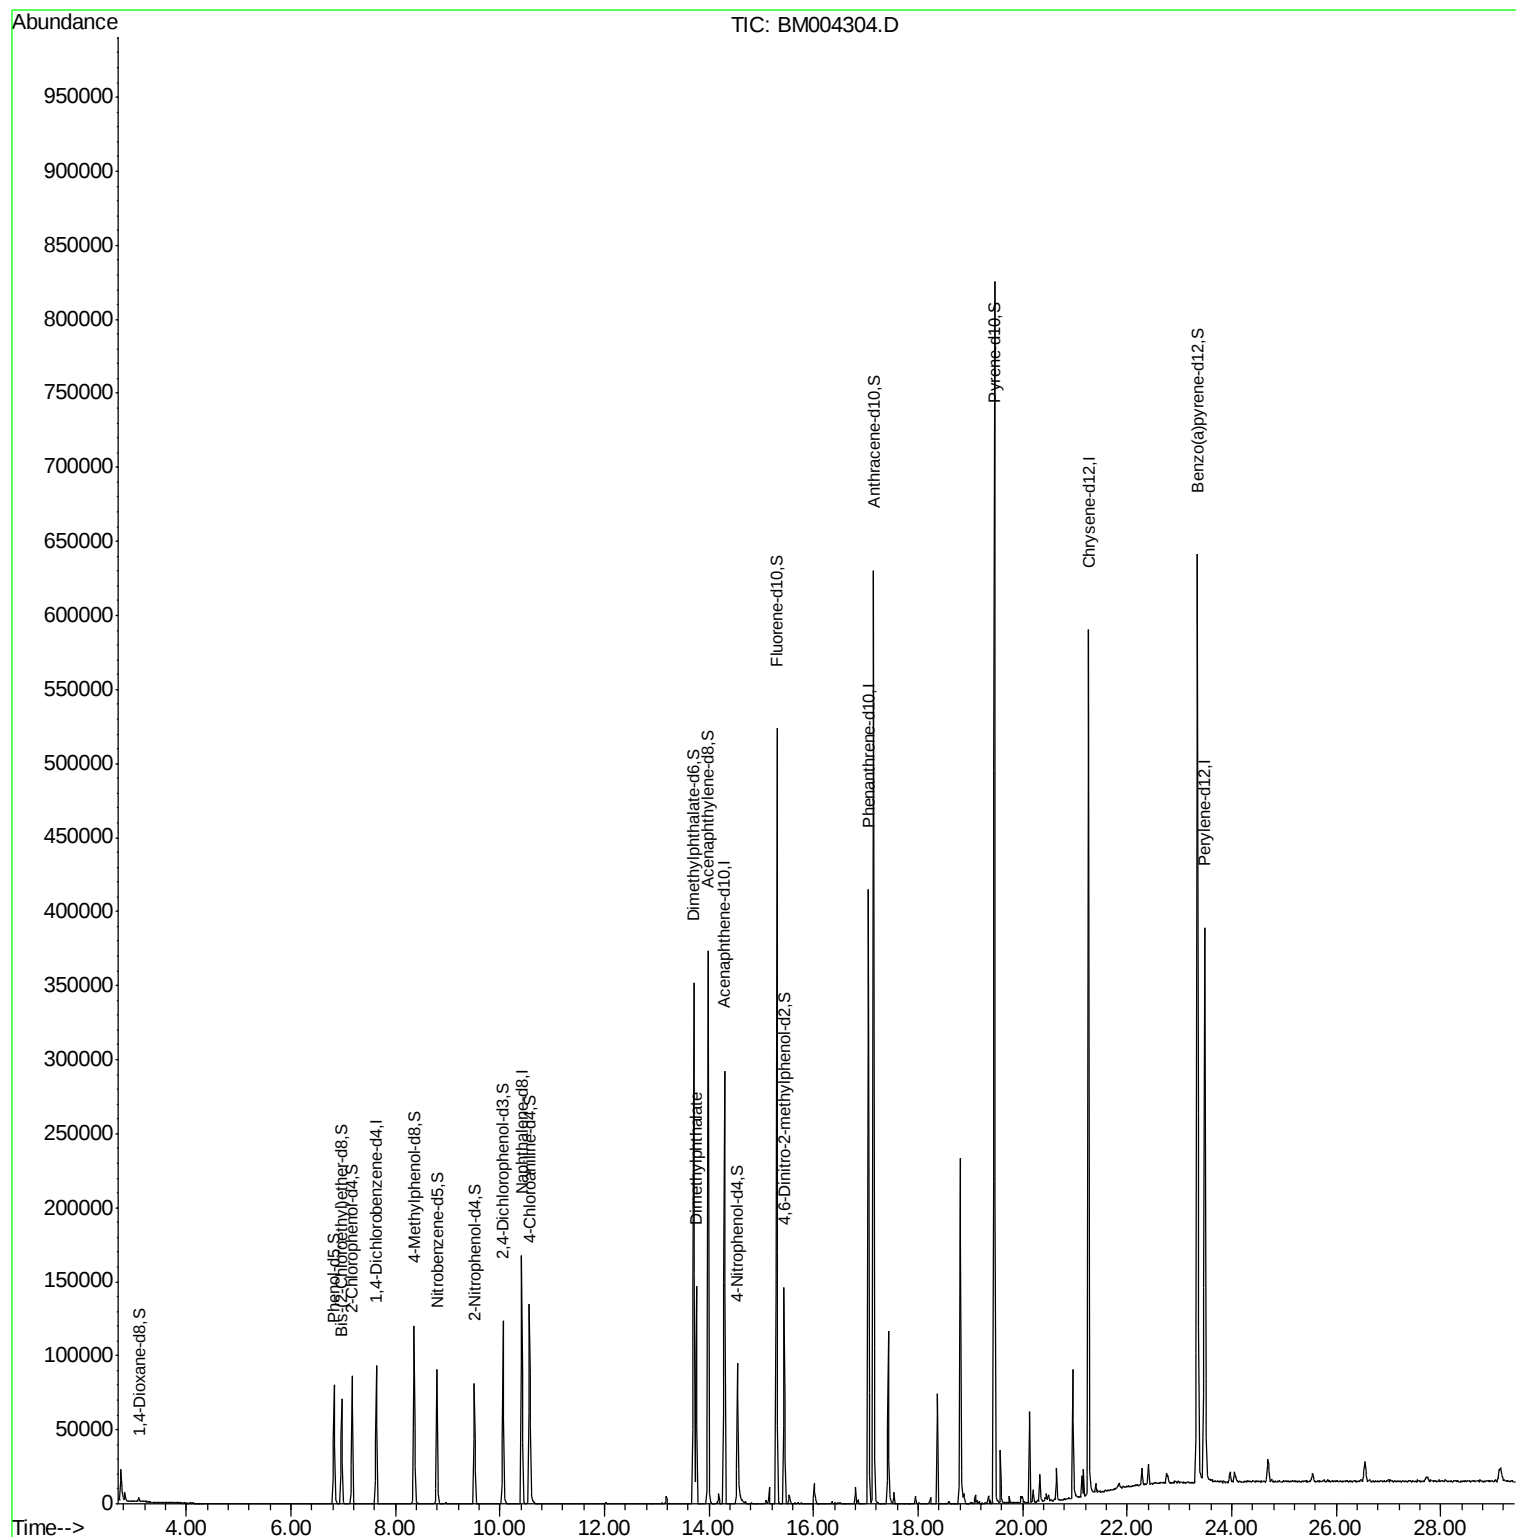

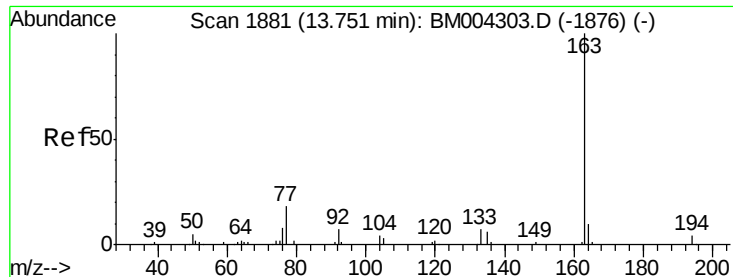

#45

Dimethylphthalate

Concen: 11.06 ng/ul

RT: 13.75 min Scan# 1881

Delta R.T. 0.00 min

Lab File: BM004304.D

Acq: 20 Feb 2016 03:31

Instrument :

BNA_M

ClientSampleId :

0311-SS34A


Tgt Ion:163 Resp: 96844

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.2 7.8 11.8

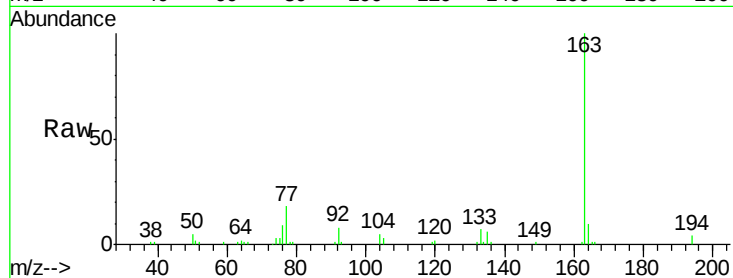

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

