

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021916\
 Data File : BM004288.D
 Acq On : 19 Feb 2016 16:07
 Operator : SJ/UM
 Sample : H1497-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-SS32A

Quant Time: Feb 19 23:34:27 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM021216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 19 23:29:57 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	24342	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	117698	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	75472	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	181664	20.00	ng/ul	0.00
78) Chrysene-d12	21.26	240	216172	20.00	ng/ul	0.00
86) Perylene-d12	23.49	264	212892	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	2500	5.17	ng/uL	0.00
5) Phenol-d5	6.82	99	56310	28.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	31622	29.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	50755	29.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	50794	30.50	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	26332	29.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	30700	30.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	52099	28.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	77249	35.57	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	207909	33.10	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	238017	31.19	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	32220	31.71	ng/ul	0.00
58) Fluorene-d10	15.29	176	176465	33.34	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	29532	26.69	ng/ul	0.00
71) Anthracene-d10	17.15	188	288458	32.48	ng/ul	0.00
79) Pyrene-d10	19.46	212	344136	29.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.34	264	365084	32.14	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	94300	14.37	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021916\
Data File : BM004288.D
Acq On : 19 Feb 2016 16:07
Operator : SJ/UM
Sample : H1497-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-SS32A

Quant Time: Feb 19 23:34:27 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 19 23:29:57 2016
Response via : Initial Calibration

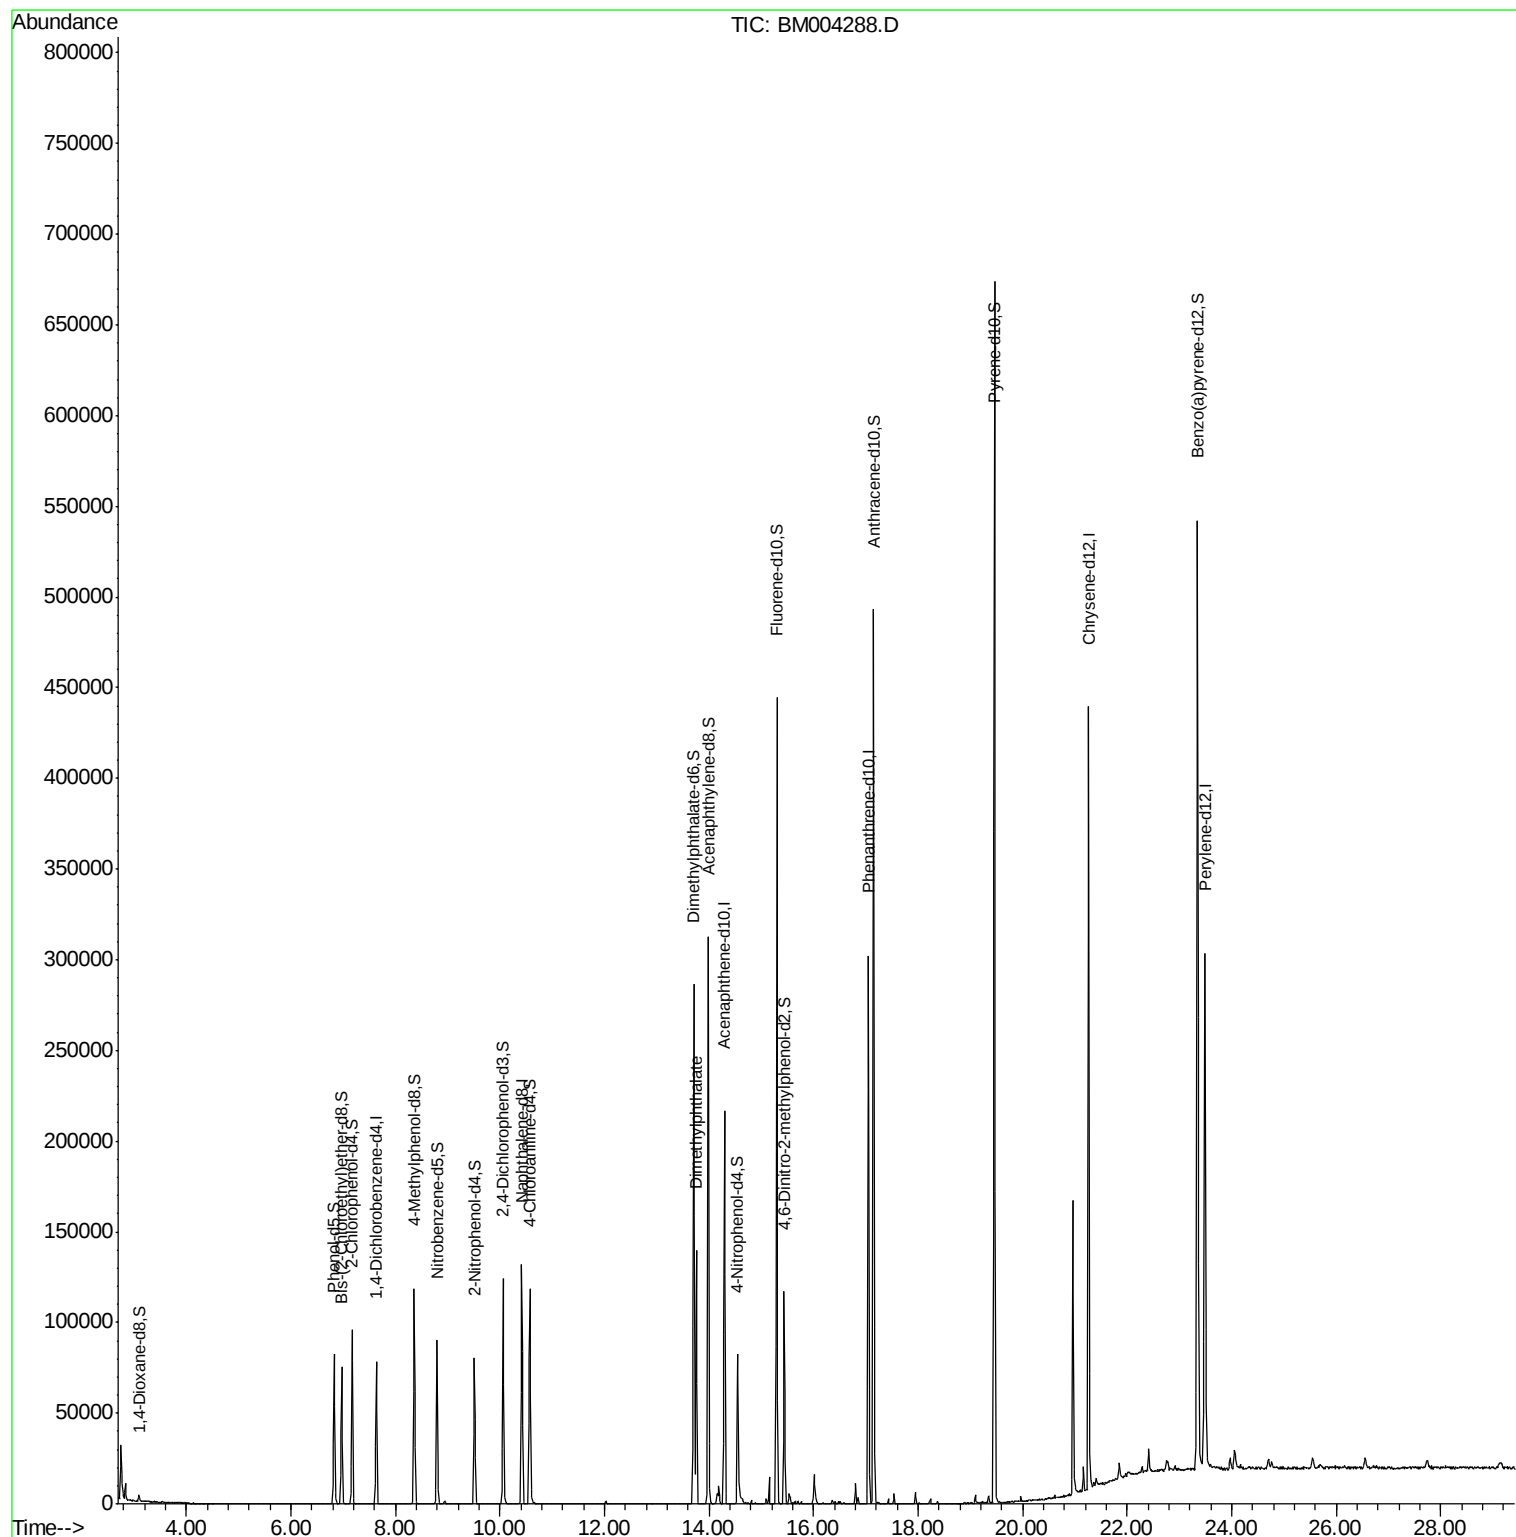

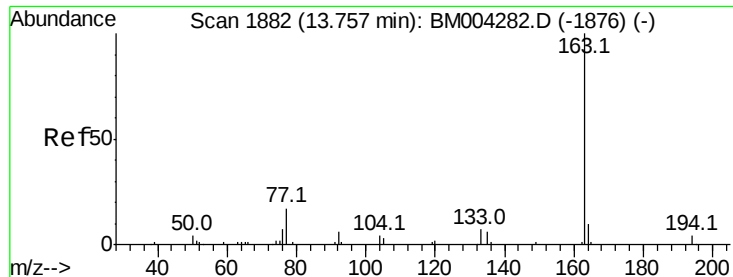

#45

Dimethylphthalate

Concen: 14.37 ng/ul

RT: 13.75 min Scan# 1881

Delta R.T. -0.01 min

Lab File: BM004288.D

Acq: 19 Feb 2016 16:07

Instrument :

BNA_M

ClientSampleId :

0311-SS32A


Tot Ion:163 Resp: 94300

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 10.5 7.8 11.8

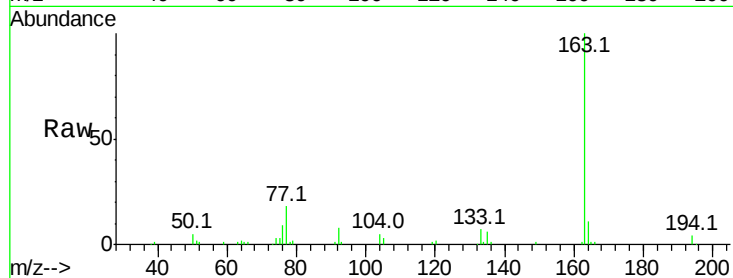

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

