

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021916\
 Data File : BM004293.D
 Acq On : 19 Feb 2016 20:03
 Operator : SJ/UM
 Sample : H1497-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S13-0003

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.752	6	11	21	rVV	28557	47930	4.48%	0.513%
2	2.828	21	24	31	rVB	9942	11932	1.12%	0.128%
3	3.087	65	68	74	rVB	3722	4455	0.42%	0.048%
4	6.822	698	703	715	rBB	86737	137315	12.84%	1.471%
5	6.969	722	728	736	rBB	79019	119428	11.16%	1.279%
6	7.169	756	762	771	rBB	98214	152261	14.23%	1.631%
7	7.628	835	840	847	rBB	85272	133202	12.45%	1.426%
8	8.357	958	964	975	rBB	129433	209193	19.56%	2.240%
9	8.792	1032	1038	1046	rBV	98832	156155	14.60%	1.672%
10	9.510	1155	1160	1168	rBB	87287	138040	12.90%	1.478%
11	10.057	1247	1253	1267	rBB	126821	217223	20.31%	2.326%
12	10.416	1308	1314	1323	rBB	149238	241366	22.56%	2.585%
13	10.563	1333	1339	1355	rBV	134354	236895	22.15%	2.537%
14	12.022	1584	1587	1591	rBB	1299	1743	0.16%	0.019%
15	13.704	1867	1873	1877	rBV	335344	454255	42.46%	4.865%
16	13.751	1877	1881	1888	rVB	131013	170736	15.96%	1.828%
17	13.980	1914	1920	1935	rBB	353802	522744	48.87%	5.598%
18	14.151	1945	1949	1951	rBV	3639	4759	0.44%	0.051%
19	14.186	1951	1955	1960	rVB	9771	12932	1.21%	0.138%
20	14.292	1967	1973	1980	rBB2	260693	390967	36.55%	4.187%
21	14.539	2010	2015	2027	rBV	84456	159808	14.94%	1.711%
22	14.804	2058	2060	2063	rBB	1866	1696	0.16%	0.018%
23	15.145	2114	2118	2121	rBB	13710	16616	1.55%	0.178%
24	15.292	2137	2143	2152	rBB	499608	698514	65.30%	7.481%
25	15.433	2162	2167	2177	rBB	131961	175783	16.43%	1.882%
26	15.533	2180	2184	2190	rBB2	6302	10612	0.99%	0.114%
27	15.698	2210	2212	2215	rBB	1261	1353	0.13%	0.014%
28	16.004	2261	2264	2274	rBV	14872	23370	2.18%	0.250%
29	16.351	2320	2323	2326	rBV	1529	1890	0.18%	0.020%
30	16.798	2396	2399	2403	rBB	5929	6742	0.63%	0.072%
31	16.845	2403	2407	2411	rBB2	1332	2183	0.20%	0.023%
32	17.045	2435	2441	2450	rBV	383436	514267	48.07%	5.507%
33	17.145	2452	2458	2477	rVB2	566669	810788	75.79%	8.683%
34	18.015	2603	2606	2609	rBB	1081	1210	0.11%	0.013%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021916\
 Data File : BM004293.D
 Acq On : 19 Feb 2016 20:03
 Operator : SJ/UM
 Sample : H1497-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S13-0003

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Title : SVOA CALIBRATION

35	19.092	2785	2789	2792	rBV	5314	6513	0.61%	0.070%
36	19.345	2828	2832	2835	rBV	3893	5036	0.47%	0.054%
37	19.456	2844	2851	2859	rBV	767659	1043560	97.55%	11.176%
38	19.515	2859	2861	2865	rVB2	1265	1342	0.13%	0.014%
39	19.992	2939	2942	2946	rBV2	1034	1254	0.12%	0.013%
40	20.492	3024	3027	3030	rVB2	1609	1118	0.10%	0.012%
41	20.962	3103	3107	3113	rBV4	14259	20332	1.90%	0.218%
42	21.033	3117	3119	3121	rBV2	1218	1133	0.11%	0.012%
43	21.162	3138	3141	3145	rVB	7429	8296	0.78%	0.089%
44	21.256	3152	3157	3173	rBV	520092	680763	63.64%	7.290%
45	21.397	3179	3181	3184	rBV3	3025	2846	0.27%	0.030%
46	21.827	3252	3254	3258	rVB2	2954	2754	0.26%	0.029%
47	22.756	3408	3412	3413	rBV3	5949	8352	0.78%	0.089%
48	22.827	3421	3424	3431	rVB5	5268	8803	0.82%	0.094%
49	23.344	3504	3512	3523	rBV	581141	1069722	100.00%	11.456%
50	23.486	3529	3536	3549	rVB	339398	639592	59.79%	6.850%
51	23.962	3613	3617	3626	rVB3	13344	26062	2.44%	0.279%
52	26.556	4051	4058	4064	rBV5	9656	21908	2.05%	0.235%


Sum of corrected areas: 9337749

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021916\
Data File : BM004293.D
Acq On : 19 Feb 2016 20:03
Operator : SJ/UM
Sample : H1497-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S13-0003

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

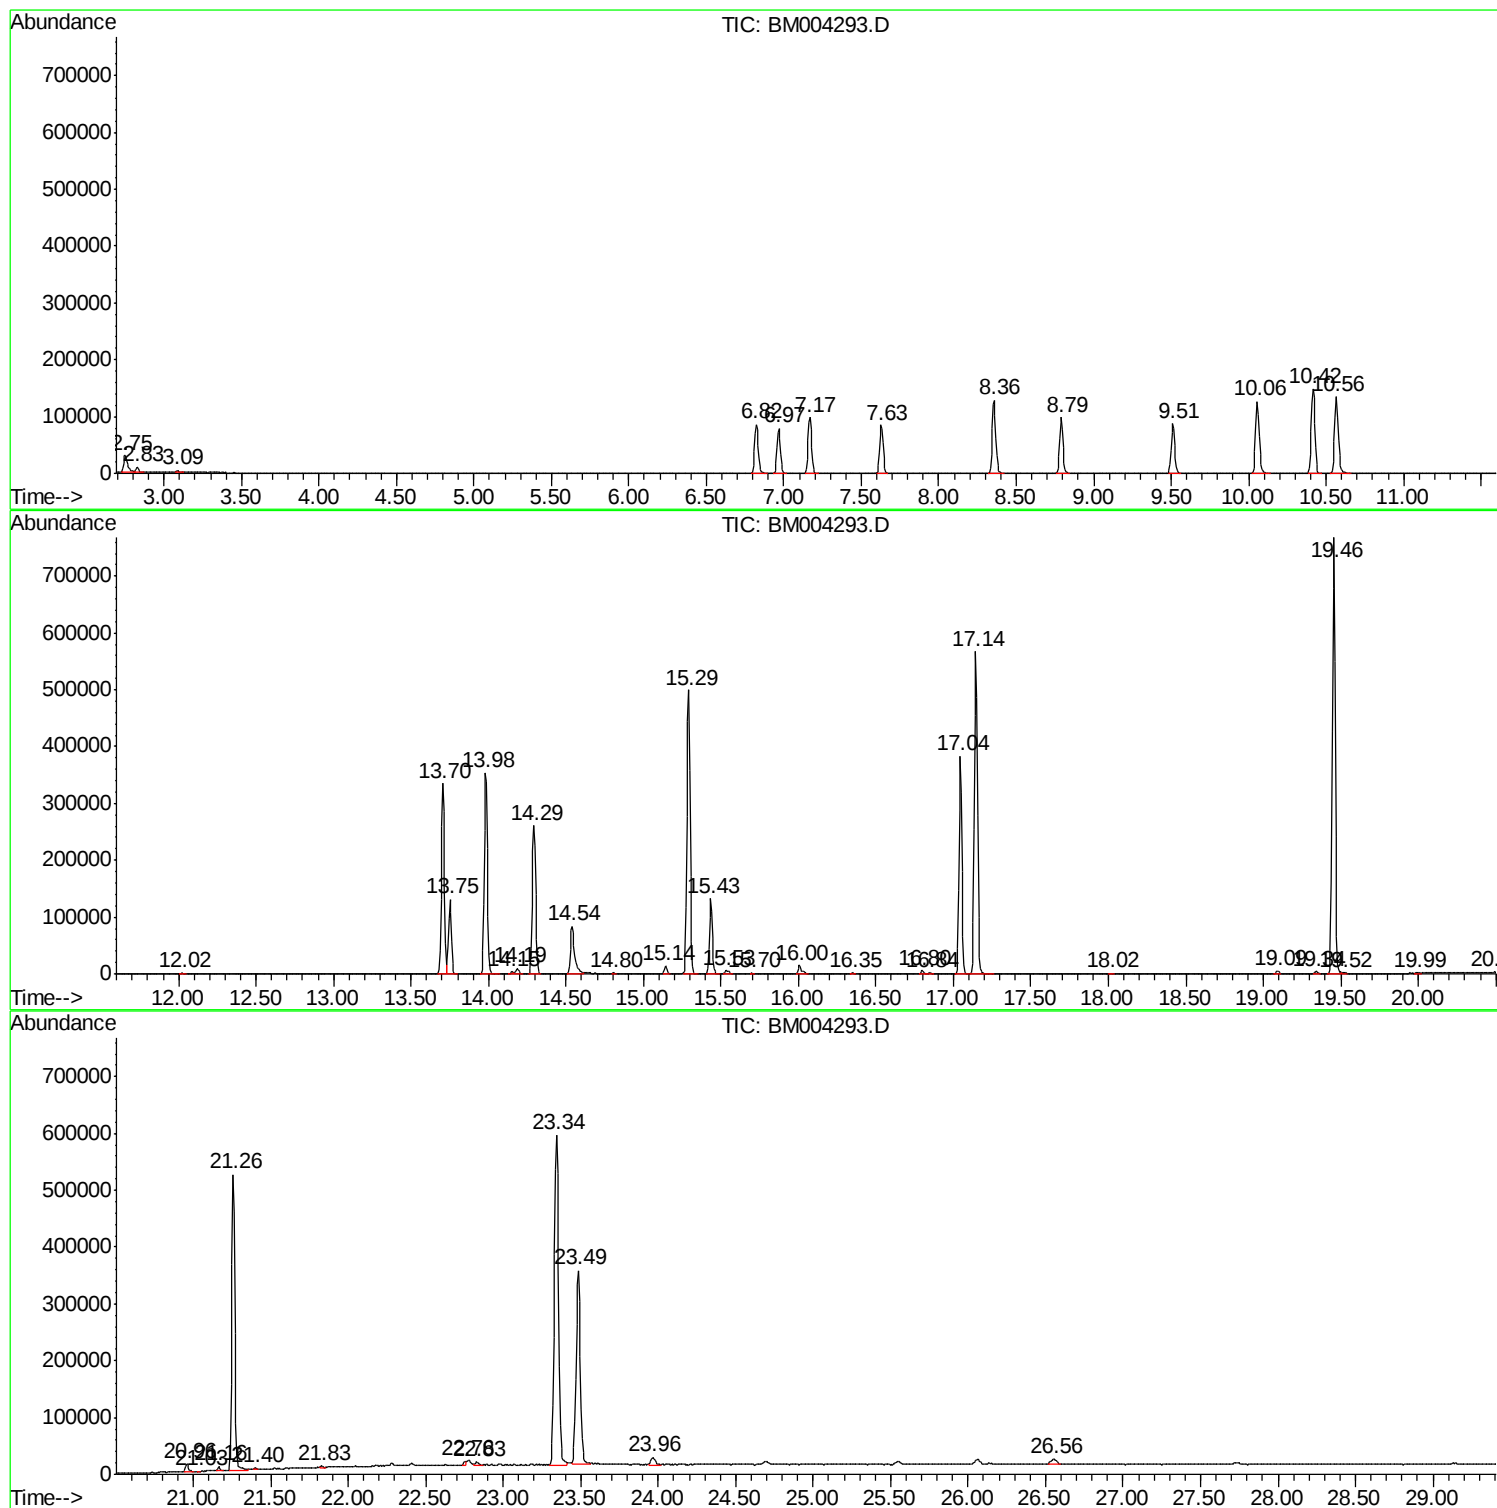

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
Data File : BM004293.D
Acq On : 19 Feb 2016 20:03
Operator : SJ/UM
Sample : H1497-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S13-0003

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
Data File : BM004293.D
Acq On : 19 Feb 2016 20:03
Operator : SJ/UM
Sample : H1497-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S13-0003

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc