

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021916\
 Data File : BM004296.D
 Acq On : 19 Feb 2016 21:52
 Operator : SJ/UM
 Sample : H1497-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-SS34C

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.751	6	11	21	rVV	23327	38757	4.01%	0.453%
2	2.828	21	24	31	rVB	7083	8619	0.89%	0.101%
3	3.087	65	68	73	rVB	3233	3978	0.41%	0.047%
4	4.157	246	250	254	rBB	3664	4754	0.49%	0.056%
5	6.822	698	703	715	rBB	79223	125942	13.02%	1.473%
6	6.969	722	728	737	rBB	72540	109611	11.33%	1.282%
7	7.169	756	762	772	rBB	88828	138439	14.31%	1.620%
8	7.628	835	840	847	rBB	79240	124132	12.83%	1.452%
9	8.357	958	964	976	rBB	116095	191080	19.75%	2.236%
10	8.792	1032	1038	1048	rBB	88813	141782	14.66%	1.659%
11	8.951	1062	1065	1069	rBB2	861	1269	0.13%	0.015%
12	9.510	1155	1160	1168	rBB	78464	122866	12.70%	1.437%
13	10.057	1247	1253	1266	rBV	115067	193697	20.02%	2.266%
14	10.416	1308	1314	1323	rBB	137414	226417	23.40%	2.649%
15	10.563	1333	1339	1356	rBV	121091	214520	22.17%	2.510%
16	12.027	1585	1588	1591	rBB	1051	1426	0.15%	0.017%
17	13.704	1867	1873	1877	rBV	297687	407735	42.15%	4.770%
18	13.751	1877	1881	1889	rVB	140000	186657	19.29%	2.184%
19	13.980	1914	1920	1933	rBV	317937	471410	48.73%	5.515%
20	14.151	1945	1949	1951	rBV	2460	3689	0.38%	0.043%
21	14.186	1951	1955	1960	rVB	10200	13278	1.37%	0.155%
22	14.292	1967	1973	1980	rBB2	238593	361829	37.40%	4.233%
23	14.539	2010	2015	2027	rBV	75561	140953	14.57%	1.649%
24	14.627	2029	2030	2037	rVV2	3298	5284	0.55%	0.062%
25	14.692	2037	2041	2043	rVB	1343	1421	0.15%	0.017%
26	14.804	2058	2060	2063	rBB	2203	2202	0.23%	0.026%
27	15.092	2106	2109	2113	rBB	2069	2804	0.29%	0.033%
28	15.139	2114	2117	2122	rBB	15982	19636	2.03%	0.230%
29	15.292	2137	2143	2152	rBB	438033	631920	65.32%	7.393%
30	15.433	2162	2167	2174	rBV	114464	149654	15.47%	1.751%
31	15.533	2180	2184	2191	rBB3	6193	11531	1.19%	0.135%
32	15.586	2191	2193	2196	rBB	1086	973	0.10%	0.011%
33	15.645	2200	2203	2205	rBB	1228	1320	0.14%	0.015%
34	15.698	2209	2212	2215	rBB	1926	1799	0.19%	0.021%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021916\
 Data File : BM004296.D
 Acq On : 19 Feb 2016 21:52
 Operator : SJ/UM
 Sample : H1497-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-SS34C

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Title : SVOA CALIBRATION

35	15.762	2221	2223	2226	rBB	1583	1402	0.14%	0.016%
36	16.004	2260	2264	2275	rBV	19035	30166	3.12%	0.353%
37	16.345	2320	2322	2326	rBV	1952	2717	0.28%	0.032%
38	16.409	2330	2333	2336	rBB	1491	1024	0.11%	0.012%
39	16.798	2396	2399	2403	rBB	10828	11850	1.22%	0.139%
40	16.845	2403	2407	2411	rBB3	3007	4533	0.47%	0.053%
41	17.045	2435	2441	2447	rBV	347845	481120	49.73%	5.629%
42	17.145	2452	2458	2471	rVB2	510890	727671	75.22%	8.513%
43	17.539	2522	2525	2528	rBV	3050	3012	0.31%	0.035%
44	18.015	2602	2606	2608	rBV	958	1116	0.12%	0.013%
45	19.092	2785	2789	2792	rBV	4400	5191	0.54%	0.061%
46	19.339	2827	2831	2835	rBV	3771	4449	0.46%	0.052%
47	19.450	2844	2850	2859	rBV2	661089	919781	95.08%	10.761%
48	19.509	2859	2860	2866	rVB	1180	1225	0.13%	0.014%
49	20.921	3097	3100	3101	rBV2	1033	1036	0.11%	0.012%
50	20.956	3103	3106	3112	rVV2	16592	20842	2.15%	0.244%
51	21.033	3117	3119	3123	rVB2	2123	3135	0.32%	0.037%
52	21.162	3138	3141	3144	rBV	6910	6504	0.67%	0.076%
53	21.256	3152	3157	3169	rBV	478798	628276	64.94%	7.350%
54	21.397	3178	3181	3184	rBV2	2366	3452	0.36%	0.040%
55	21.821	3251	3253	3257	rBV3	2490	3172	0.33%	0.037%
56	22.280	3328	3331	3336	rVB3	4848	6085	0.63%	0.071%
57	22.409	3350	3353	3356	rVB2	4600	5027	0.52%	0.059%
58	23.338	3504	3511	3524	rBV	515929	967399	100.00%	11.318%
59	23.480	3528	3535	3545	rVV2	315077	600130	62.04%	7.021%
60	23.962	3613	3617	3623	rVB2	12055	20107	2.08%	0.235%
61	24.691	3736	3741	3751	rVB3	11860	25686	2.66%	0.301%


Sum of corrected areas: 8547492

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021916\
Data File : BM004296.D
Acq On : 19 Feb 2016 21:52
Operator : SJ/UM
Sample : H1497-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
0311-SS34C

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

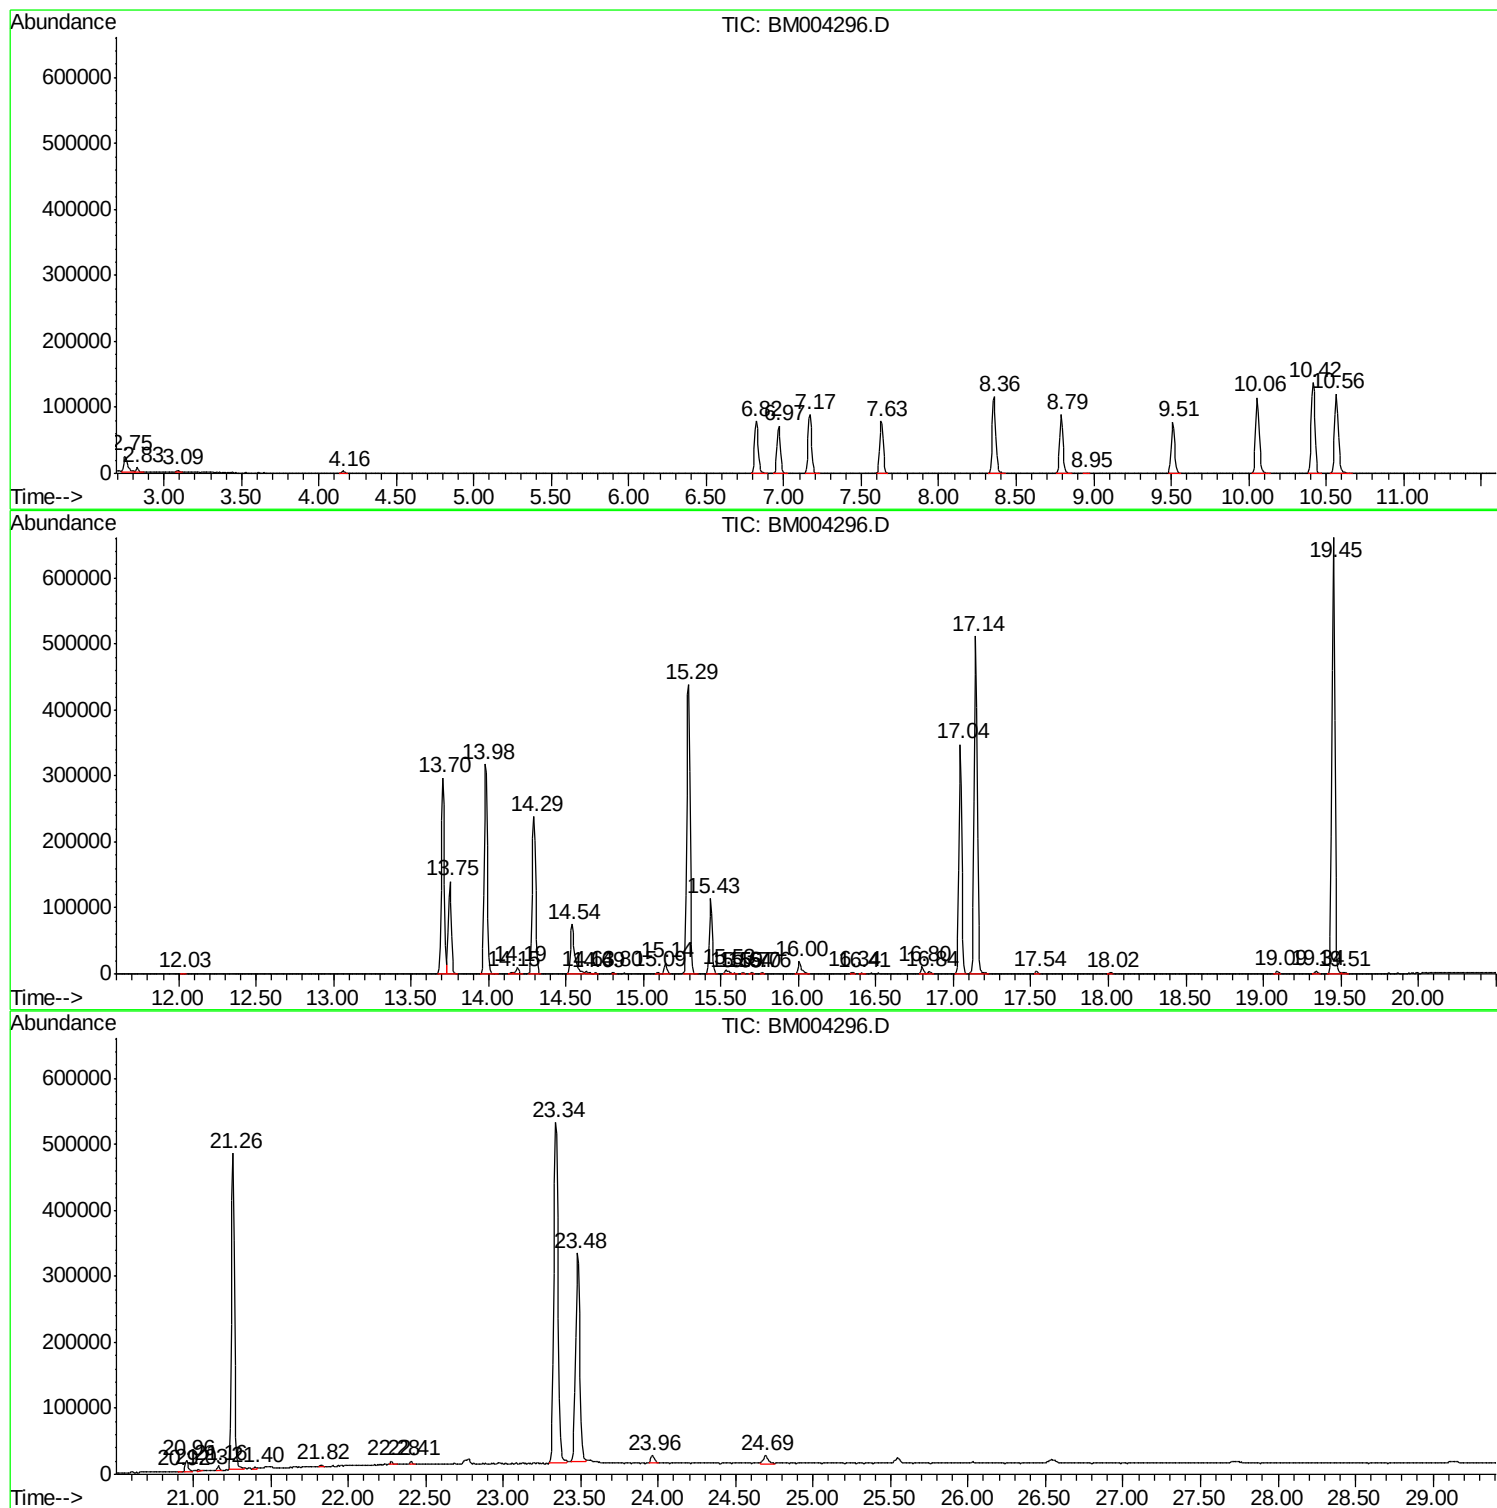

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
Data File : BM004296.D
Acq On : 19 Feb 2016 21:52
Operator : SJ/UM
Sample : H1497-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-SS34C

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
Data File : BM004296.D
Acq On : 19 Feb 2016 21:52
Operator : SJ/UM
Sample : H1497-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-SS34C

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc