

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021916\
 Data File : BM004301.D
 Acq On : 20 Feb 2016 00:53
 Operator : SJ/UM
 Sample : H1497-21
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S08-0003

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.746	6	10	21	rVV	28806	49806	4.44%	0.492%
2	2.828	21	24	31	rVB	10200	12715	1.13%	0.126%
3	3.087	65	68	73	rVB	4551	4953	0.44%	0.049%
4	6.822	697	703	714	rBV	100111	159448	14.23%	1.575%
5	6.969	722	728	736	rBV	88360	135311	12.08%	1.337%
6	7.169	756	762	772	rBB	107983	172744	15.42%	1.707%
7	7.628	835	840	847	rBB	87665	135927	12.13%	1.343%
8	8.357	958	964	975	rBV	148408	245613	21.92%	2.427%
9	8.793	1032	1038	1046	rBV	111330	177845	15.87%	1.757%
10	9.510	1154	1160	1168	rBB	98494	157827	14.09%	1.559%
11	10.057	1247	1253	1267	rBV	147940	254298	22.69%	2.513%
12	10.416	1307	1314	1323	rBB	156680	251154	22.41%	2.481%
13	10.563	1333	1339	1361	rBV	151297	270558	24.15%	2.673%
14	12.022	1584	1587	1591	rBB	1478	2116	0.19%	0.021%
15	13.704	1867	1873	1877	rBV	366122	498652	44.50%	4.927%
16	13.751	1877	1881	1888	rVB	125230	165125	14.74%	1.631%
17	13.980	1914	1920	1936	rBB	403287	592594	52.89%	5.855%
18	14.157	1946	1950	1951	rBV	1747	2267	0.20%	0.022%
19	14.186	1951	1955	1959	rVB	10898	13583	1.21%	0.134%
20	14.292	1967	1973	1980	rBB2	266741	401979	35.87%	3.972%
21	14.539	2010	2015	2028	rBV	98953	186774	16.67%	1.845%
22	14.633	2028	2031	2038	rVV3	3636	7951	0.71%	0.079%
23	14.686	2038	2040	2044	rVB	2480	2365	0.21%	0.023%
24	14.804	2058	2060	2063	rBB	2483	2410	0.22%	0.024%
25	15.092	2106	2109	2113	rBB	2148	2688	0.24%	0.027%
26	15.145	2114	2118	2122	rBB	17571	21372	1.91%	0.211%
27	15.292	2137	2143	2154	rBB	538980	781792	69.77%	7.724%
28	15.433	2162	2167	2179	rBB	150032	198156	17.68%	1.958%
29	15.533	2180	2184	2191	rBB4	6936	13042	1.16%	0.129%
30	15.592	2191	2194	2196	rBB	1398	1143	0.10%	0.011%
31	15.645	2200	2203	2205	rBB	1742	1525	0.14%	0.015%
32	15.698	2209	2212	2215	rBB	1940	2081	0.19%	0.021%
33	15.763	2221	2223	2226	rBB	1984	1454	0.13%	0.014%
34	16.004	2260	2264	2273	rBV	19626	31880	2.85%	0.315%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021916\
 Data File : BM004301.D
 Acq On : 20 Feb 2016 00:53
 Operator : SJ/UM
 Sample : H1497-21
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S08-0003

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
 Title : SVOA CALIBRATION

35	16.351	2319	2323	2326	rBV2	2081	3247	0.29%	0.032%
36	16.410	2330	2333	2336	rVB	1509	1291	0.12%	0.013%
37	16.798	2396	2399	2403	rBV	11418	12874	1.15%	0.127%
38	16.845	2403	2407	2412	rVB3	2844	4777	0.43%	0.047%
39	17.045	2435	2441	2447	rBV	381054	518066	46.23%	5.119%
40	17.145	2452	2458	2477	rVB2	604824	871794	77.80%	8.614%
41	17.533	2522	2524	2528	rBB	3646	4001	0.36%	0.040%
42	17.945	2591	2594	2599	rBB	8271	9456	0.84%	0.093%
43	18.016	2603	2606	2609	rBB	1762	2061	0.18%	0.020%
44	19.086	2783	2788	2790	rBV	5846	6677	0.60%	0.066%
45	19.115	2790	2793	2799	rVB	10294	12994	1.16%	0.128%
46	19.339	2827	2831	2835	rBV	4500	5682	0.51%	0.056%
47	19.457	2844	2851	2860	rBV	787674	1120524	100.00%	11.071%
48	20.604	3043	3046	3050	rVB	2828	3024	0.27%	0.030%
49	20.951	3101	3105	3116	rVB2	47610	68267	6.09%	0.675%
50	21.033	3116	3119	3123	rBV	4951	6920	0.62%	0.068%
51	21.162	3137	3141	3145	rBV	20898	22462	2.00%	0.222%
52	21.256	3151	3157	3169	rBV	505103	686595	61.27%	6.784%
53	21.392	3178	3180	3185	rVB4	2831	3454	0.31%	0.034%
54	21.821	3250	3253	3255	rBV3	3531	4616	0.41%	0.046%
55	22.274	3327	3330	3335	rBV2	5507	7164	0.64%	0.071%
56	22.745	3406	3410	3412	rBV2	7022	9269	0.83%	0.092%
57	22.815	3419	3422	3429	rBV2	6592	13609	1.21%	0.134%
58	23.339	3504	3511	3526	rVB	602162	1110092	99.07%	10.968%
59	23.480	3527	3535	3548	rVB	332162	624561	55.74%	6.171%
60	23.962	3613	3617	3622	rVB2	9020	14676	1.31%	0.145%
61	24.692	3737	3741	3746	rVB4	7463	13761	1.23%	0.136%


Sum of corrected areas: 10121062

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021916\
Data File : BM004301.D
Acq On : 20 Feb 2016 00:53
Operator : SJ/UM
Sample : H1497-21
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S08-0003

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

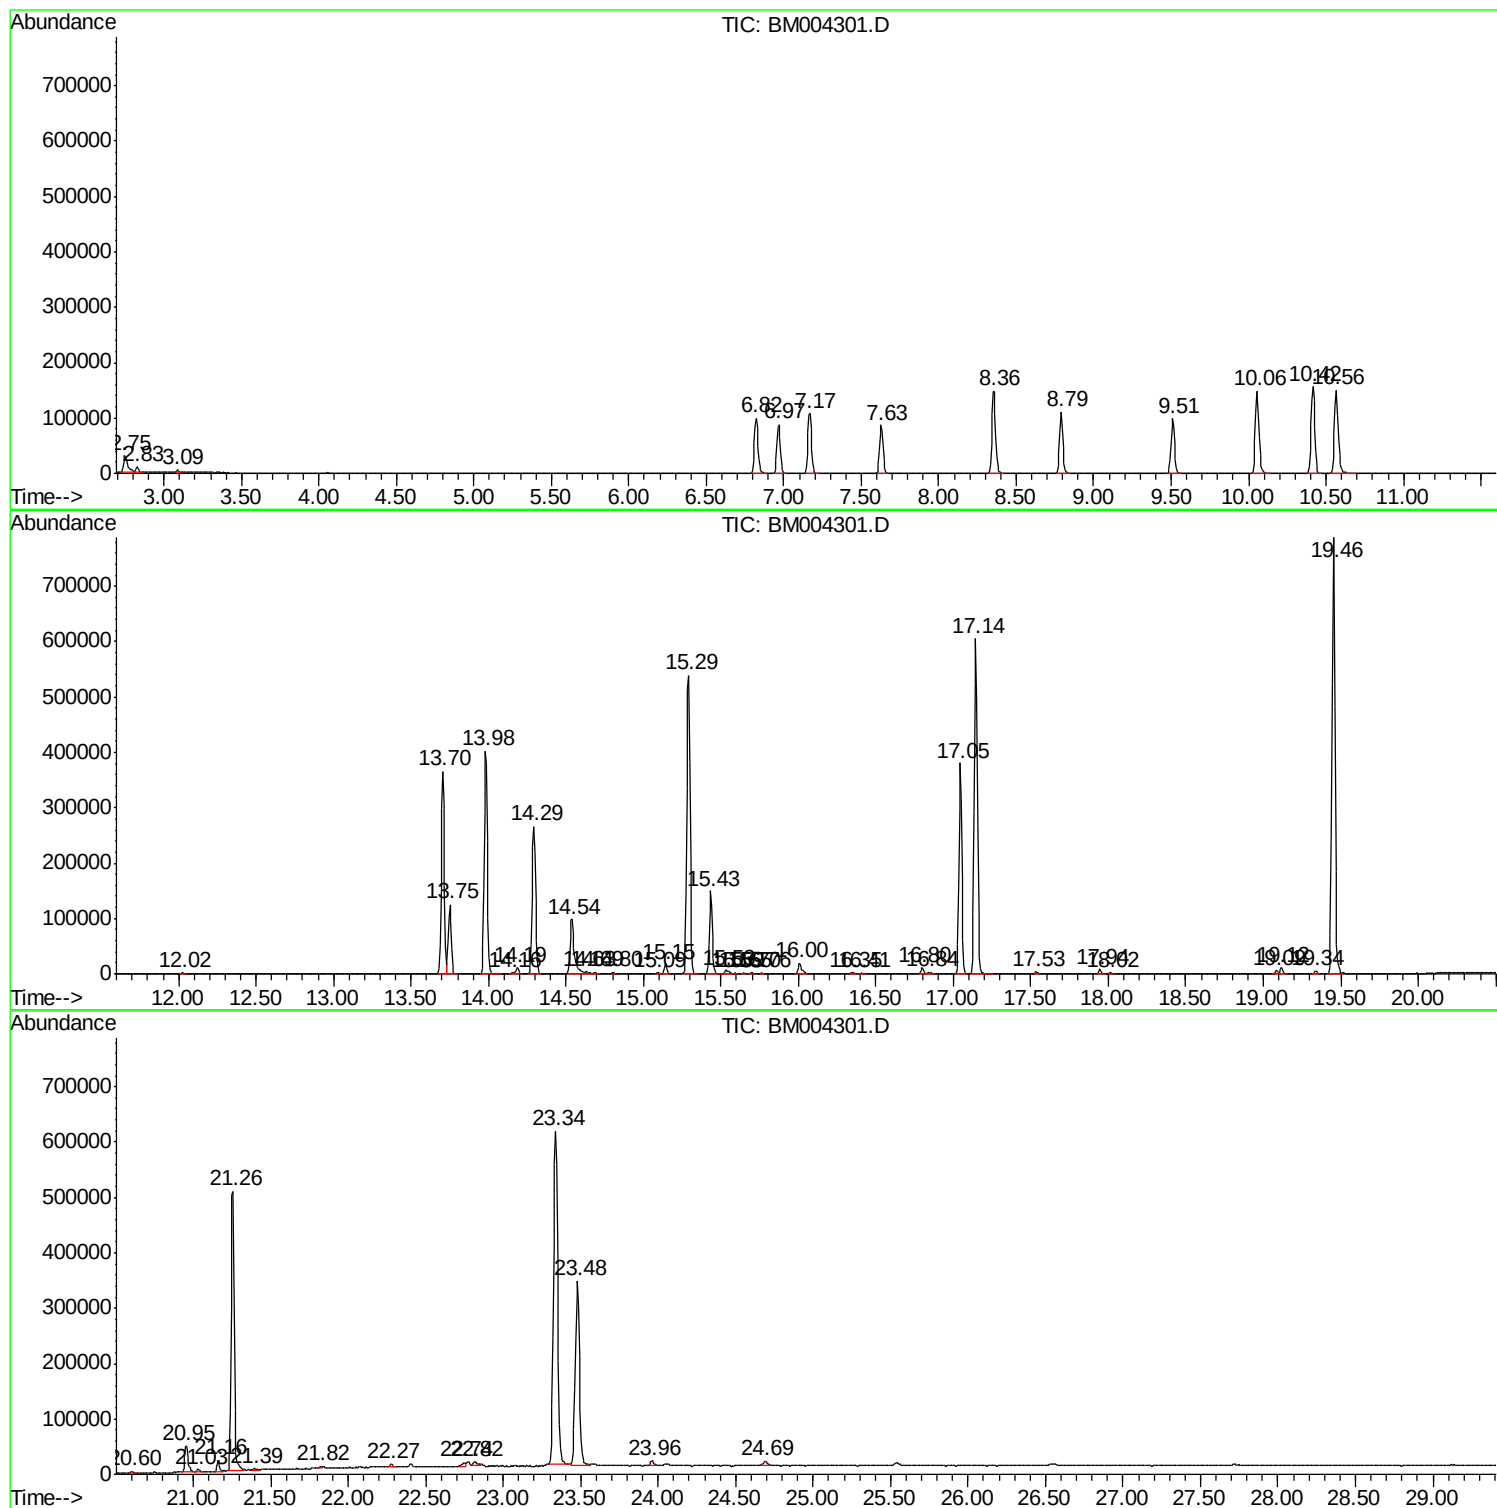

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
Data File : BM004301.D
Acq On : 20 Feb 2016 00:53
Operator : SJ/UM
Sample : H1497-21
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S08-0003

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021916\
Data File : BM004301.D
Acq On : 20 Feb 2016 00:53
Operator : SJ/UM
Sample : H1497-21
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S08-0003

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM021216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc