
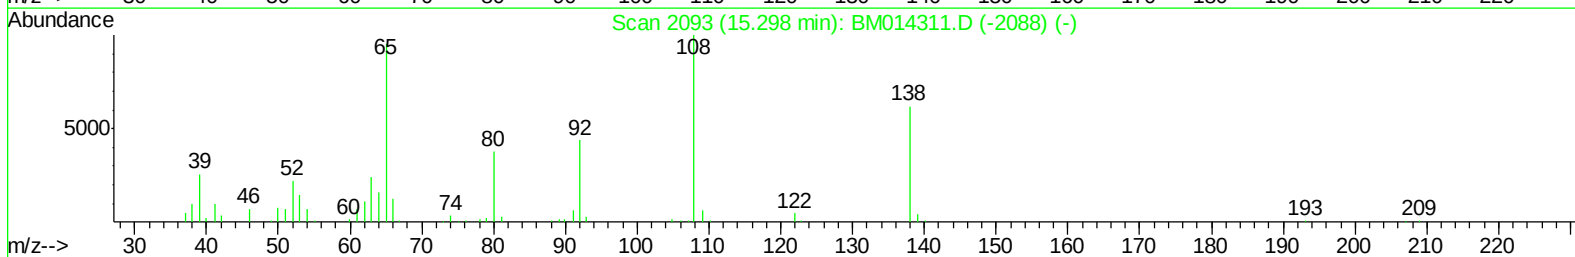
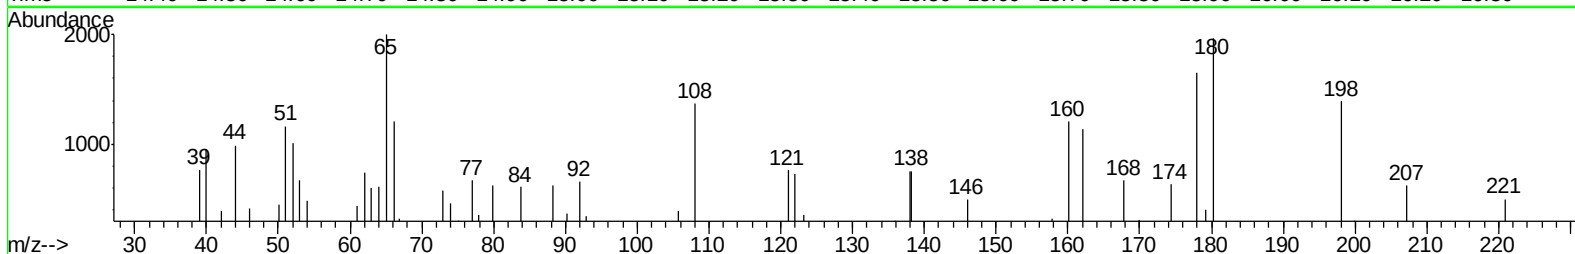


Data Path : Z:\HPCHEM1\BNA M\DATA\BM021918\
Data File : BM014316.D
Acq On : 20 Feb 2018 04:55
Operator : SJ/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 20 06:02:04 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 20 03:49:19 2018
Response via : Initial Calibration

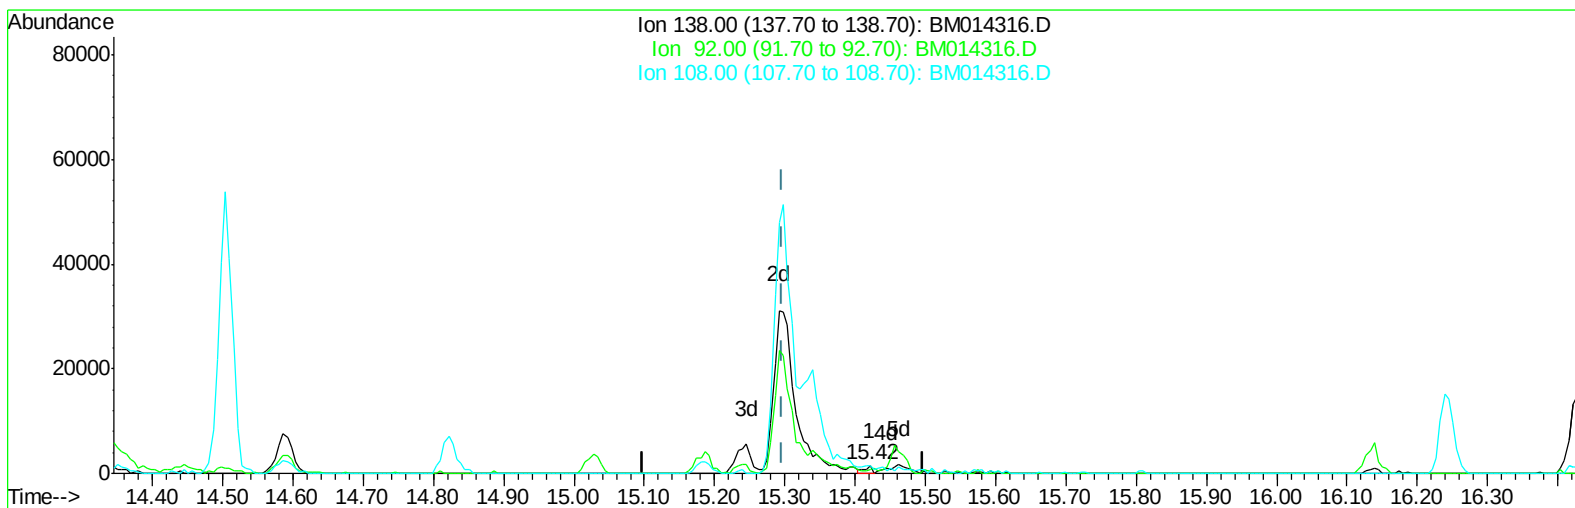

TIC: BM014316.D

(60) 4-Nitroaniline

15.421min (+0.124) 0.28ng/ul

response 1078

Ion	Exp%	Act%
138.00	100	100
92.00	50.00	43.69
108.00	100.00	90.77
0.00	0.00	0.00