

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021918\
 Data File : BM014315.D
 Acq On : 20 Feb 2018 04:19
 Operator : SJ/JU
 Sample : J1524-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 20 06:01:53 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 20 03:49:19 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	2170	20.00	ng/ul	0.10
18) Naphthalene-d8	10.30	136	281186	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.18	164	199230	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.95	188	453685	20.00	ng/ul	0.00
75) Chrysene-d12	21.15	240	404224	20.00	ng/ul	0.00
83) Perylene-d12	23.32	264	362107	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.26	176	571	0.04	ng/ul	0.08
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	16.95	188	453685	20.73	ng/ul	-0.09
76) Pyrene-d10	0.00	212	0	0.00	ng/ul	
87) Benzo(a)pyrene-d12	23.32	264	342449	19.43	ng/ul	0.14


Target Compounds				Ovalue
2) 1,4-Dioxane	3.03	88	177	3.143 ng/uL# 8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021918\
Data File : BM014315.D
Acq On : 20 Feb 2018 04:19
Operator : SJ/JU
Sample : J1524-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 20 06:01:53 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 20 03:49:19 2018
Response via : Initial Calibration

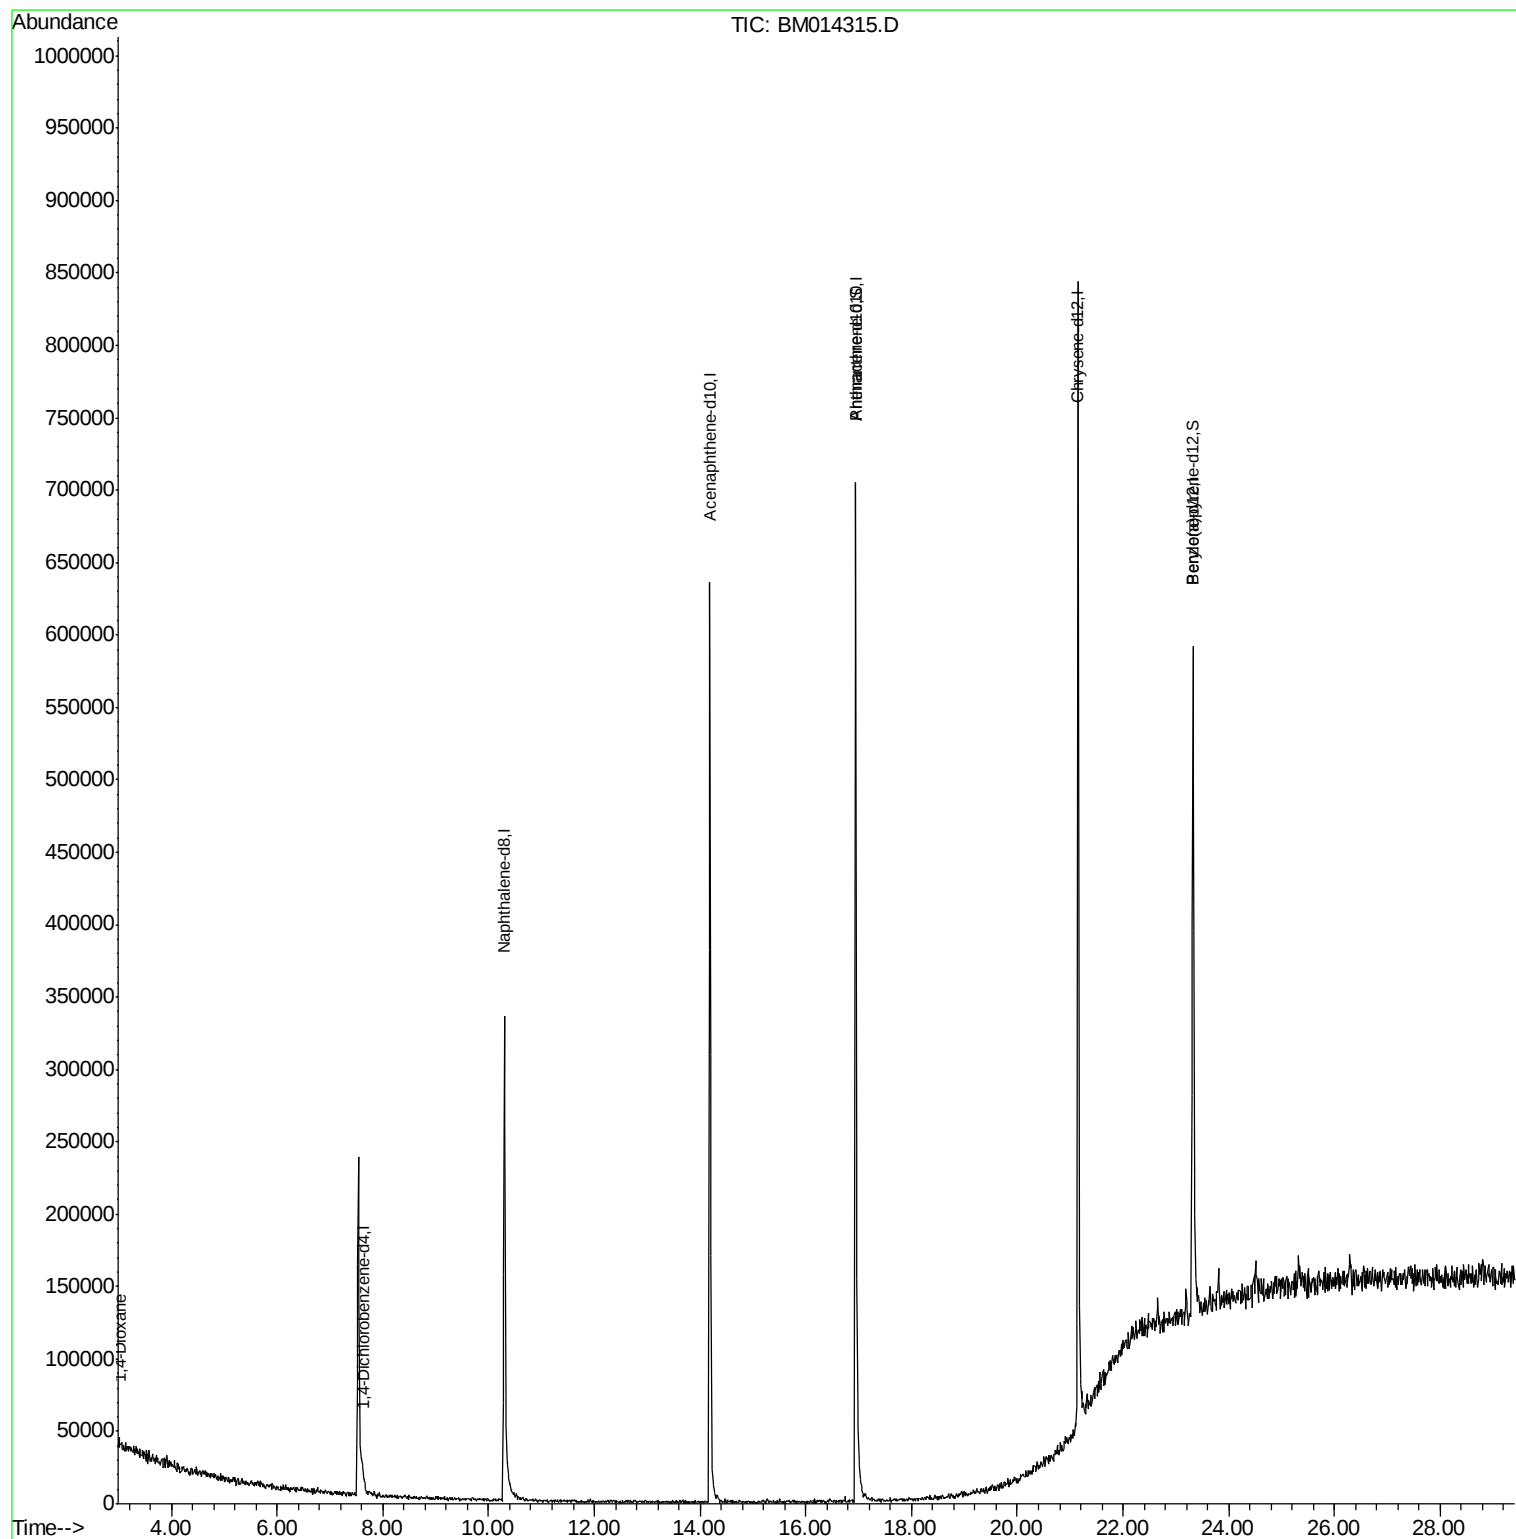

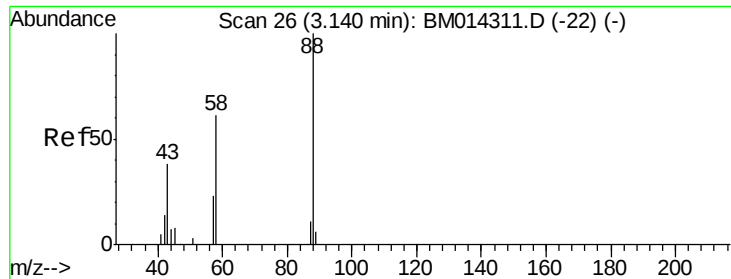

#2
 1,4-Dioxane
 Concen: 3.143 ng/uL
 RT: 3.03 min Scan# 8
 Delta R.T. -0.11 min
 Lab File: BM014315.D
 Acq: 20 Feb 2018 04:19

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
88	100		
43	0.0	48.0	72.0#
58	0.0	80.0	120.0#

