

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021918\
 Data File : BM014309.D
 Acq On : 20 Feb 2018 00:39
 Operator : SJ/JU
 Sample : J1570-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C02Y0

Manual Integrations
 APPROVED

Sohil
 2/20/2018 3:14:02 PM

Quant Time: Feb 20 03:32:30 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 20 01:37:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	72455m	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	315963	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.19	164	212719	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.94	188	512030	20.00	ng/ul	0.00
75) Chrysene-d12	21.15	240	529379	20.00	ng/ul	0.00
83) Perylene-d12	23.32	264	476908	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.11	96	10287m	6.08	ng/uL	0.00
5) Phenol-d5	6.74	99	36423	5.95	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	6.88	67	116321	31.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.07	132	117385	25.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	78913	14.73	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	75688	32.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.40	143	79867	33.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.94	165	136348m	27.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.30	131	258	0.05	ng/ul	-0.16
43) Dimethylphthalate-d6	13.61	166	613079	34.90	ng/ul	0.00
46) Acenaphthylene-d8	13.87	160	741054	34.21	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	9894m	4.08	ng/ul	0.07
57) Fluorene-d10	15.19	176	541268	34.39	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.34	200	83001	27.02	ng/ul	0.00
70) Anthracene-d10	17.04	188	874064	35.38	ng/ul	0.00
76) Pyrene-d10	19.35	212	997244	36.52	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.19	264	801221	34.52	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) 1,4-Dioxane	3.14	88	8106	4.310	ng/uL#	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM021918\
Data File : BM014309.D
Acq On : 20 Feb 2018 00:39
Operator : SJ/JU
Sample : J1570-15
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C02Y0

Manual Integrations
APPROVED

Sohil
2/20/2018 3:14:02 PM

Quant Time: Feb 20 03:32:30 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 20 01:37:12 2018
Response via : Initial Calibration

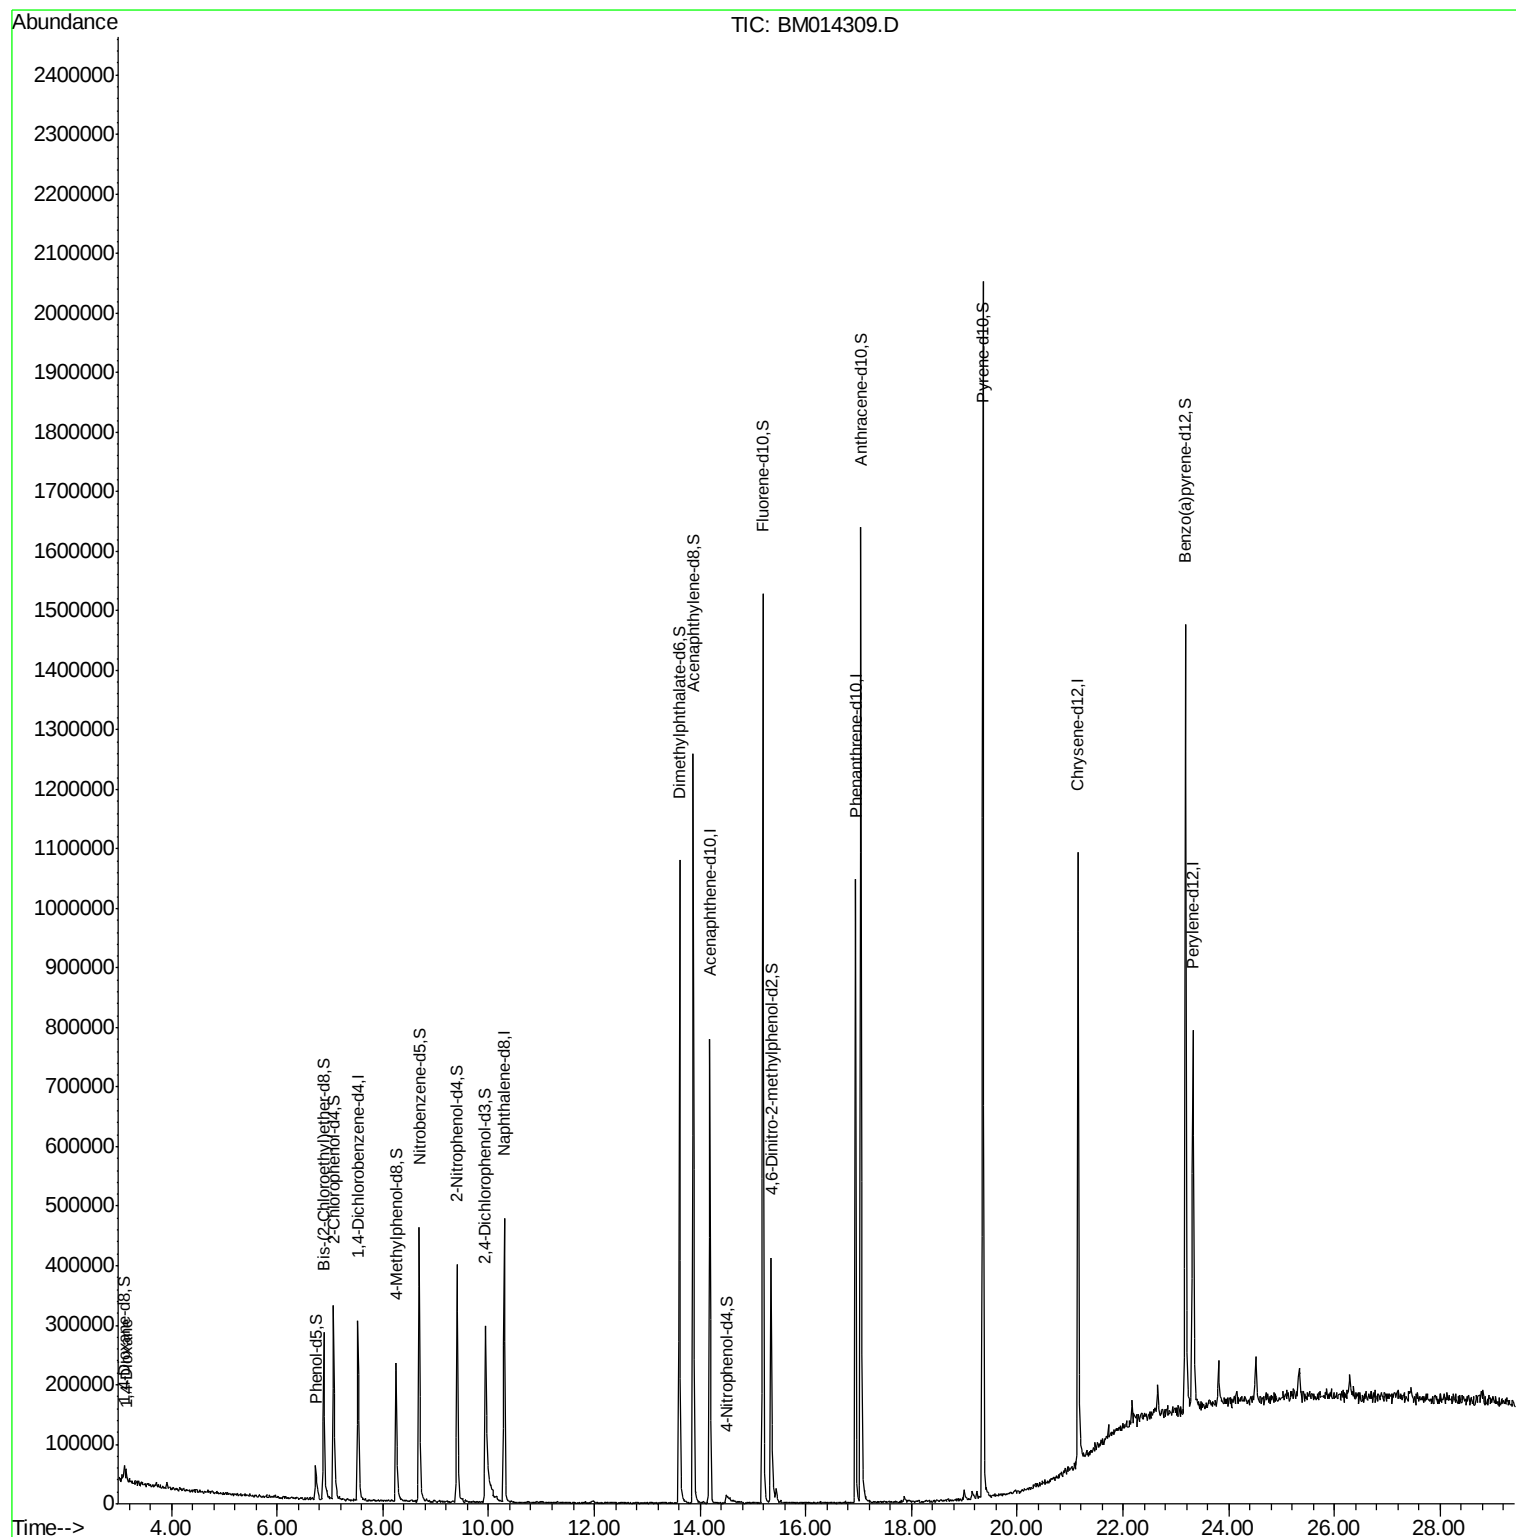

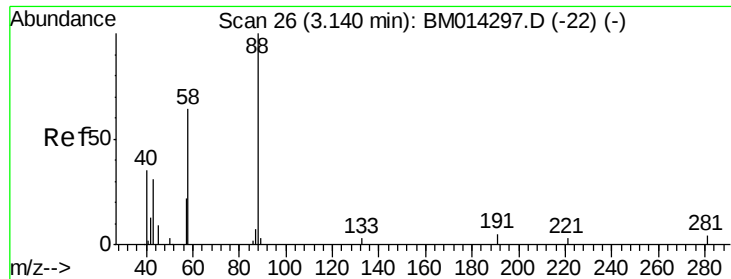

#2
 1,4-Dioxane
 Concen: 4.310 ng/uL
 RT: 3.14 min Scan# 26
 Delta R.T. 0.00 min
 Lab File: BM014309.D
 Acq: 20 Feb 2018 00:39

Instrument :
 BNA_M
 ClientSampleId :
 C02Y0

Tot Ion	Ratio	Lower	Upper
88	100		
43	44.7	48.0	72.0#
58	62.9	80.0	120.0#

Manual Integrations
 APPROVED

Sohil
 2/20/2018 3:14:02 PM

