

Data Path : Z:\HPCHEM1\BNA M\DATA\BM021918\
 Data File : BM014312.D
 Acq On : 20 Feb 2018 02:32
 Operator : SJ/JU
 Sample : J1570-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C02W4

Manual Integrations
 APPROVED

Sohil
 2/20/2018 3:14:09 PM

Quant Time: Feb 20 03:59:59 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 20 03:49:19 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	88569	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	409898	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.19	164	270119	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.95	188	614145	20.00	ng/ul	0.00
75) Chrysene-d12	21.15	240	589402	20.00	ng/ul	0.00
83) Perylene-d12	23.32	264	505857	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.11	96	14251m	6.89	ng/uL	0.00
5) Phenol-d5	6.73	99	54803	7.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.88	67	172160	37.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.07	132	171017	29.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	112791	17.22	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	120950	39.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.40	143	129065	41.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.94	165	214401m	33.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	1884	0.29	ng/ul	0.07
43) Dimethylphthalate-d6	13.61	166	868600	38.94	ng/ul	0.00
46) Acenaphthylene-d8	13.87	160	1061875	38.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	11427m	3.71	ng/ul	0.05
57) Fluorene-d10	15.19	176	761549	38.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.34	200	114679	31.13	ng/ul	0.00
70) Anthracene-d10	17.05	188	1184638	39.98	ng/ul	0.00
76) Pyrene-d10	19.35	212	1335348	43.93	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.19	264	986383	40.06	ng/ul	0.00

Target Compounds				Ovalue	
2) 1,4-Dioxane	3.15	88	6293	2.737	ng/uL#

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM021918\
Data File : BM014312.D
Acq On : 20 Feb 2018 02:32
Operator : SJ/JU
Sample : J1570-18
Misc :
ALS Vial : 16 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
C02W4

Manual Integrations
APPROVED

Sohil
2/20/2018 3:14:09 PM

Quant Time: Feb 20 03:59:59 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 20 03:49:19 2018
Response via : Initial Calibration

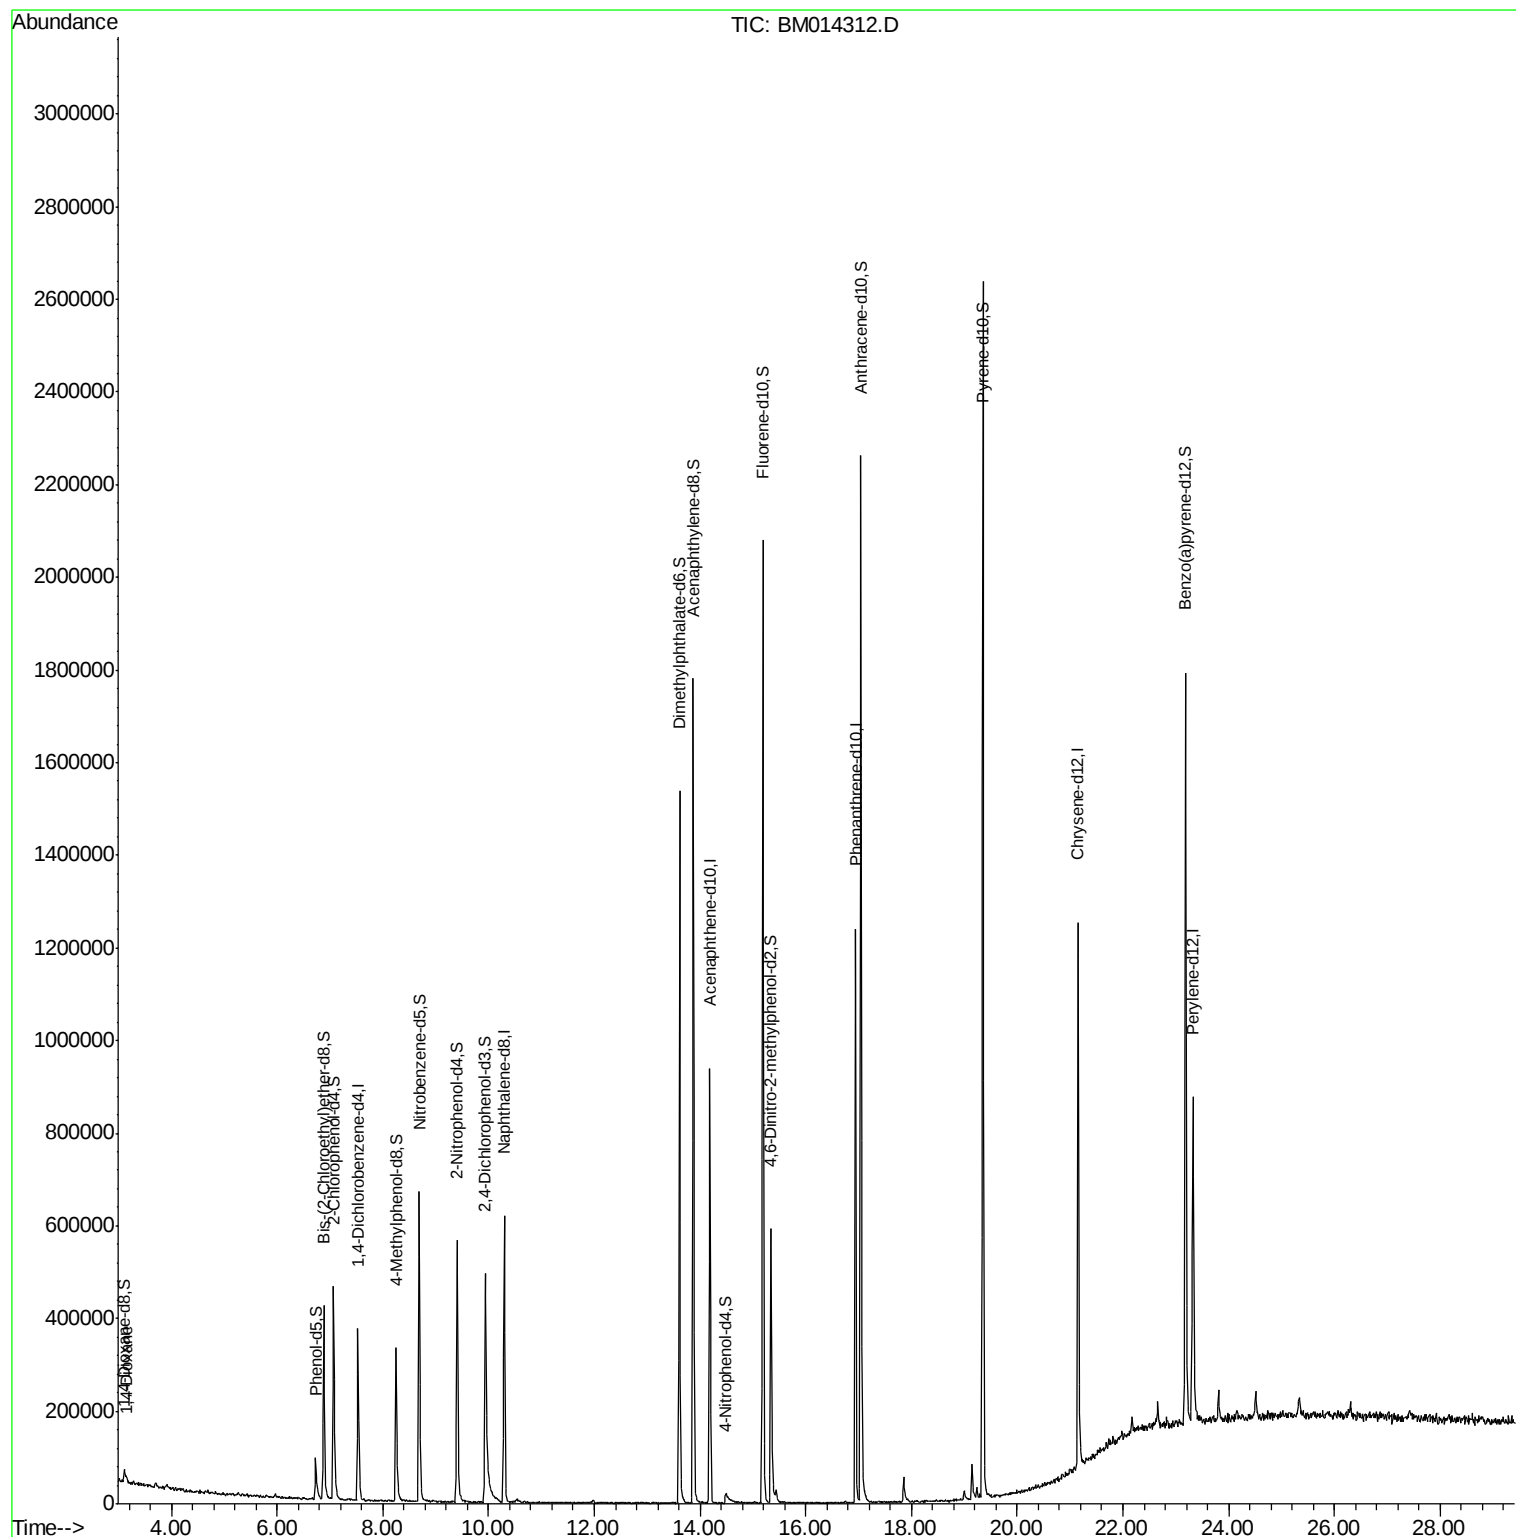

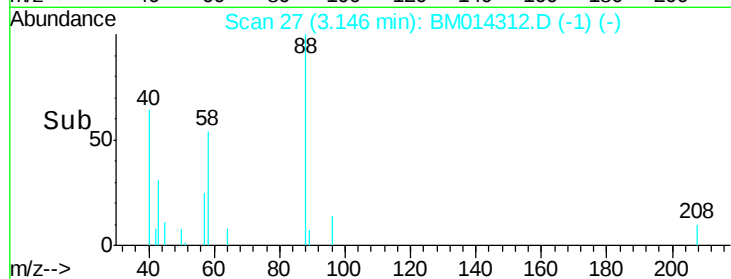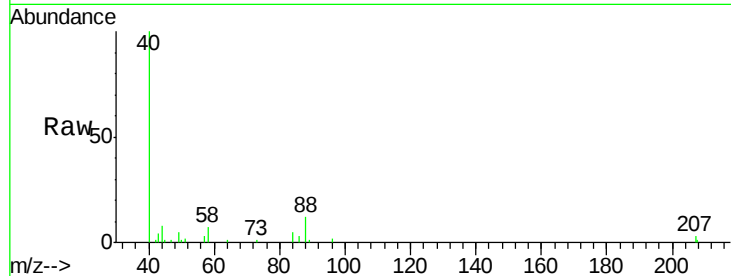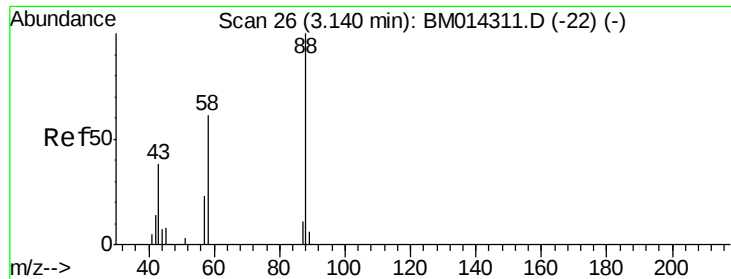

#2

1,4-Dioxane

Concen: 2.737 ng/uL

RT: 3.15 min Scan# 27

Delta R.T. 0.01 min

Lab File: BM014312.D

Acq: 20 Feb 2018 02:32

Tot Ion:	88	Resp:	6293
Ion Ratio	Lower	Upper	
88	100		
43	32.0	48.0	72.0#
58	58.4	80.0	120.0#

Instrument :

BNA_M

ClientSampleId :

C02W4

Manual Integrations
APPROVED

Sohil
2/20/2018 3:14:09 PM

