

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021920\
 Data File : BM024966.D
 Acq On : 20 Feb 2020 04:28
 Operator : CG/JU
 Sample : L1423-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5AZ3

Quant Time: Feb 20 05:46:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 19 03:36:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	331245	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.13	136	1193630	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.03	164	715679	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	1486488	20.00	ng/ul	-0.01
78) Chrysene-d12	21.00	240	1483390	20.00	ng/ul	-0.01
86) Perylene-d12	23.09	264	1612345	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.03	96	33819	4.91	ng/uL	0.00
5) Phenol-d5	6.58	99	531206	24.14	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.74	67	337897	27.19	ng/ul	-0.01
9) 2-Chlorophenol-d4	6.93	132	455967	23.13	ng/ul	-0.01
13) 4-Methylphenol-d8	8.10	113	354579	19.10	ng/ul	-0.01
19) Nitrobenzene-d5	8.52	128	211335	24.48	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.23	143	236294	23.17	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.77	165	419069	20.37	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.28	131	454402	23.61	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	1260047	23.32	ng/ul	-0.01
47) Acenaphthylene-d8	13.72	160	1520768	24.10	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.26	143	132741	15.12	ng/ul	0.00
58) Fluorene-d10	15.03	176	1098403	22.96	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.17	200	156518	16.15	ng/ul	-0.01
71) Anthracene-d10	16.89	188	1598206	23.55	ng/ul	-0.01
79) Pyrene-d10	19.19	212	1887942	25.44	ng/ul	-0.01
90) Benzo(a)pyrene-d12	22.96	264	2036325	25.15	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.50	163	104215	1.849	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021920\
Data File : BM024966.D
Acq On : 20 Feb 2020 04:28
Operator : CG/JU
Sample : L1423-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5AZ3

Quant Time: Feb 20 05:46:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 03:36:08 2020
Response via : Initial Calibration

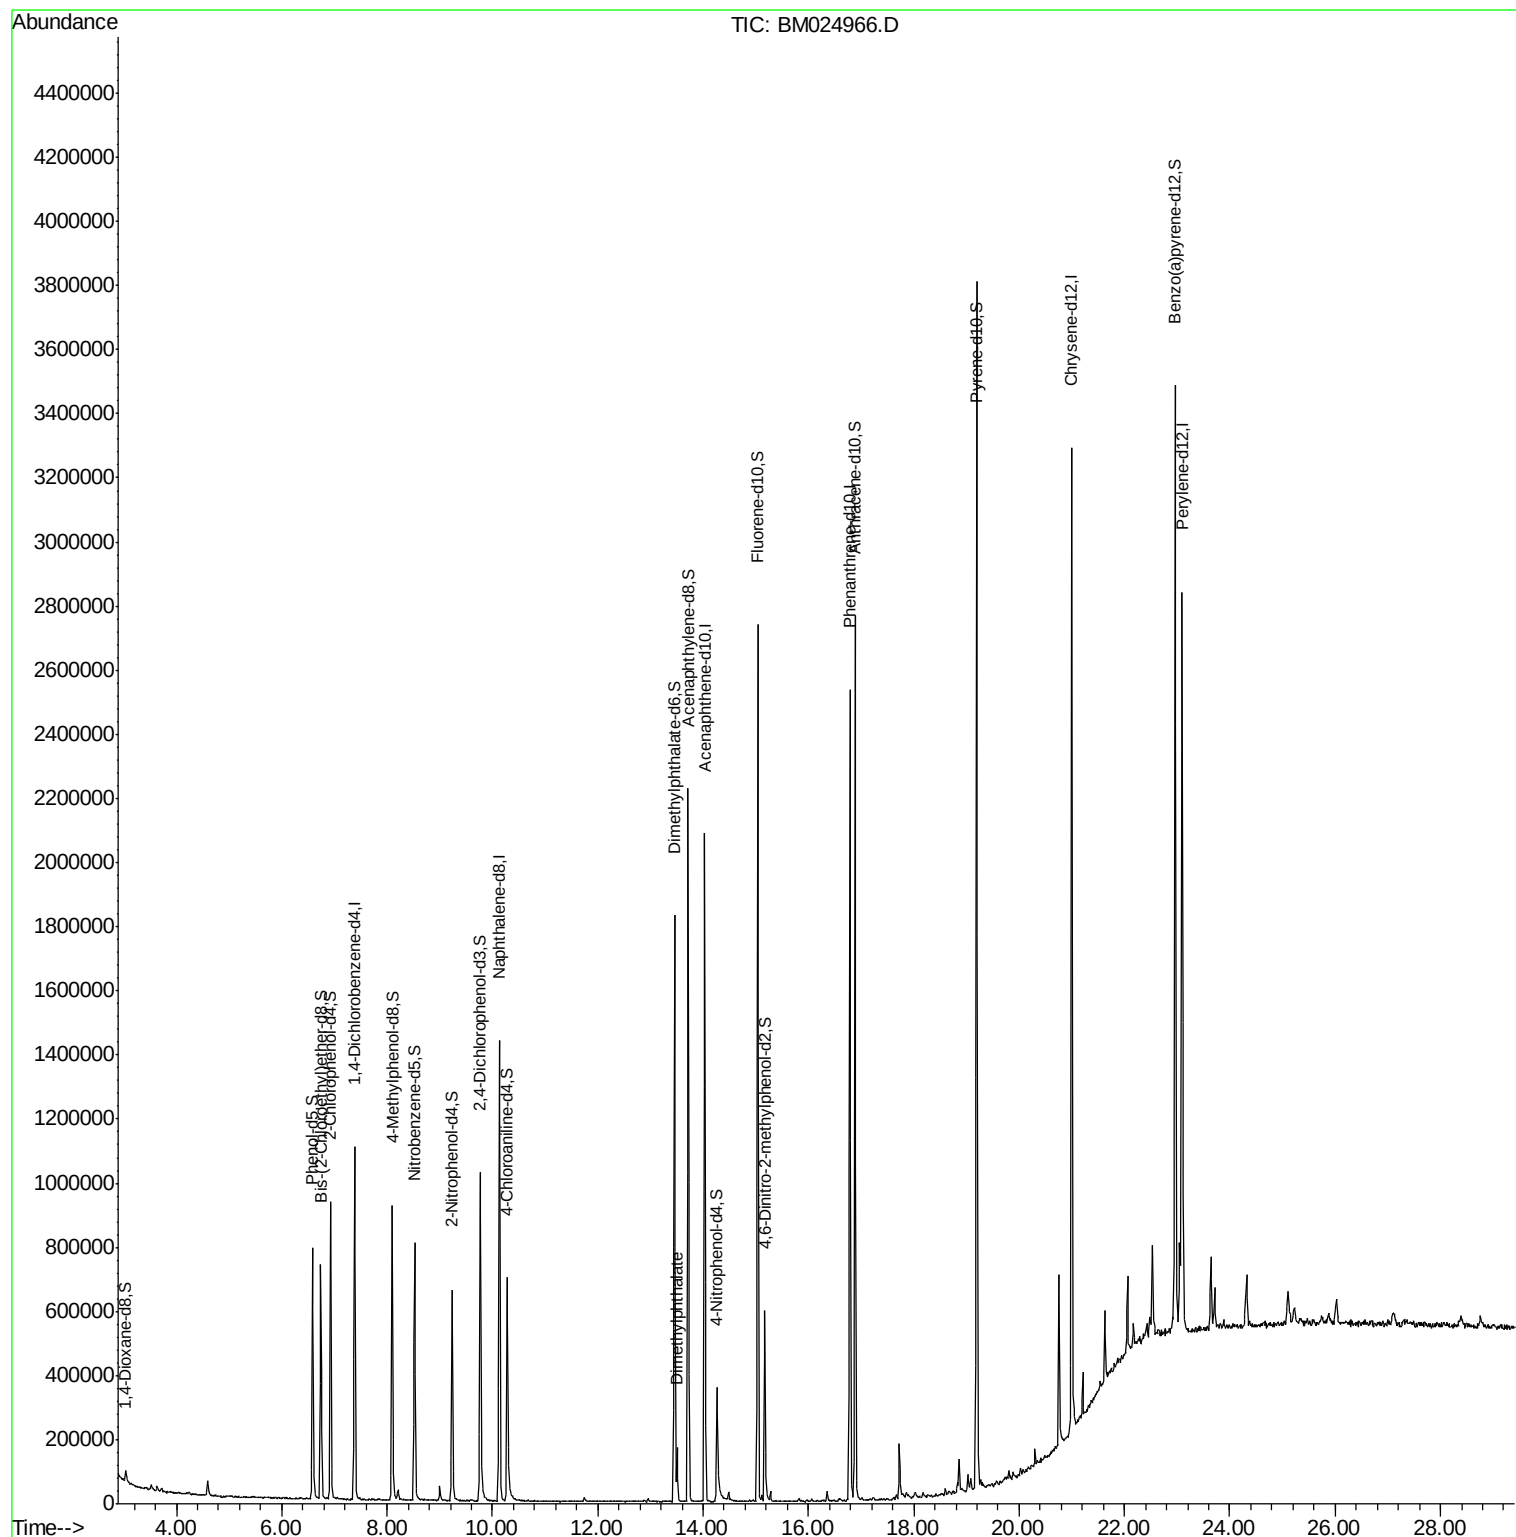

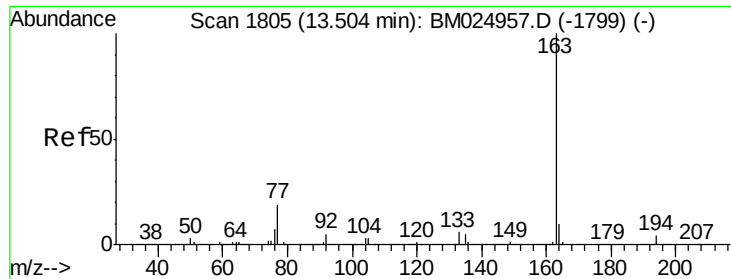

#45

Dimethylphthalate

Concen: 1.849 ng/ul

RT: 13.50 min Scan# 1805

Delta R.T. -0.01 min

Lab File: BM024966.D

Acq: 20 Feb 2020 04:28

Instrument :

BNA_M

ClientSampleId :

C5AZ3


Tot Ion:163 Resp: 104215

Ion Ratio Lower Upper

163 100

194 4.5 3.5 5.3

164 10.6 8.2 12.2

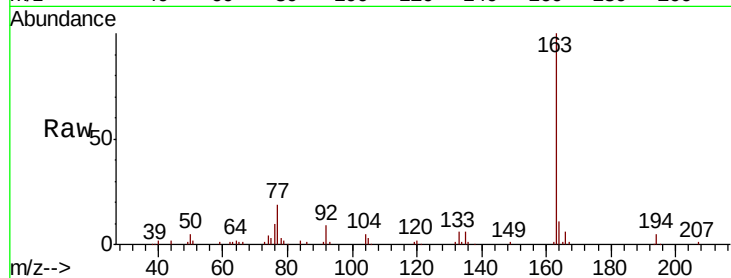

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

