

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021920\
 Data File : BM024972.D
 Acq On : 20 Feb 2020 08:03
 Operator : CG/JU
 Sample : L1423-15
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5B17

Quant Time: Feb 20 09:56:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 19 03:36:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	368026	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.13	136	1319180	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.03	164	775496	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.79	188	1604085	20.00	ng/ul	-0.01
78) Chrysene-d12	21.00	240	1608029	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	1779722	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.03	96	30953	4.05	ng/uL	0.00
5) Phenol-d5	6.58	99	482939	19.75	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.74	67	315716	22.86	ng/ul	-0.01
9) 2-Chlorophenol-d4	6.93	132	417334	19.05	ng/ul	-0.01
13) 4-Methylphenol-d8	8.10	113	307943	14.93	ng/ul	-0.01
19) Nitrobenzene-d5	8.52	128	196379	20.59	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.23	143	216182	19.18	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.77	165	390240	17.16	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.28	131	416988	19.61	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	1164969	19.90	ng/ul	-0.01
47) Acenaphthylene-d8	13.72	160	1399676	20.47	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.26	143	99944	10.51	ng/ul	0.00
58) Fluorene-d10	15.03	176	1014843	19.58	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.17	200	132834	12.70	ng/ul	-0.01
71) Anthracene-d10	16.89	188	1490263	20.35	ng/ul	-0.01
79) Pyrene-d10	19.19	212	1700045	21.14	ng/ul	-0.01
90) Benzo(a)pyrene-d12	22.97	264	1866208	20.88	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.50	163	175434	2.873	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021920\
Data File : BM024972.D
Acq On : 20 Feb 2020 08:03
Operator : CG/JU
Sample : L1423-15
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5B17

Quant Time: Feb 20 09:56:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 03:36:08 2020
Response via : Initial Calibration

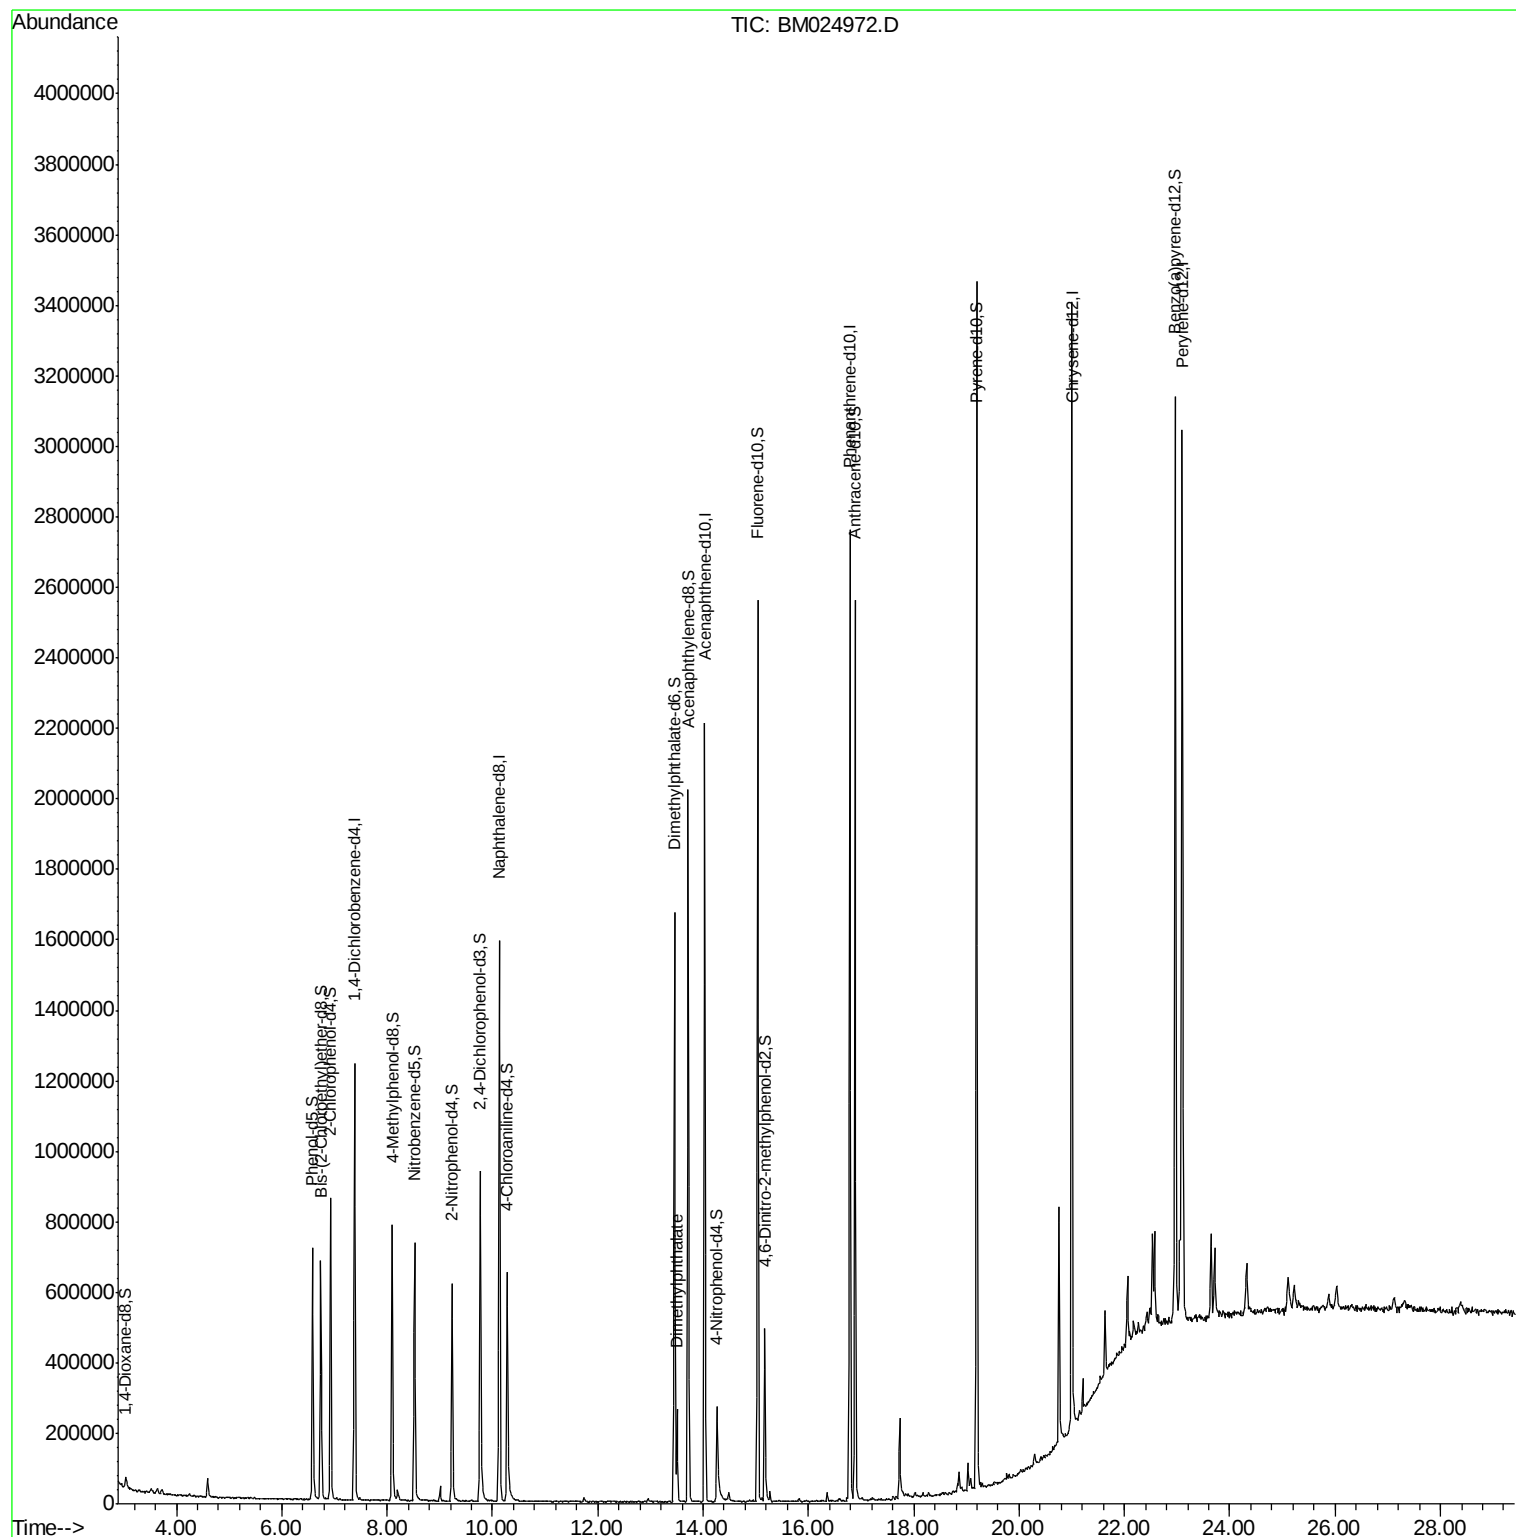

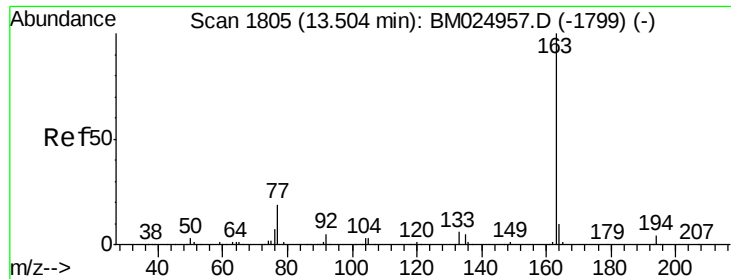

#45

Dimethylphthalate

Concen: 2.873 ng/ul

RT: 13.50 min Scan# 1805

Delta R.T. -0.01 min

Lab File: BM024972.D

Acq: 20 Feb 2020 08:03

Instrument :

BNA_M

ClientSampleId :

C5B17


Tot Ion:163 Resp: 175434

Ion Ratio Lower Upper

163 100

194 4.7 3.5 5.3

164 10.3 8.2 12.2

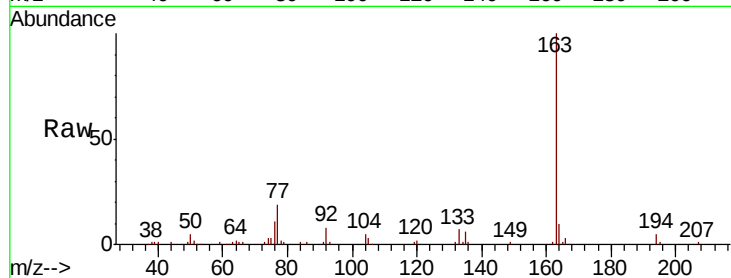

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

