

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021920\  
 Data File : BM024946.D  
 Acq On : 19 Feb 2020 16:28  
 Operator : CG/JU  
 Sample : PB126856BL  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SBLK56

## Integration Parameters: LSCINT.P

Integrator: RTE  
 Smoothing : OFF  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0

Filtering: 5  
 Min Area: 0.1 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
 Title : SVOA CALIBRATION

Signal : TIC

| peak # | R.T. min | first scan | max scan | last scan | PK TY | peak height | corr. area | corr. % max. | % of total |
|--------|----------|------------|----------|-----------|-------|-------------|------------|--------------|------------|
| 1      | 3.034    | 21         | 25       | 34        | rBV   | 43493       | 89683      | 1.56%        | 0.148%     |
| 2      | 3.646    | 124        | 129      | 131       | rBV2  | 11321       | 18468      | 0.32%        | 0.030%     |
| 3      | 3.704    | 137        | 139      | 142       | rBV3  | 5546        | 6084       | 0.11%        | 0.010%     |
| 4      | 4.246    | 228        | 231      | 235       | rVB6  | 6530        | 8901       | 0.15%        | 0.015%     |
| 5      | 4.593    | 286        | 290      | 296       | rBV   | 33222       | 56123      | 0.98%        | 0.092%     |
| 6      | 5.440    | 428        | 434      | 437       | rBV5  | 6097        | 11139      | 0.19%        | 0.018%     |
| 7      | 6.587    | 620        | 629      | 643       | rBV   | 957527      | 1555813    | 27.04%       | 2.561%     |
| 8      | 6.740    | 649        | 655      | 671       | rBV   | 810317      | 1339973    | 23.29%       | 2.206%     |
| 9      | 6.928    | 680        | 687      | 698       | rBV   | 1118862     | 1816339    | 31.57%       | 2.990%     |
| 10     | 7.040    | 703        | 706      | 712       | rVB5  | 4260        | 8594       | 0.15%        | 0.014%     |
| 11     | 7.387    | 758        | 765      | 776       | rBV   | 1066888     | 1709914    | 29.72%       | 2.815%     |
| 12     | 8.098    | 880        | 886      | 900       | rBV   | 1246825     | 1957172    | 34.02%       | 3.222%     |
| 13     | 8.522    | 952        | 958      | 968       | rBV   | 945979      | 1543176    | 26.82%       | 2.541%     |
| 14     | 9.239    | 1073       | 1080     | 1090      | rBV   | 782340      | 1284598    | 22.33%       | 2.115%     |
| 15     | 9.775    | 1164       | 1171     | 1184      | rBV   | 1193643     | 2081226    | 36.17%       | 3.426%     |
| 16     | 10.139   | 1224       | 1233     | 1241      | rBV   | 1324645     | 2206467    | 38.35%       | 3.633%     |
| 17     | 10.281   | 1249       | 1257     | 1271      | rBV   | 939269      | 1856032    | 32.26%       | 3.056%     |
| 18     | 11.745   | 1499       | 1506     | 1515      | rBV2  | 12551       | 27032      | 0.47%        | 0.045%     |
| 19     | 13.463   | 1791       | 1798     | 1810      | rBV   | 1981783     | 2888377    | 50.20%       | 4.755%     |
| 20     | 13.721   | 1834       | 1842     | 1857      | rBV   | 2410073     | 3581197    | 62.24%       | 5.896%     |
| 21     | 14.033   | 1888       | 1895     | 1904      | rBV2  | 2052357     | 2878677    | 50.03%       | 4.739%     |
| 22     | 14.263   | 1928       | 1934     | 1955      | rBV   | 498092      | 1000131    | 17.38%       | 1.647%     |
| 23     | 14.510   | 1973       | 1976     | 1982      | rVB4  | 9174        | 13318      | 0.23%        | 0.022%     |
| 24     | 15.039   | 2059       | 2066     | 2083      | rBV   | 3176734     | 4373325    | 76.01%       | 7.200%     |
| 25     | 15.174   | 2083       | 2089     | 2103      | rVV   | 701646      | 1063365    | 18.48%       | 1.751%     |
| 26     | 15.280   | 2103       | 2107     | 2113      | rVB2  | 36303       | 51935      | 0.90%        | 0.086%     |
| 27     | 15.827   | 2197       | 2200     | 2206      | rBV2  | 10259       | 13503      | 0.23%        | 0.022%     |
| 28     | 16.574   | 2323       | 2327     | 2334      | rBV2  | 7432        | 12306      | 0.21%        | 0.020%     |
| 29     | 16.792   | 2357       | 2364     | 2374      | rBV   | 2304841     | 3259607    | 56.65%       | 5.367%     |
| 30     | 16.886   | 2374       | 2380     | 2400      | rVB2  | 3315416     | 4793425    | 83.31%       | 7.892%     |
| 31     | 17.745   | 2521       | 2526     | 2528      | rBV4  | 9254        | 14972      | 0.26%        | 0.025%     |
| 32     | 17.768   | 2528       | 2530     | 2537      | rVB3  | 13602       | 20628      | 0.36%        | 0.034%     |
| 33     | 18.833   | 2708       | 2711     | 2716      | rBV   | 33494       | 38126      | 0.66%        | 0.063%     |
| 34     | 19.039   | 2743       | 2746     | 2748      | rBV3  | 8934        | 8922       | 0.16%        | 0.015%     |

## LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021920\  
Data File : BM024946.D  
Acq On : 19 Feb 2020 16:28  
Operator : CG/JU  
Sample : PB126856BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK56

## Integration Parameters: LSCINT.P

Integrator: RTE  
Smoothing : OFF  
Sampling : 1  
Start Thrs: 0.2  
Stop Thrs : 0  
Filtering: 5  
Min Area: 0.1 % of largest Peak  
Max Peaks: 100  
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
Title : SVOA CALIBRATION

|    |        |      |      |      |      |         |         |         |        |
|----|--------|------|------|------|------|---------|---------|---------|--------|
| 35 | 19.086 | 2750 | 2754 | 2758 | rVB  | 30009   | 38099   | 0.66%   | 0.063% |
| 36 | 19.198 | 2767 | 2773 | 2781 | rBV  | 4295944 | 5642919 | 98.08%  | 9.290% |
| 37 | 19.268 | 2781 | 2785 | 2791 | rVB  | 275290  | 297551  | 5.17%   | 0.490% |
| 38 | 20.645 | 3016 | 3019 | 3023 | rVB4 | 46232   | 44126   | 0.77%   | 0.073% |
| 39 | 20.968 | 3071 | 3074 | 3075 | rBV  | 46070   | 44366   | 0.77%   | 0.073% |
| 40 | 21.003 | 3075 | 3080 | 3091 | rVB  | 2870308 | 3610818 | 62.76%  | 5.945% |
| 41 | 22.974 | 3408 | 3415 | 3424 | rBV  | 3429526 | 5753644 | 100.00% | 9.473% |
| 42 | 23.103 | 3431 | 3437 | 3445 | rVB  | 2134885 | 3719269 | 64.64%  | 6.123% |


Sum of corrected areas: 60739340

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021920\  
Data File : BM024946.D  
Acq On : 19 Feb 2020 16:28  
Operator : CG/JU  
Sample : PB126856BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK56

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

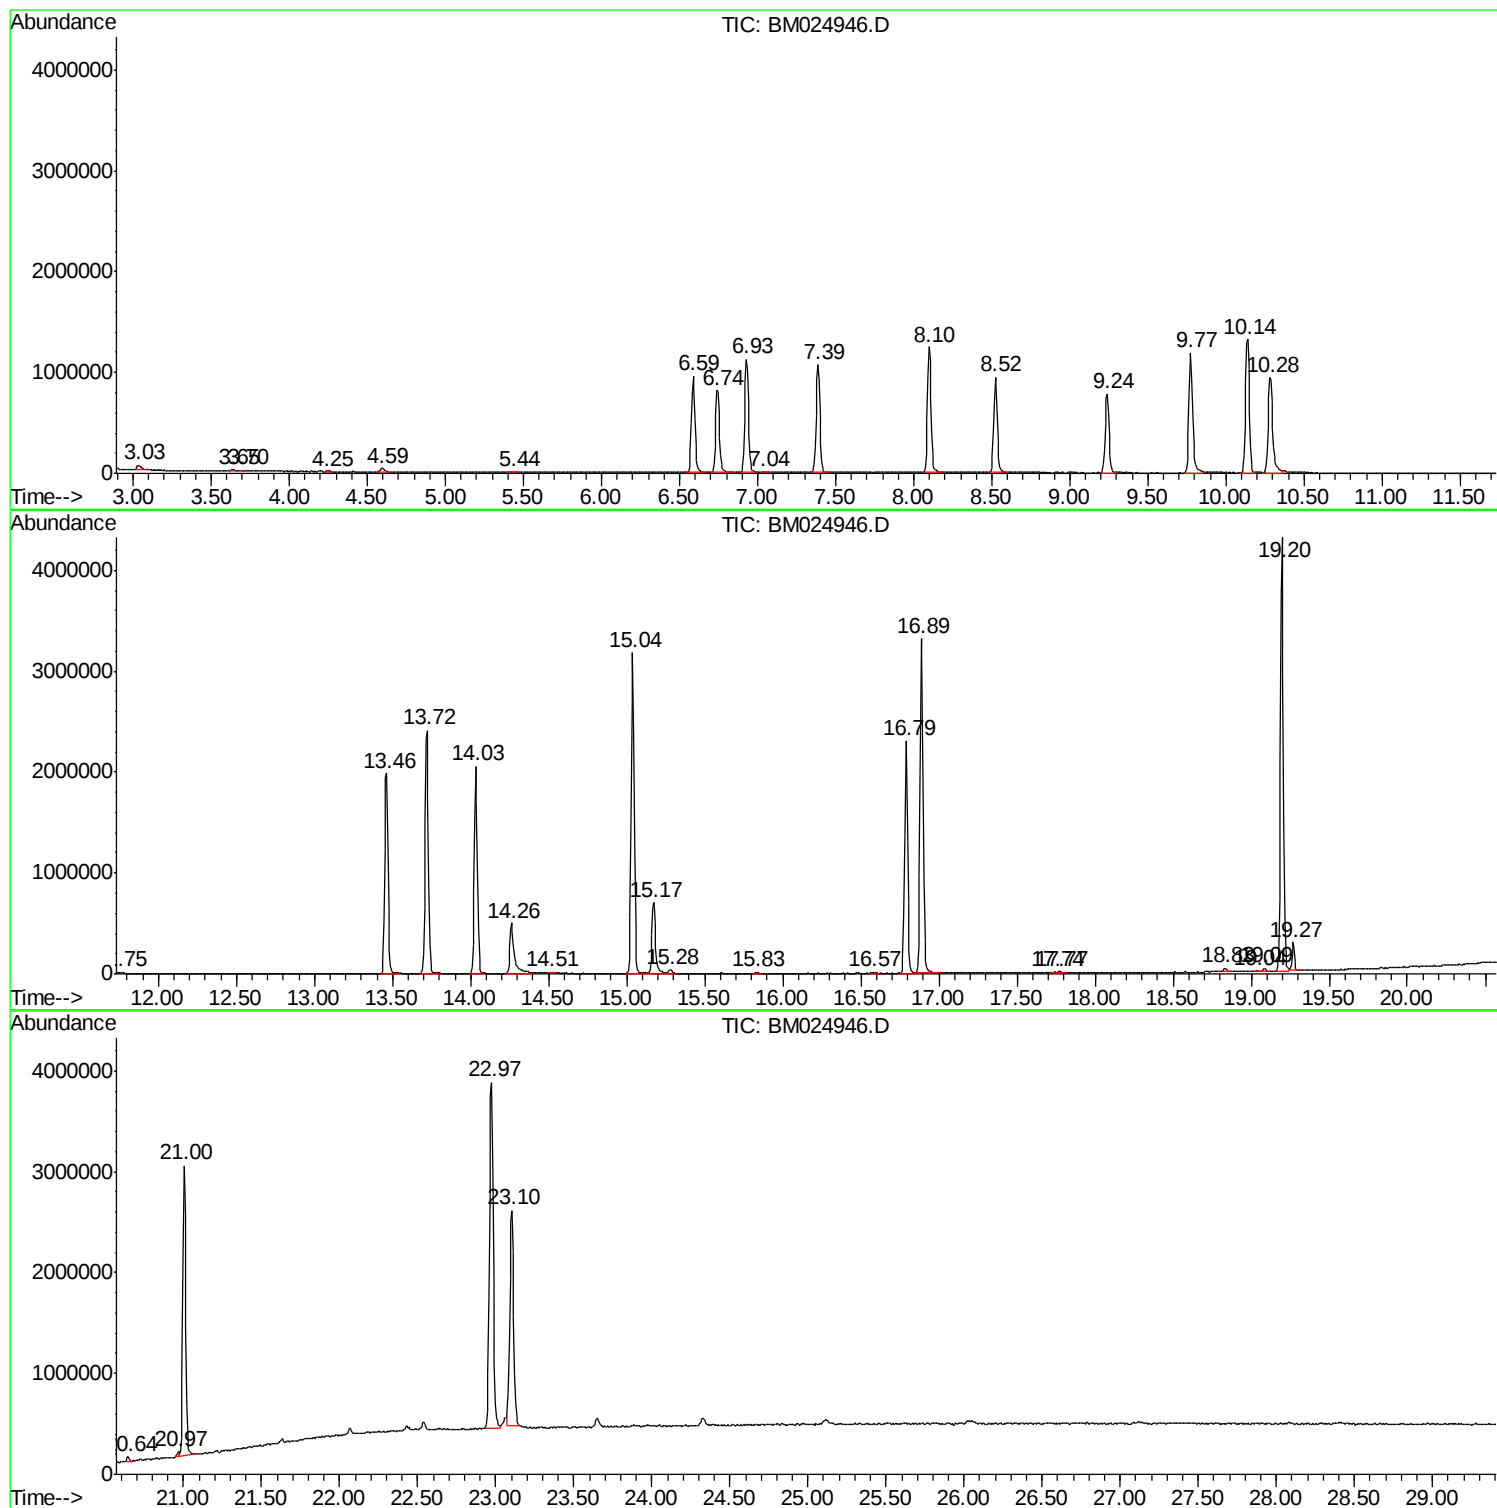

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM021920\  
Data File : BM024946.D  
Acq On : 19 Feb 2020 16:28  
Operator : CG/JU  
Sample : PB126856BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK56

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM021920\  
Data File : BM024946.D  
Acq On : 19 Feb 2020 16:28  
Operator : CG/JU  
Sample : PB126856BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK56

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |