

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021920\  
 Data File : BM024951.D  
 Acq On : 19 Feb 2020 19:29  
 Operator : CG/JU  
 Sample : L1486-17  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DBCW9

## Integration Parameters: LSCINT.P

Integrator: RTE  
 Smoothing : OFF  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0

Filtering: 5  
 Min Area: 0.1 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
 Title : SVOA CALIBRATION

Signal : TIC

| peak # | R.T. min | first scan | max scan | last scan | PK TY | peak height | corr. area | corr. % max. | % of total |
|--------|----------|------------|----------|-----------|-------|-------------|------------|--------------|------------|
| 1      | 3.034    | 21         | 25       | 36        | rVB3  | 44762       | 102652     | 1.58%        | 0.165%     |
| 2      | 3.716    | 135        | 141      | 146       | rBV6  | 11556       | 23794      | 0.37%        | 0.038%     |
| 3      | 4.116    | 207        | 209      | 216       | rBV5  | 5500        | 10059      | 0.15%        | 0.016%     |
| 4      | 6.587    | 623        | 629      | 644       | rBV   | 222595      | 394017     | 6.05%        | 0.633%     |
| 5      | 6.739    | 649        | 655      | 667       | rBV   | 890031      | 1486375    | 22.81%       | 2.388%     |
| 6      | 6.928    | 680        | 687      | 696       | rBV   | 1000734     | 1638190    | 25.14%       | 2.632%     |
| 7      | 7.386    | 758        | 765      | 778       | rBV   | 1084951     | 1731665    | 26.58%       | 2.782%     |
| 8      | 8.098    | 880        | 886      | 898       | rBV   | 700752      | 1113901    | 17.10%       | 1.790%     |
| 9      | 8.522    | 951        | 958      | 975       | rBV   | 1058294     | 1772272    | 27.20%       | 2.847%     |
| 10     | 9.016    | 1037       | 1042     | 1045      | rVB2  | 19008       | 27827      | 0.43%        | 0.045%     |
| 11     | 9.239    | 1073       | 1080     | 1093      | rBV   | 870090      | 1466191    | 22.50%       | 2.355%     |
| 12     | 9.775    | 1164       | 1171     | 1188      | rBV   | 1164678     | 2229017    | 34.21%       | 3.581%     |
| 13     | 10.139   | 1225       | 1233     | 1244      | rBV   | 1303841     | 2186865    | 33.57%       | 3.513%     |
| 14     | 10.298   | 1253       | 1260     | 1271      | rBV2  | 33802       | 80691      | 1.24%        | 0.130%     |
| 15     | 11.751   | 1501       | 1507     | 1517      | rVB2  | 14965       | 34288      | 0.53%        | 0.055%     |
| 16     | 13.463   | 1791       | 1798     | 1803      | rBV   | 2384213     | 3420713    | 52.50%       | 5.495%     |
| 17     | 13.510   | 1803       | 1806     | 1812      | rVB   | 120517      | 167715     | 2.57%        | 0.269%     |
| 18     | 13.721   | 1835       | 1842     | 1853      | rBV   | 2875487     | 4208484    | 64.60%       | 6.761%     |
| 19     | 14.033   | 1888       | 1895     | 1907      | rBV   | 1945348     | 2794673    | 42.90%       | 4.490%     |
| 20     | 14.274   | 1931       | 1936     | 1957      | rBV2  | 50582       | 174499     | 2.68%        | 0.280%     |
| 21     | 15.039   | 2059       | 2066     | 2077      | rBV   | 3843992     | 5267873    | 80.86%       | 8.463%     |
| 22     | 15.174   | 2083       | 2089     | 2103      | rBV   | 826708      | 1264407    | 19.41%       | 2.031%     |
| 23     | 15.280   | 2103       | 2107     | 2115      | rVB   | 44257       | 63386      | 0.97%        | 0.102%     |
| 24     | 15.827   | 2195       | 2200     | 2205      | rBV6  | 14678       | 21151      | 0.32%        | 0.034%     |
| 25     | 16.251   | 2266       | 2272     | 2275      | rBV3  | 8300        | 11736      | 0.18%        | 0.019%     |
| 26     | 16.480   | 2306       | 2311     | 2315      | rVB4  | 6805        | 6839       | 0.10%        | 0.011%     |
| 27     | 16.580   | 2320       | 2328     | 2332      | rBV3  | 8228        | 16850      | 0.26%        | 0.027%     |
| 28     | 16.792   | 2357       | 2364     | 2374      | rBV   | 2258032     | 3181111    | 48.83%       | 5.111%     |
| 29     | 16.886   | 2374       | 2380     | 2392      | rBV   | 3876530     | 5488193    | 84.24%       | 8.817%     |
| 30     | 17.009   | 2399       | 2401     | 2409      | rVB8  | 8071        | 15784      | 0.24%        | 0.025%     |
| 31     | 17.603   | 2495       | 2502     | 2509      | rBV8  | 12963       | 25727      | 0.39%        | 0.041%     |
| 32     | 17.733   | 2519       | 2524     | 2533      | rBV2  | 126043      | 196435     | 3.02%        | 0.316%     |
| 33     | 18.015   | 2568       | 2572     | 2578      | rBV2  | 13799       | 23638      | 0.36%        | 0.038%     |
| 34     | 18.756   | 2695       | 2698     | 2700      | rBV4  | 5490        | 7047       | 0.11%        | 0.011%     |

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021920\  
 Data File : BM024951.D  
 Acq On : 19 Feb 2020 19:29  
 Operator : CG/JU  
 Sample : L1486-17  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DBCW9

## Integration Parameters: LSCINT.P

Integrator: RTE  
 Smoothing : OFF  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0

Filtering: 5  
 Min Area: 0.1 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
 Title : SVOA CALIBRATION

|    |        |      |      |      |      |         |         |         |         |
|----|--------|------|------|------|------|---------|---------|---------|---------|
| 35 | 18.833 | 2708 | 2711 | 2717 | rVB2 | 39330   | 52909   | 0.81%   | 0.085%  |
| 36 | 18.909 | 2717 | 2724 | 2726 | rBV7 | 12707   | 23612   | 0.36%   | 0.038%  |
| 37 | 19.033 | 2741 | 2745 | 2749 | rBV5 | 26833   | 46053   | 0.71%   | 0.074%  |
| 38 | 19.086 | 2750 | 2754 | 2761 | rVB  | 35031   | 55155   | 0.85%   | 0.089%  |
| 39 | 19.197 | 2766 | 2773 | 2782 | rBV  | 4963554 | 6515121 | 100.00% | 10.467% |
| 40 | 19.397 | 2805 | 2807 | 2810 | rBV3 | 6240    | 7249    | 0.11%   | 0.012%  |
| 41 | 20.762 | 3035 | 3039 | 3045 | rBV  | 217971  | 310674  | 4.77%   | 0.499%  |
| 42 | 21.003 | 3075 | 3080 | 3088 | rBV  | 2721551 | 3554976 | 54.57%  | 5.711%  |
| 43 | 21.627 | 3184 | 3186 | 3190 | rBV3 | 80882   | 88072   | 1.35%   | 0.141%  |
| 44 | 22.062 | 3257 | 3260 | 3264 | rBV2 | 127142  | 146331  | 2.25%   | 0.235%  |
| 45 | 22.180 | 3277 | 3280 | 3285 | rVB  | 200057  | 244747  | 3.76%   | 0.393%  |
| 46 | 22.533 | 3337 | 3340 | 3346 | rVB3 | 169323  | 217158  | 3.33%   | 0.349%  |
| 47 | 22.968 | 3408 | 3414 | 3424 | rVB  | 3959232 | 6451027 | 99.02%  | 10.364% |
| 48 | 23.056 | 3426 | 3429 | 3431 | rVV  | 182301  | 263973  | 4.05%   | 0.424%  |
| 49 | 23.097 | 3431 | 3436 | 3444 | rVB  | 2103708 | 3614802 | 55.48%  | 5.807%  |


Sum of corrected areas: 62245924

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021920\  
Data File : BM024951.D  
Acq On : 19 Feb 2020 19:29  
Operator : CG/JU  
Sample : L1486-17  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DBCW9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

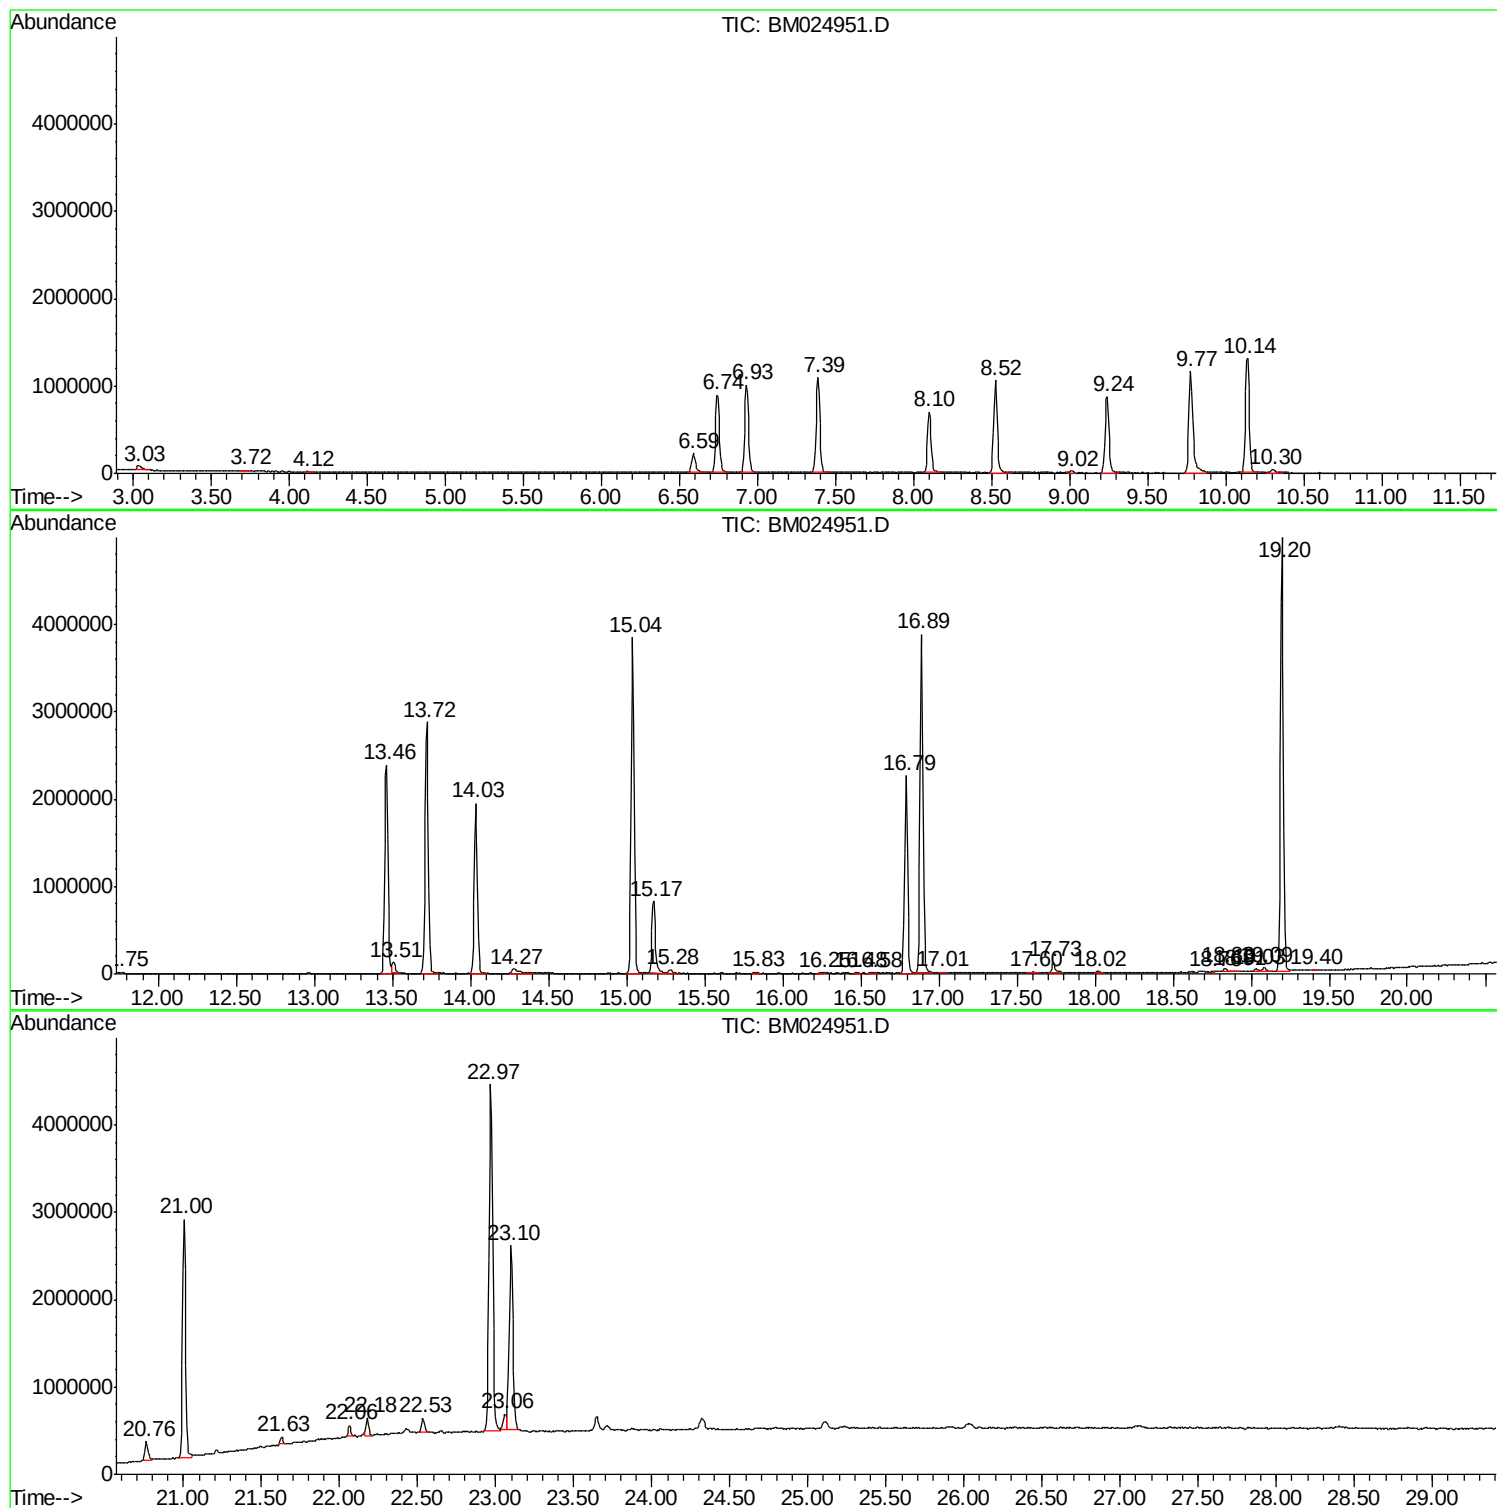

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM021920\  
Data File : BM024951.D  
Acq On : 19 Feb 2020 19:29  
Operator : CG/JU  
Sample : L1486-17  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DBCW9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM021920\  
Data File : BM024951.D  
Acq On : 19 Feb 2020 19:29  
Operator : CG/JU  
Sample : L1486-17  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DBCW9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |

-----