




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021924\
Data File : BM044182.D
Acq On : 19 Feb 2024 17:43
Operator : MA/JU
Sample : P1352-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FN6

Manual IntegrationsAPPROVED

Quant Time: Feb 19 18:17:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/20/2024
Supervised By :mohammad ahmed 02/21/2024

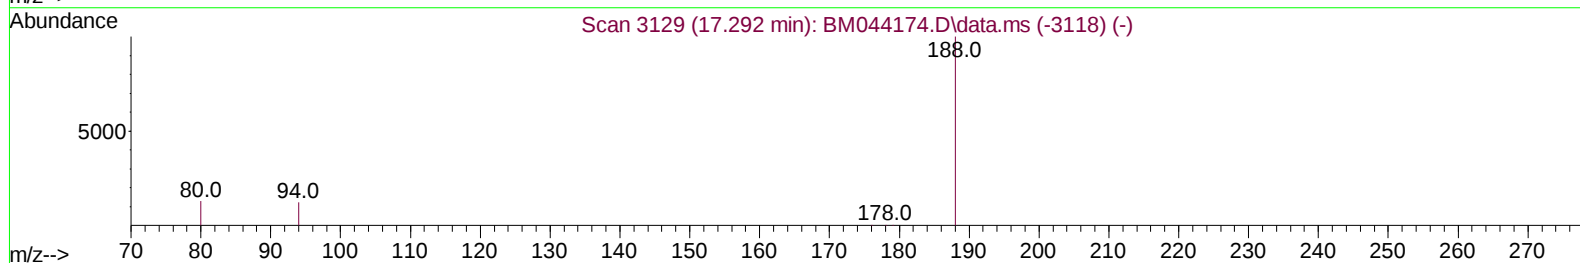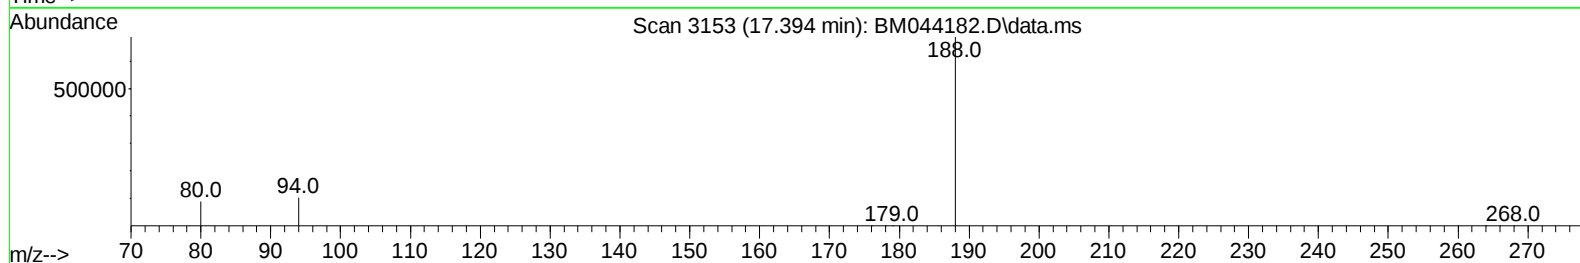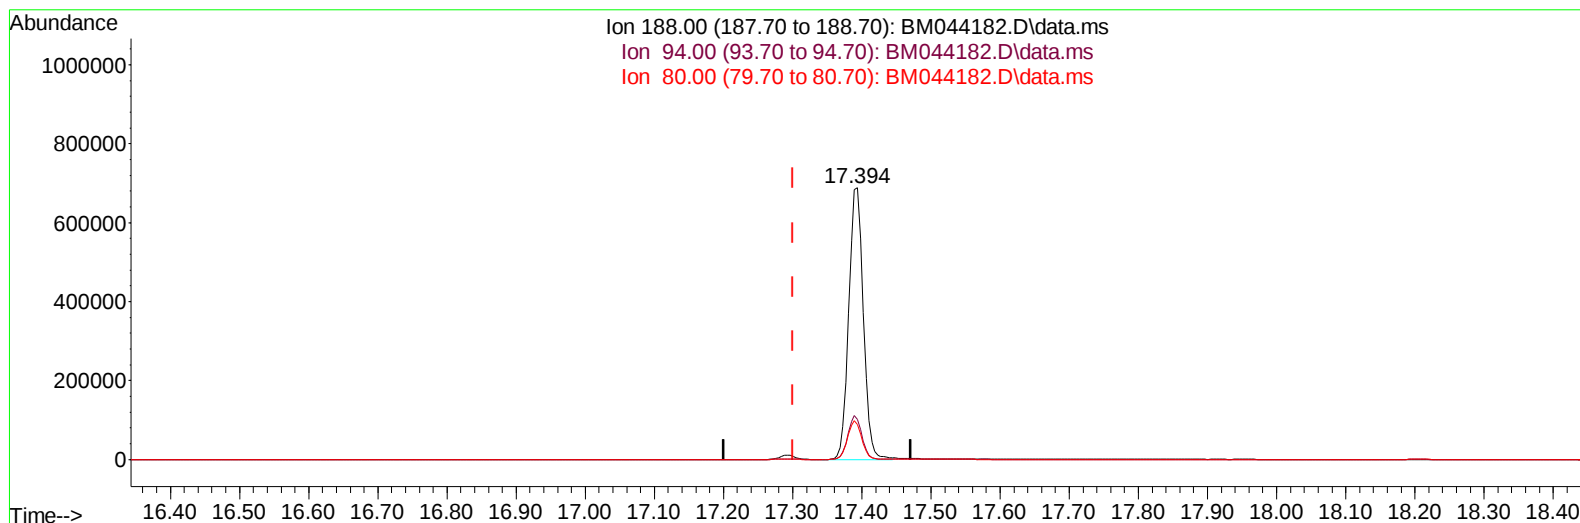

TIC: BM044182.D\data.ms

(13) Phenanthrene-d10 (I)

17.394min (+ 0.093) 0.40 ng/u1

response 1001841

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	14.77
80.00	13.40	12.81
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021924\
Data File : BM044182.D
Acq On : 19 Feb 2024 17:43
Operator : MA/JU
Sample : P1352-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FN6

Manual IntegrationsAPPROVED

Quant Time: Feb 19 18:17:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/20/2024
Supervised By :mohammad ahmed 02/21/2024

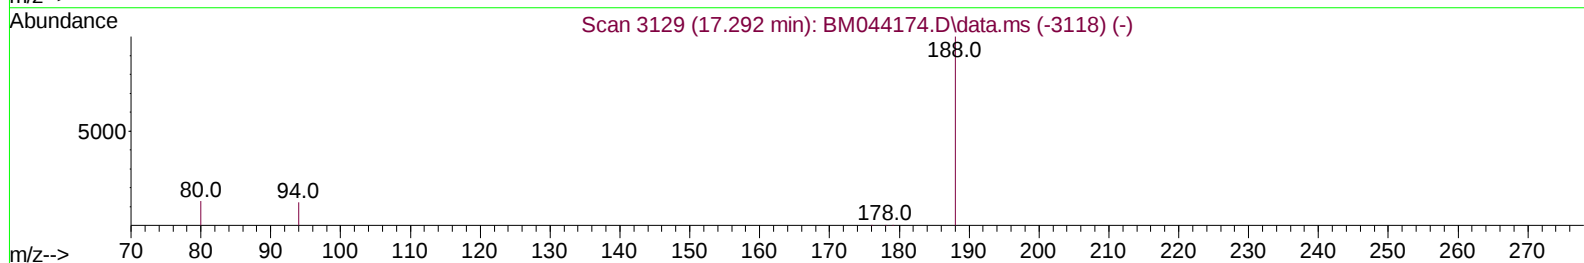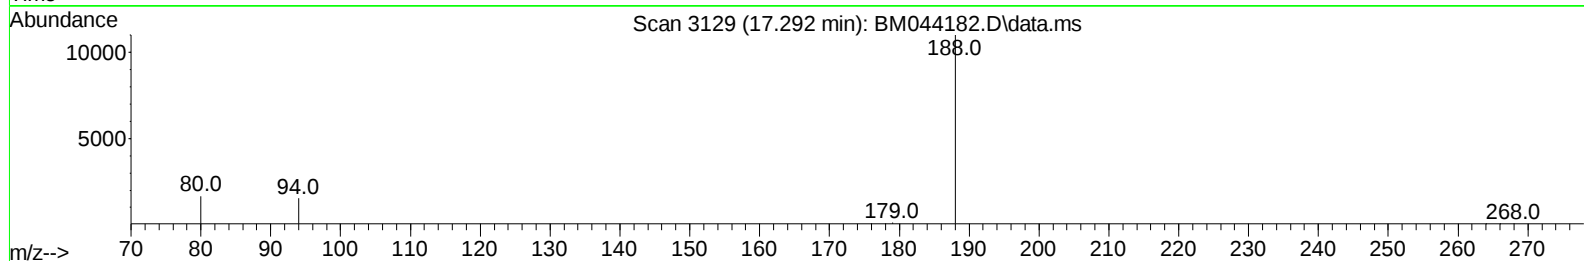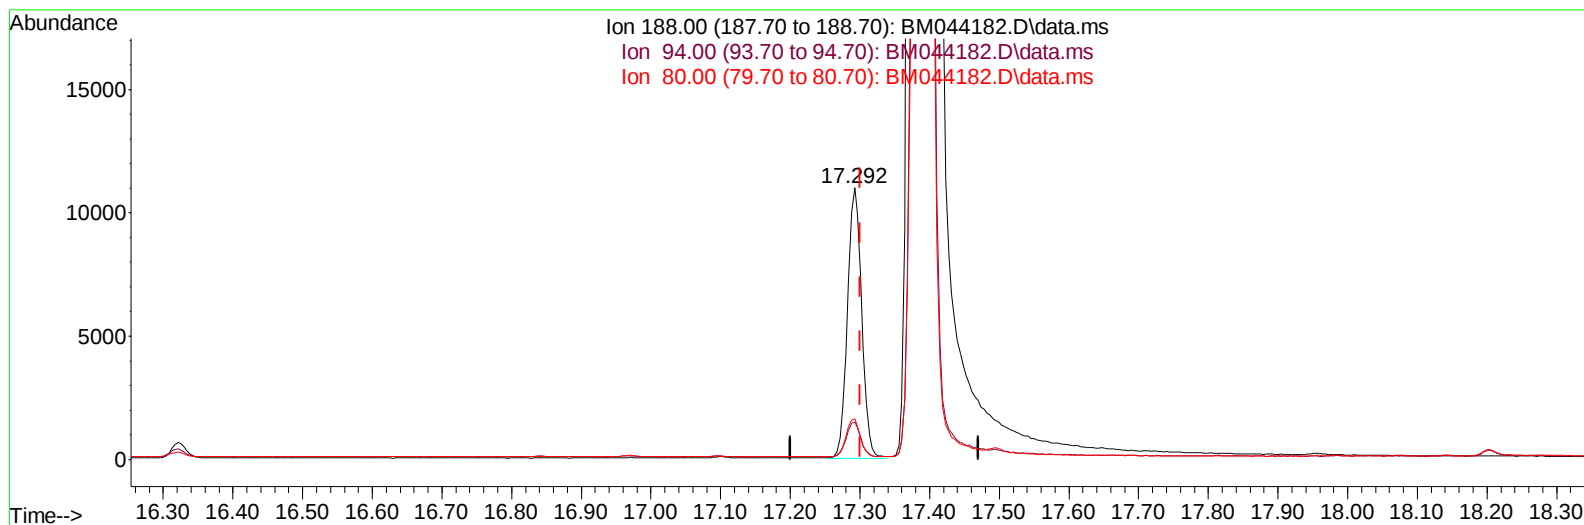

TIC: BM044182.D\data.ms

(13) Phenanthrene-d10 (I)

17.292min (-0.008) 0.40 ng/ul m

response 15507

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	13.87
80.00	13.40	14.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021924\
Data File : BM044182.D
Acq On : 19 Feb 2024 17:43
Operator : MA/JU
Sample : P1352-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COFN6

Manual IntegrationsAPPROVED

Quant Time: Feb 19 18:17:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/20/2024
Supervised By :mohammad ahmed 02/21/2024

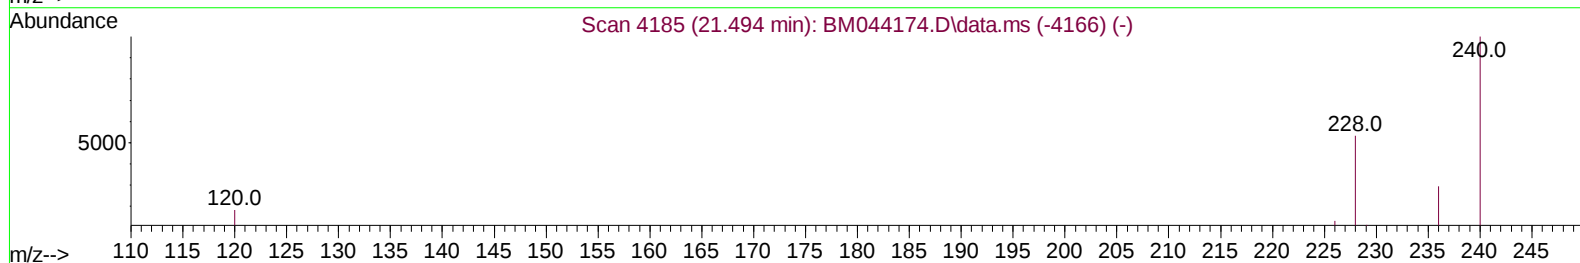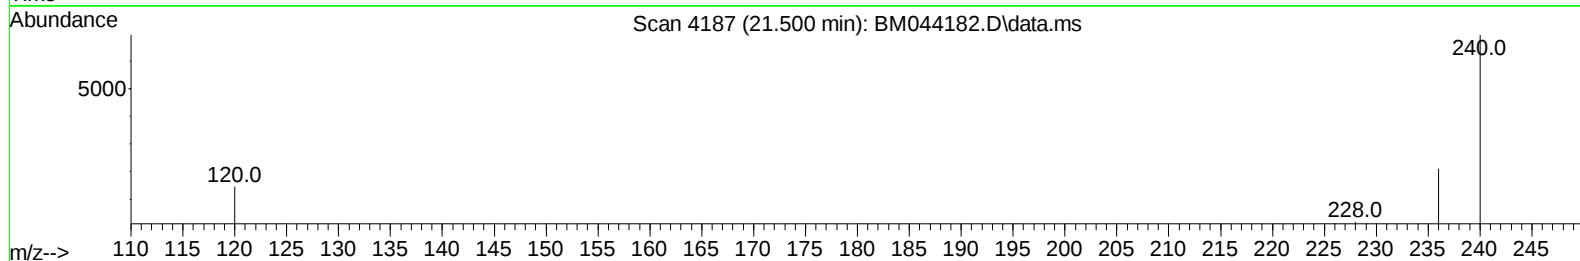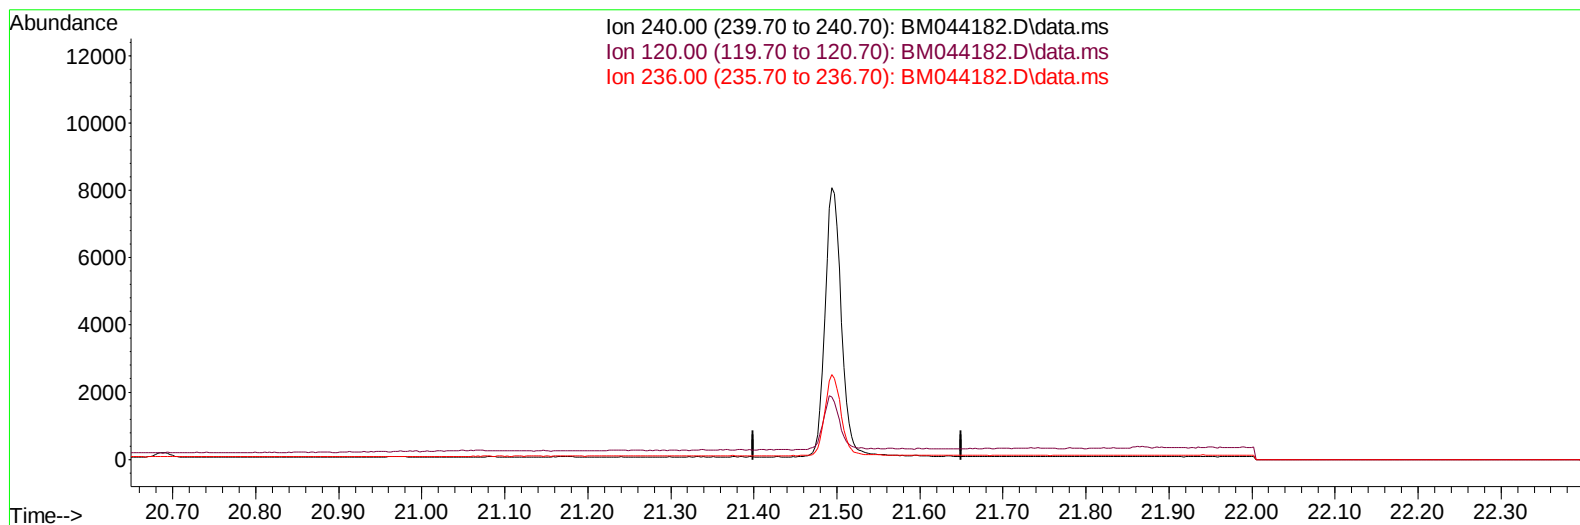

TIC: BM044182.D\data.ms

(17) Chrysene-d12

21.500min (-21.500) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.50	0.00#
236.00	30.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021924\
Data File : BM044182.D
Acq On : 19 Feb 2024 17:43
Operator : MA/JU
Sample : P1352-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FN6

Manual IntegrationsAPPROVED

Quant Time: Feb 19 18:17:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/20/2024
Supervised By :mohammad ahmed 02/21/2024

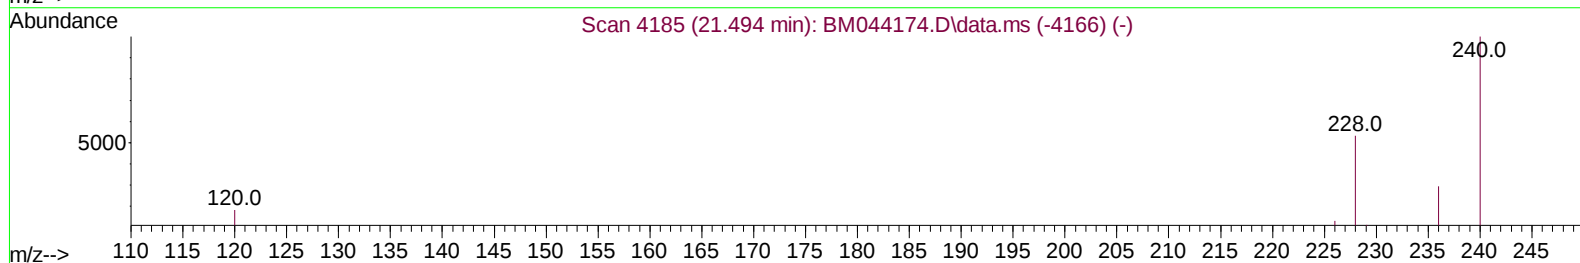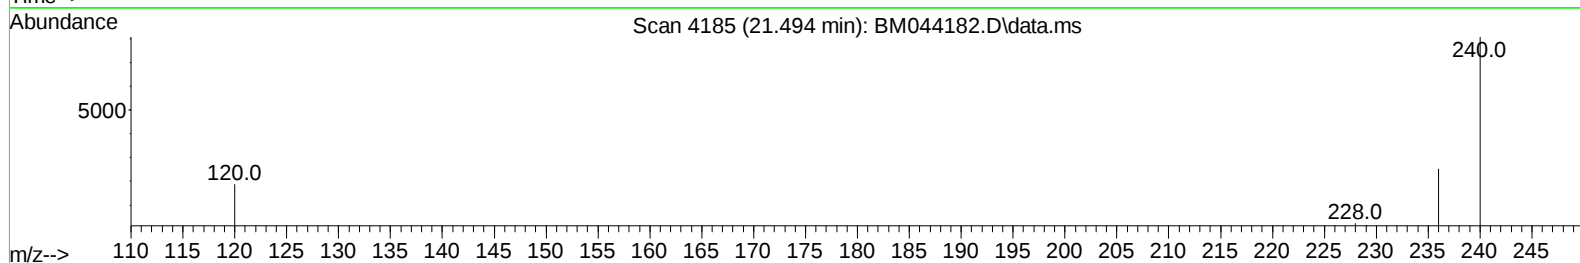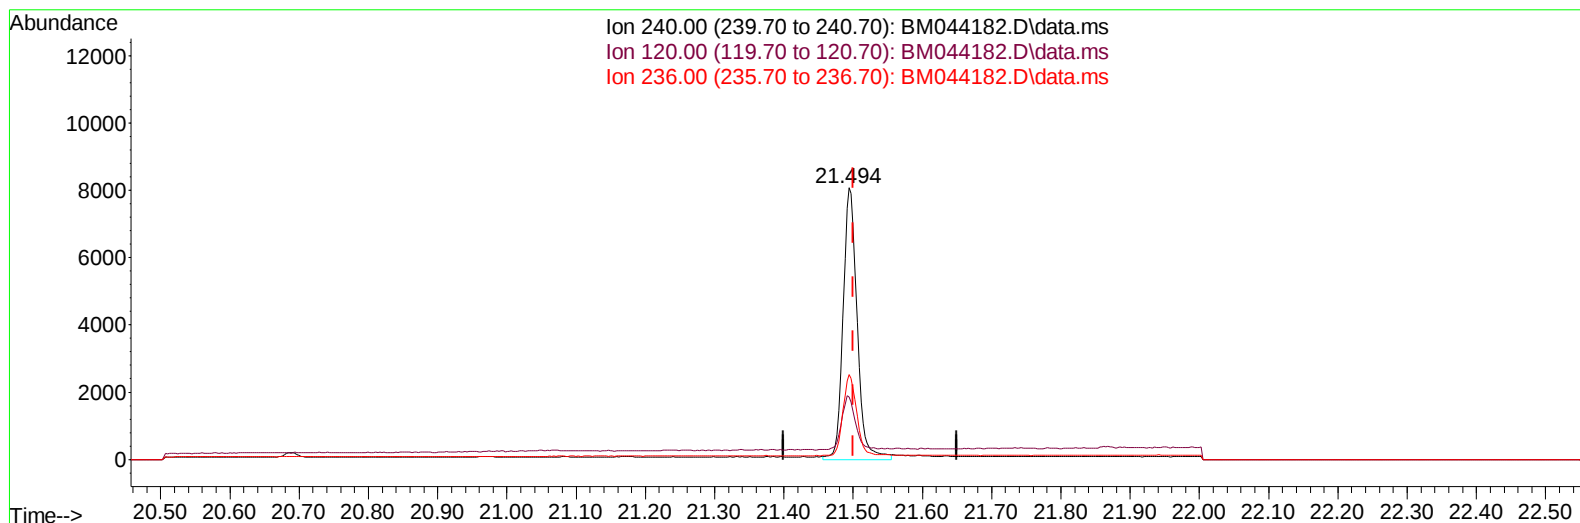

TIC: BM044182.D\data.ms

(17) Chrysene-d12

21.494min (-0.006) 0.40 ng/ul m

response 11420

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.50	23.08
236.00	30.60	31.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021924\
 Data File : BM044182.D
 Acq On : 19 Feb 2024 17:43
 Operator : MA/JU
 Sample : P1352-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0FN6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/20/2024
 Supervised By :mohammad ahmed 02/21/2024

Quant Time: Feb 19 18:17:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.896	152	5125	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	15500	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.538	164	7462	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	15507m	0.400	ng/ul	0.00
17) Chrysene-d12	21.494	240	11420m	0.400	ng/ul	0.00
23) Perylene-d12	23.885	264	16220	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	33334	4.593	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.288	152	5709	0.263	ng/ul	-0.01
18) Fluoranthene-d10	19.326	212	11485	0.337	ng/ul	0.00
Target Compounds						Qvalue
19) Fluoranthene	19.359	202	1076	0.021	ng/ul#	55

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021924\
Data File : BM044182.D
Acq On : 19 Feb 2024 17:43
Operator : MA/JU
Sample : P1352-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0FN6

Manual IntegrationsAPPROVED

Quant Time: Feb 19 18:17:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/20/2024
Supervised By :mohammad ahmed 02/21/2024

