

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021924\
 Data File : BM044186.D
 Acq On : 19 Feb 2024 20:08
 Operator : MA/JU
 Sample : P1436-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7G6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/20/2024
 Supervised By :mohammad ahmed 02/21/2024

Quant Time: Feb 19 21:55:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.896	152	5160	0.400	ng/u1	0.00
4) Naphthalene-d8	10.694	136	15592	0.400	ng/u1	-0.01
9) Acenaphthene-d10	14.538	164	7624	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.292	188	15840m	0.400	ng/u1	0.00
17) Chrysene-d12	21.497	240	11198m	0.400	ng/u1	0.00
23) Perylene-d12	23.885	264	17604	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	32431	4.438	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.288	152	9390	0.430	ng/u1	-0.01
18) Fluoranthene-d10	19.326	212	18097	0.542	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.386	88	5514	0.755	ng/u1	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021924\
Data File : BM044186.D
Acq On : 19 Feb 2024 20:08
Operator : MA/JU
Sample : P1436-02
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BH7G6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2024
Supervised By :mohammad ahmed 02/21/2024


Quant Time: Feb 19 21:55:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

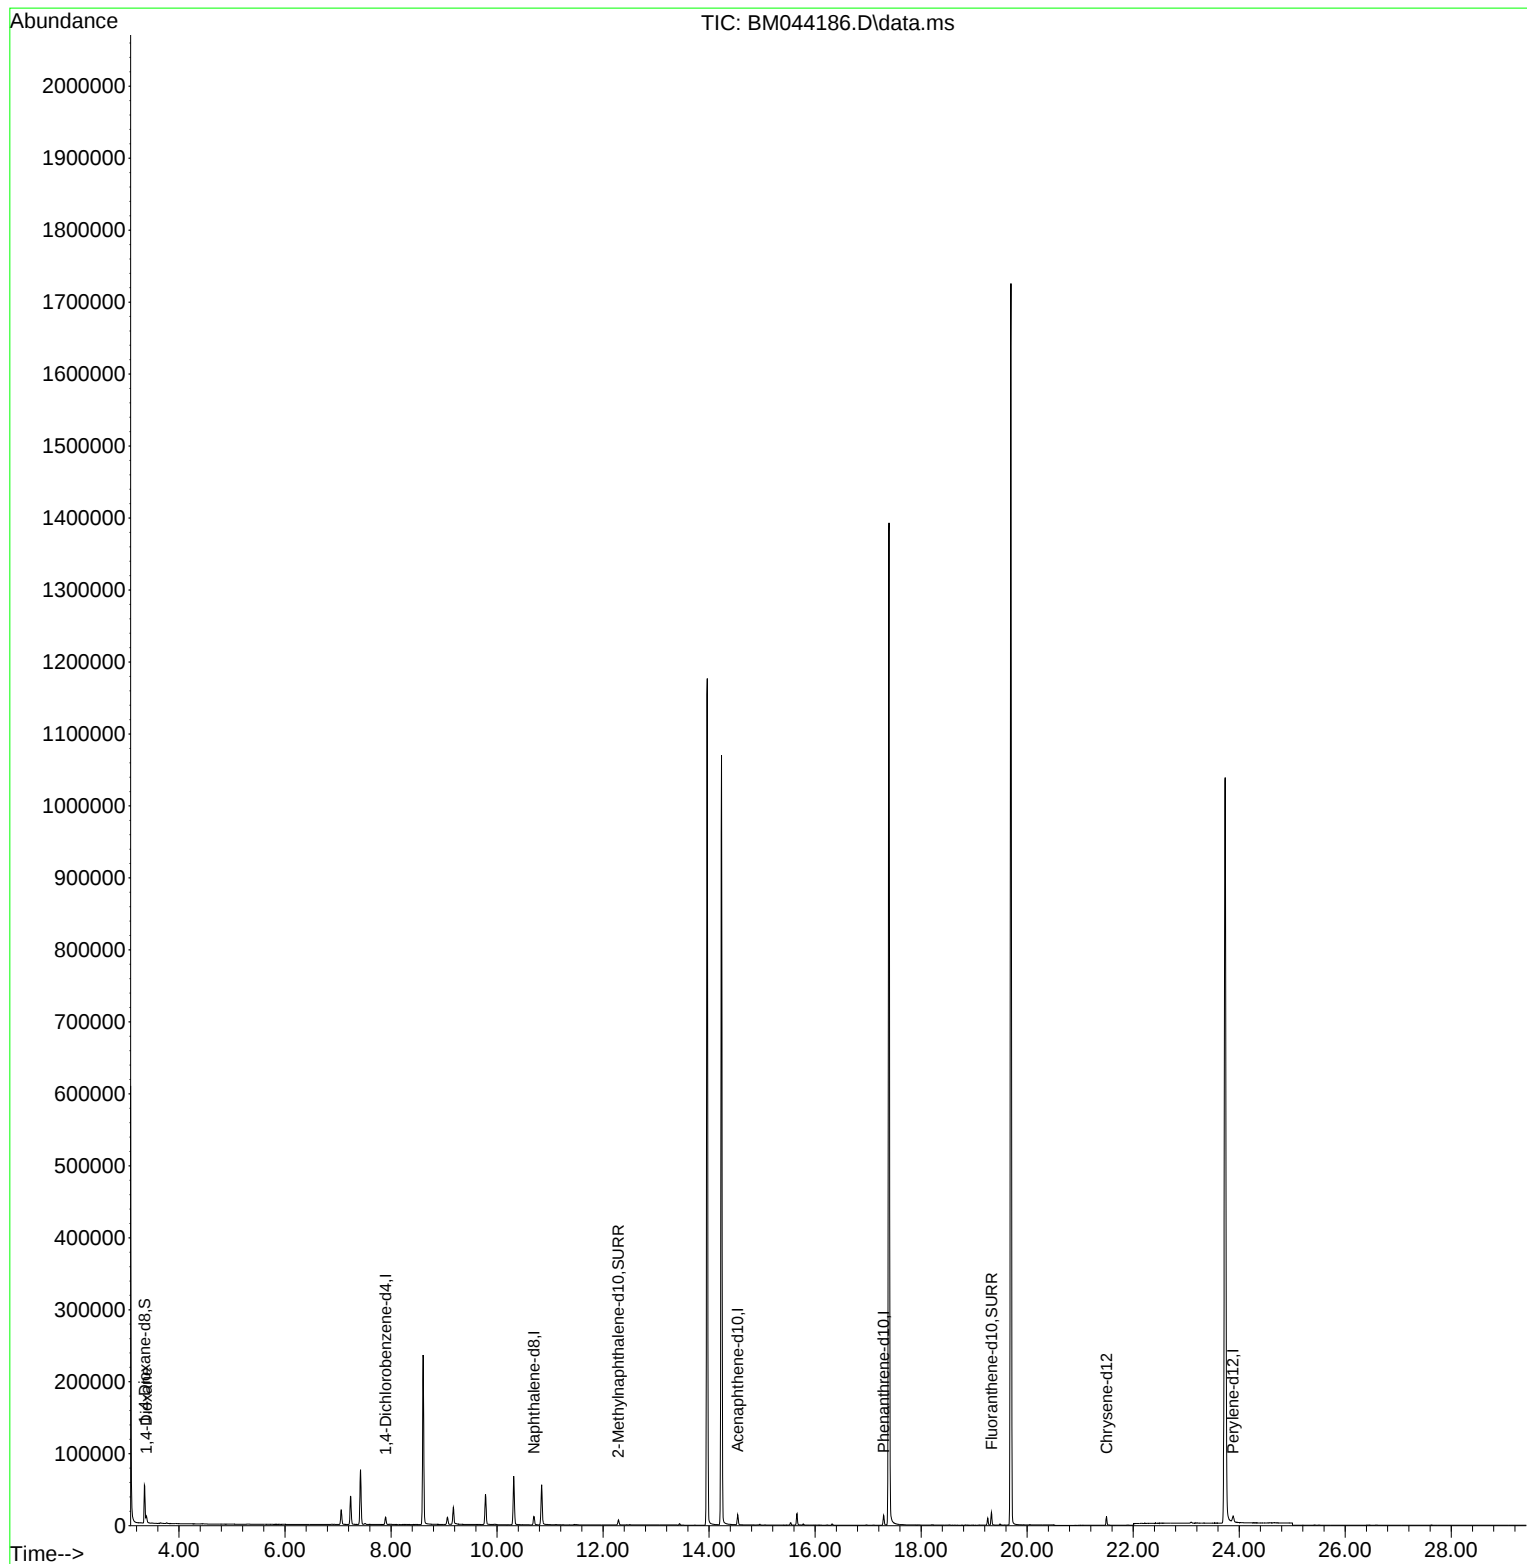

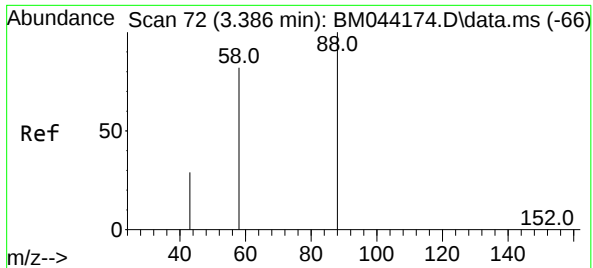

#2
 1,4-Dioxane
 Concen: 0.755 ng/ul
 RT: 3.386 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BM044186.D
 Acq: 19 Feb 2024 20:08

Instrument :
 BNA_M
 ClientSampleId :
 BH7G6

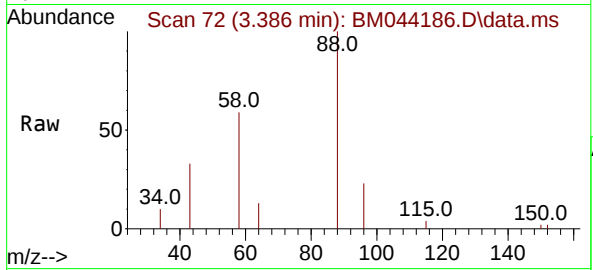

Tgt Ion: 88 Resp: 5514

Ion	Ratio	Lower	Upper
88	100		
43	33.5	32.2	48.2
58	58.6	40.6	60.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/20/2024
 Supervised By :mohammad ahmed 02/21/2024

