

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021924\
 Data File : BM044206.D
 Acq On : 20 Feb 2024 14:56
 Operator : MA/JU
 Sample : P1455-13
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2024
 Supervised By :mohammad ahmed 02/21/2024

Quant Time: Feb 20 15:53:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.896	152	4982	0.400	ng/ul	0.00
4) Naphthalene-d8	10.693	136	15244	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.538	164	7464	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.292	188	15156m	0.400	ng/ul	0.00
17) Chrysene-d12	21.497	240	10678m	0.400	ng/ul	0.00
23) Perylene-d12	23.882	264	17523	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	30860	4.374	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.288	152	9484	0.444	ng/ul	-0.01
18) Fluoranthene-d10	19.326	212	17860	0.561	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.386	88	1011	0.143	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021924\
Data File : BM044206.D
Acq On : 20 Feb 2024 14:56
Operator : MA/JU
Sample : P1455-13
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AF2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2024
Supervised By :mohammad ahmed 02/21/2024


Quant Time: Feb 20 15:53:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

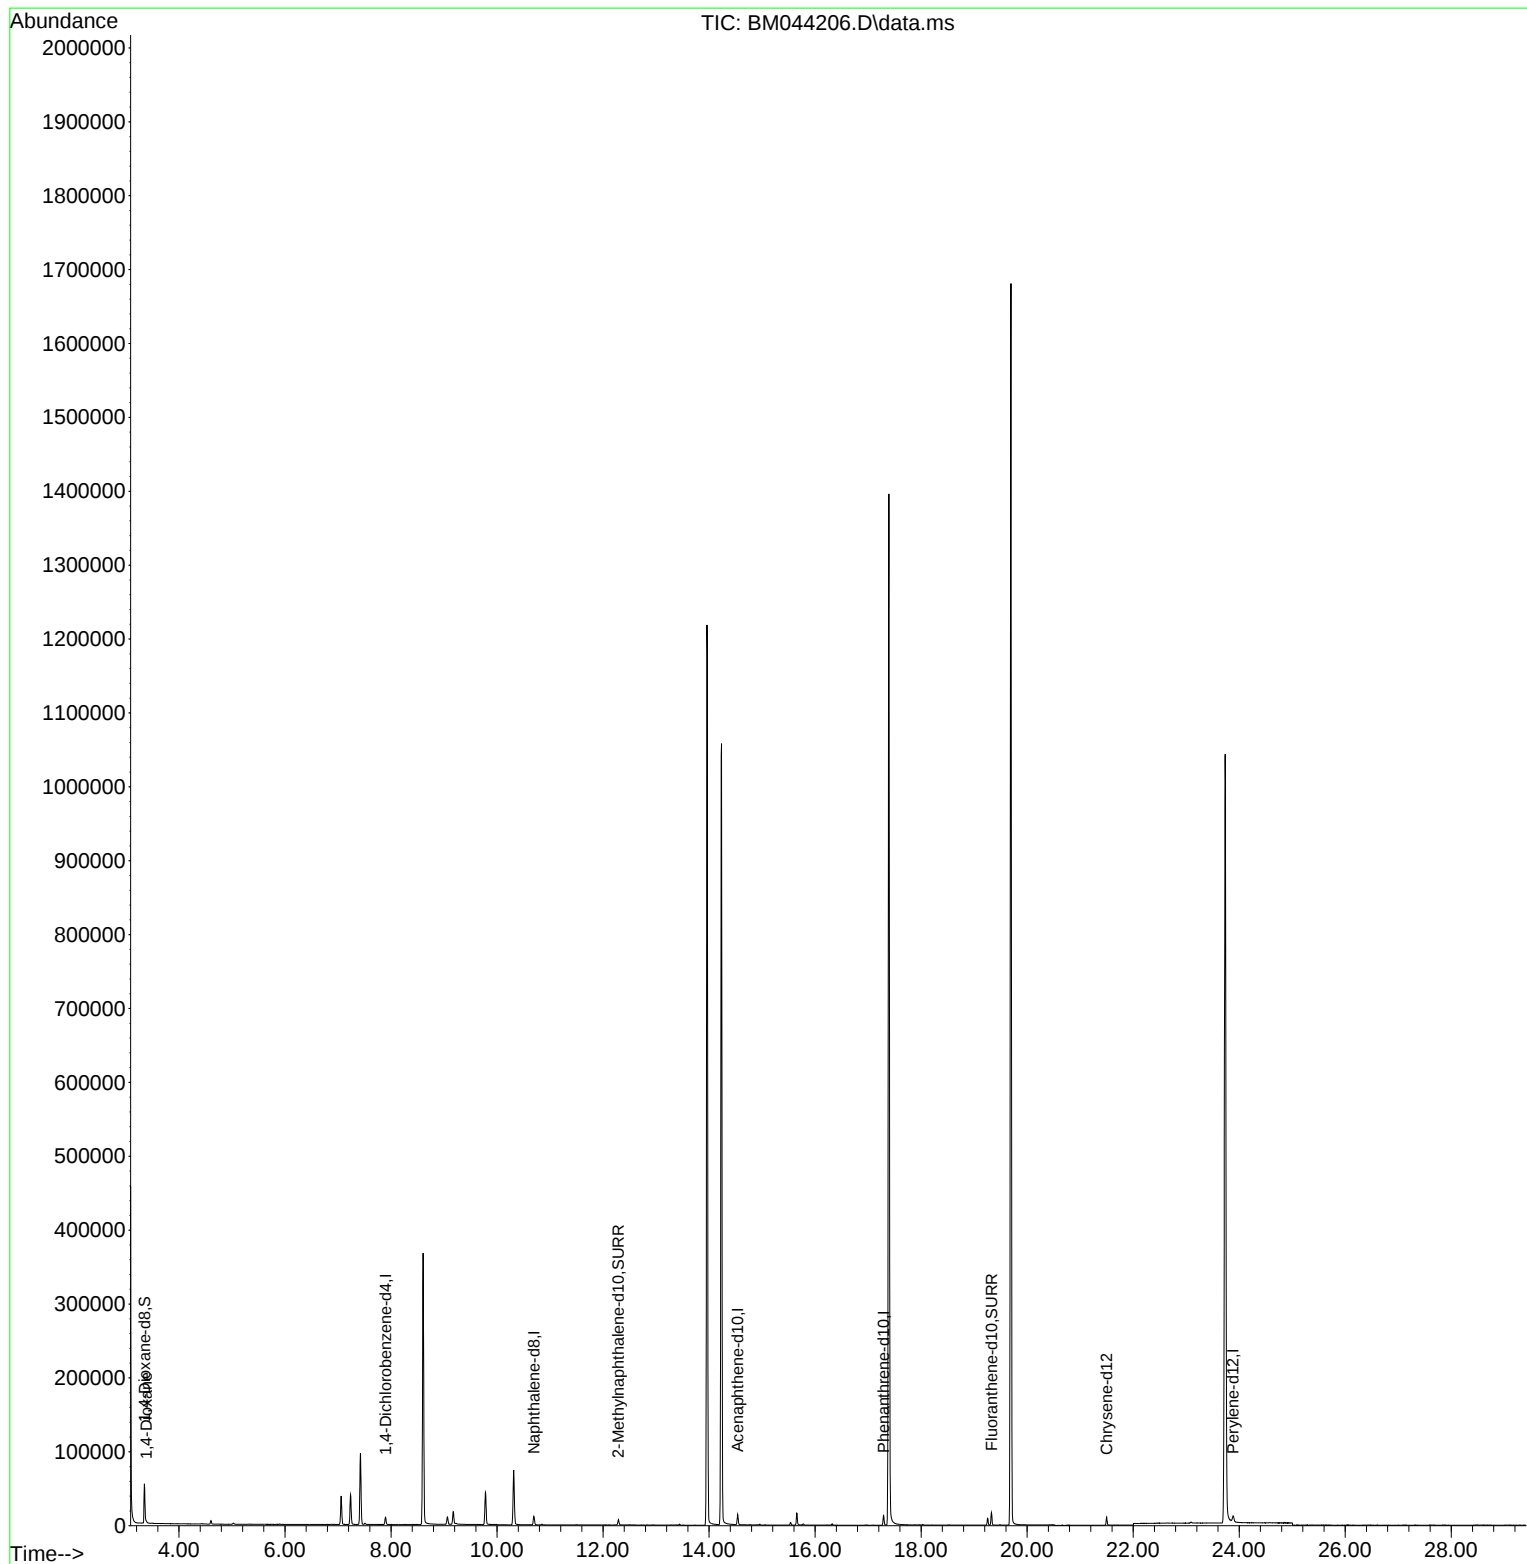

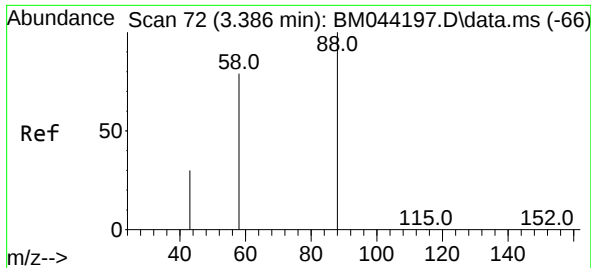

#2
 1,4-Dioxane
 Concen: 0.143 ng/ul
 RT: 3.386 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BM044206.D
 Acq: 20 Feb 2024 14:56

Instrument :
 BNA_M
 ClientSampleId :
 C0AF2

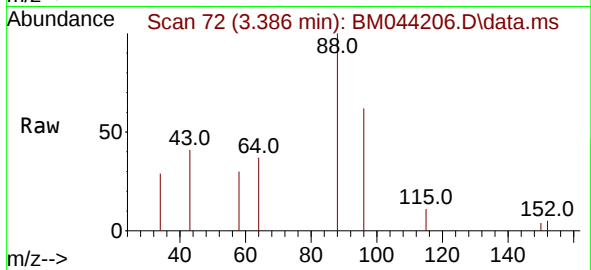

Tgt Ion: 88 Resp: 101
 Ion Ratio Lower Upper
 88 100
 43 40.9 32.2 48.2
 58 30.4 40.6 60.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2024
 Supervised By :mohammad ahmed 02/21/2024

