


Data Path : Z:\HPCHEM1\BNA_M\Data\BM022015\
Data File : BM000553.D
Acq On : 20 Feb 2015 10:49
Operator : TP/IZ
Sample : DFTPP27
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP27

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-MA-BM022015.M
Title : SVOA CALIBRATION
Last Update : Sat Feb 21 00:39:15 2015

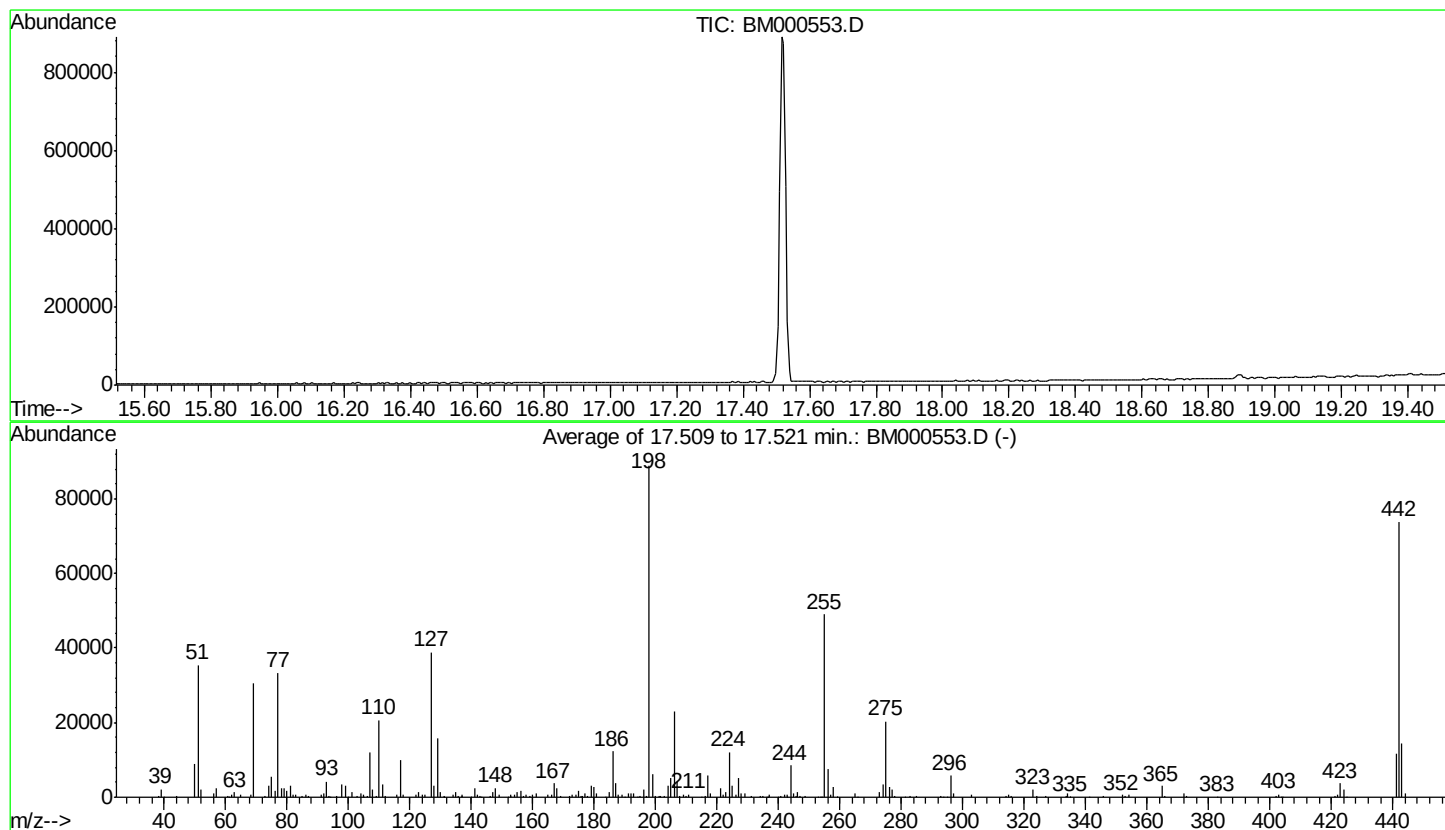

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	35378	PASS
68	69	0.00	2	1.8	559	PASS
69	198	0.00	100	34.4	30621	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.6	38789	PASS
197	198	0.00	2	0.5	439	PASS
198	198	100	100	100.0	88896	PASS
199	198	5	9	7.0	6220	PASS
275	198	10	60	22.9	20340	PASS
365	198	1	100	3.3	2949	PASS
441	443	0.01	100	81.2	11660	PASS
442	198	50	100	83.1	73834	PASS
443	442	15	24	19.5	14361	PASS