

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022015\
 Data File : BM000561.D
 Acq On : 20 Feb 2015 15:33
 Operator : TP/IZ
 Sample : MDL-02-W
 Misc : MDL-WATER-3PPM-SOM0
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-02-W

Quant Time: Feb 21 03:12:12 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-MA-BM022015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 21 00:39:15 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	106411	20.00	ng/ul	0.00
16) Naphthalene-d8	10.46	136	479525	20.00	ng/ul	0.00
33) Acenaphthene-d10	14.33	164	327158	20.00	ng/ul	0.00
59) Phenanthrene-d10	17.07	188	753075	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	614197	20.00	ng/ul	0.00
83) Perylene-d12	23.47	264	442768	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) Phenol-d5	6.85	99	242339	31.28	ng/ul	0.00
5) Bis-(2-Chloroethyl)ether-d	7.01	67	157223	34.34	ng/ul	0.00
7) 2-Chlorophenol-d4	7.20	132	216199	32.81	ng/ul	0.00
11) 4-Methylphenol-d8	8.39	113	214677	32.69	ng/ul	0.00
17) Nitrobenzene-d5	8.83	128	110385	34.30	ng/ul	0.00
20) 2-Nitrophenol-d4	9.55	143	128314	34.44	ng/ul	0.00
24) 2,4-Dichlorophenol-d3	10.09	165	241943	30.66	ng/ul	0.00
27) 4-Chloroaniline-d4	10.60	131	337245	47.91	ng/ul	0.00
41) Dimethylphthalate-d6	13.74	166	863940	36.49	ng/ul	0.00
44) Acenaphthylene-d8	14.02	160	1036062	32.66	ng/ul	0.00
49) 4-Nitrophenol-d4	14.53	143	122108	32.25	ng/ul	0.00
55) Fluorene-d10	15.32	176	784436	33.90	ng/ul	0.00
60) 4,6-Dinitro-2-methylphenol	15.44	200	113892	26.02	ng/ul	0.00
68) Anthracene-d10	17.17	188	1211169	34.00	ng/ul	0.00
76) Pyrene-d10	19.47	212	1239841	34.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.34	264	705207	33.97	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
70) 1,2,3,4-Tetrachlorobenzene	13.12	216	22894	2.05	ng/uL	93
71) Pentachlorobenzene	14.64	250	45952	4.30	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022015\
Data File : BM000561.D
Acq On : 20 Feb 2015 15:33
Operator : TP/IZ
Sample : MDL-02-W
Misc : MDL-WATER-3PPM-SOM0
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MDL-02-W

Quant Time: Feb 21 03:12:12 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-MA-BM022015.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 21 00:39:15 2015
Response via : Initial Calibration




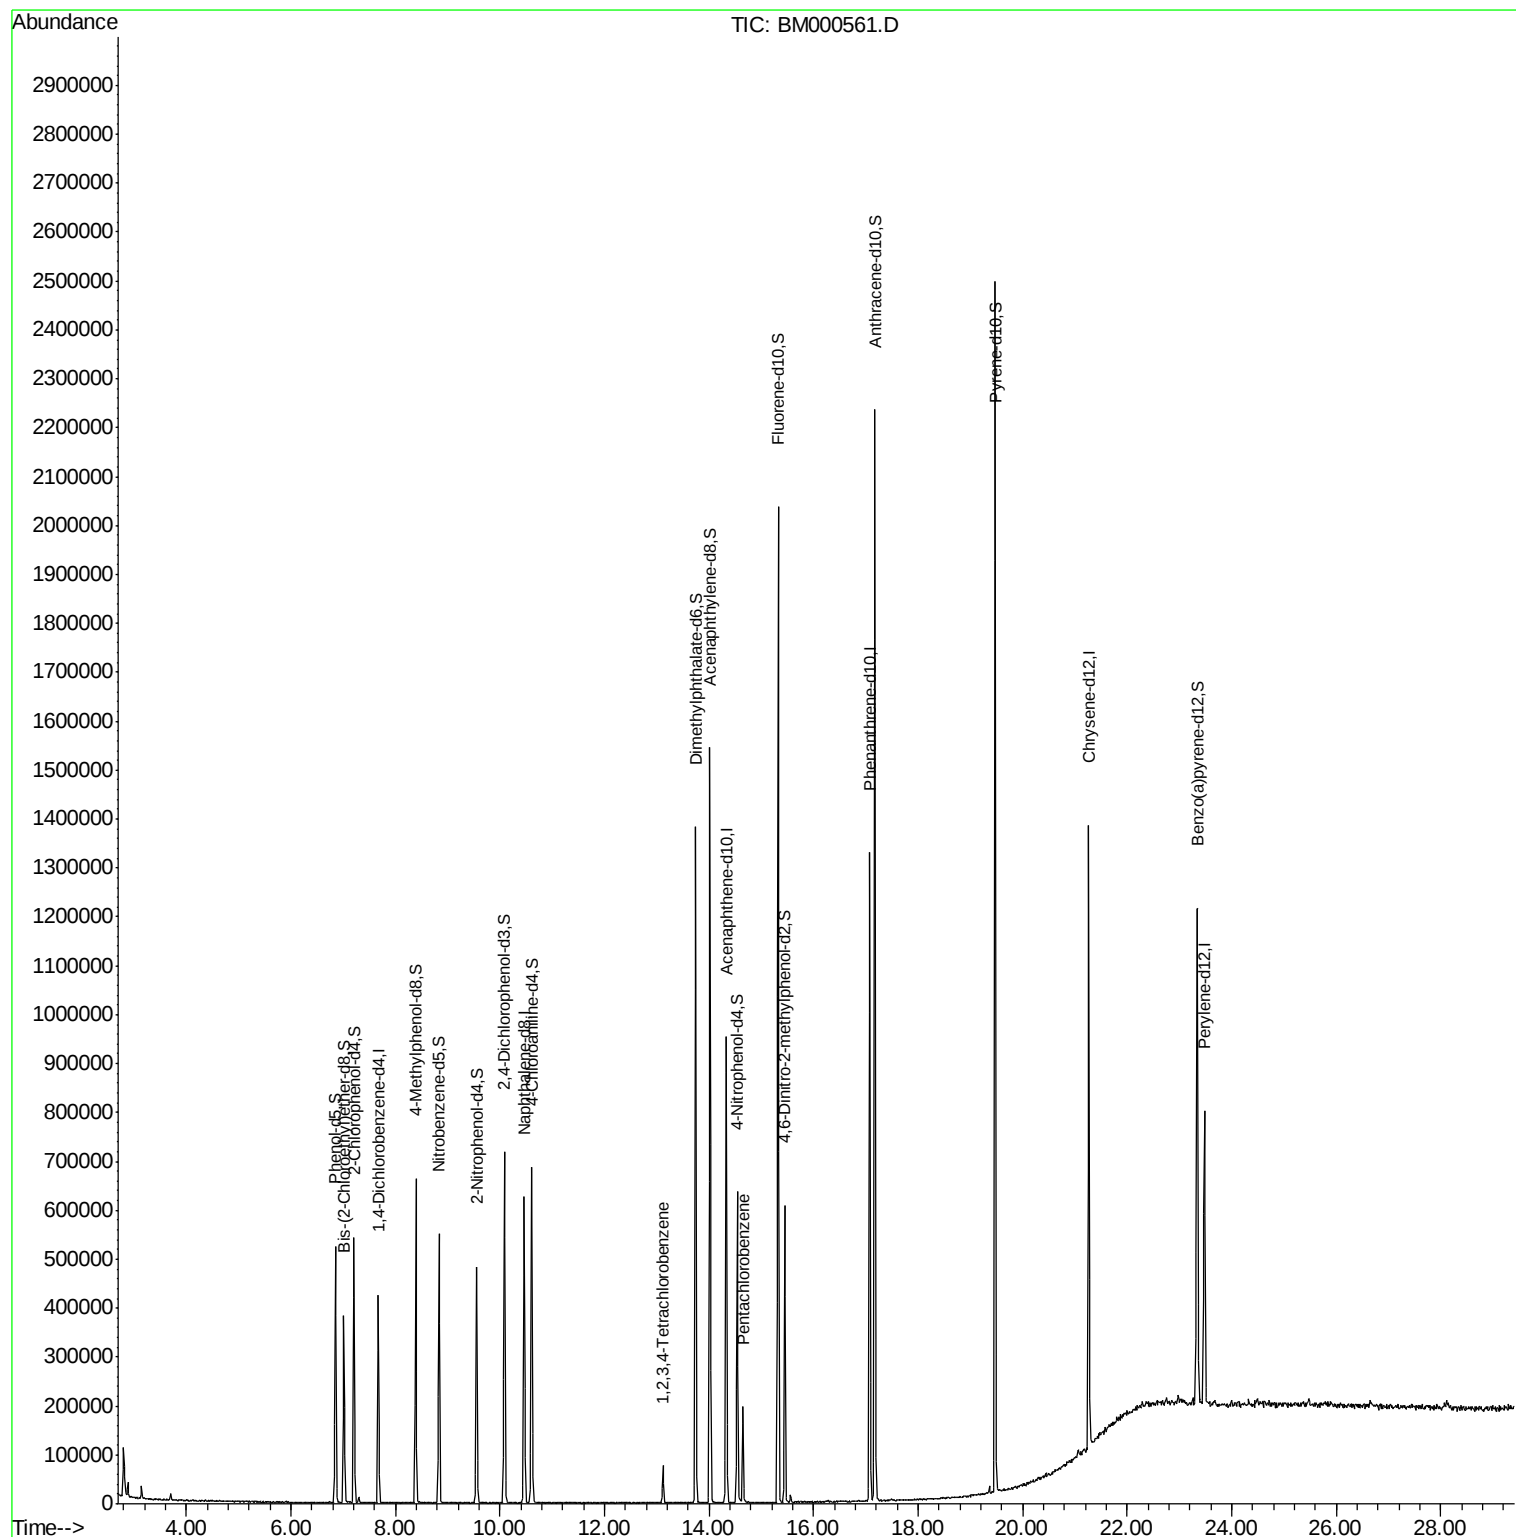


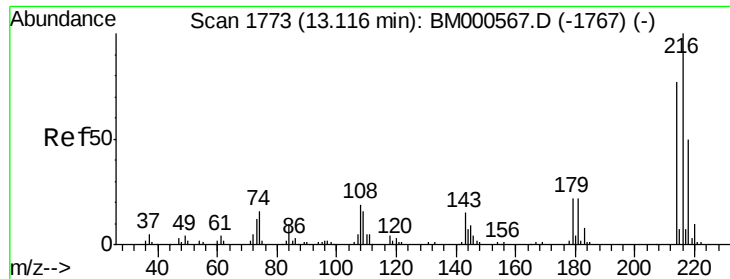

#70
 1,2,3,4-Tetrachlorobenzene
 Concen: 2.05 ng/uL
 RT: 13.12 min Scan# 1773
 Delta R.T. -0.00 min
 Lab File: BM000561.D
 Acq: 20 Feb 2015 15:33

Instrument :
 BNA_M
 ClientSampleId :
 MDL-02-W

Tgt Ion:216 Resp: 22894
 Ion Ratio Lower Upper
 216 100
 214 81.1 59.1 88.7
 218 43.3 37.6 56.4

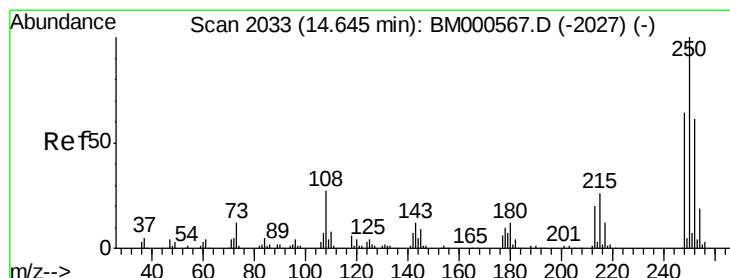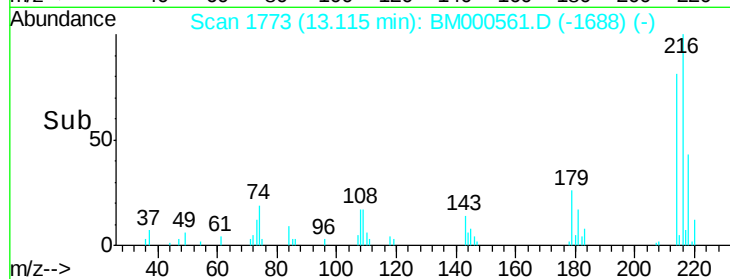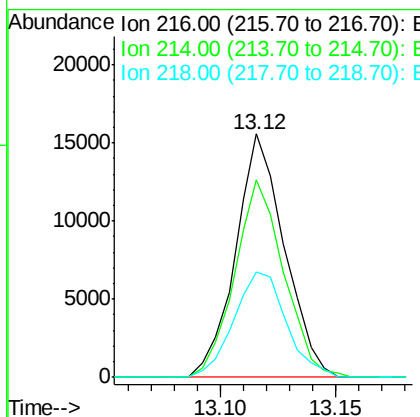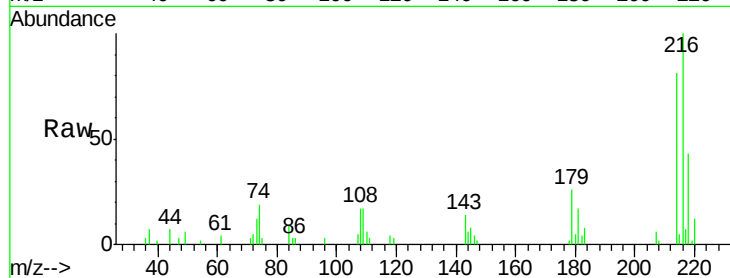

#71
 Pentachlorobenzene
 Concen: 4.30 ng/uL
 RT: 14.64 min Scan# 2033
 Delta R.T. -0.00 min
 Lab File: BM000561.D
 Acq: 20 Feb 2015 15:33

Tgt Ion:250 Resp: 45952
 Ion Ratio Lower Upper
 250 100
 248 61.4 52.4 78.6
 252 66.4 51.5 77.3

