


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022019\
Data File : BM018877.D
Acq On : 20 Feb 2019 10:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 11 16:02:12 2019

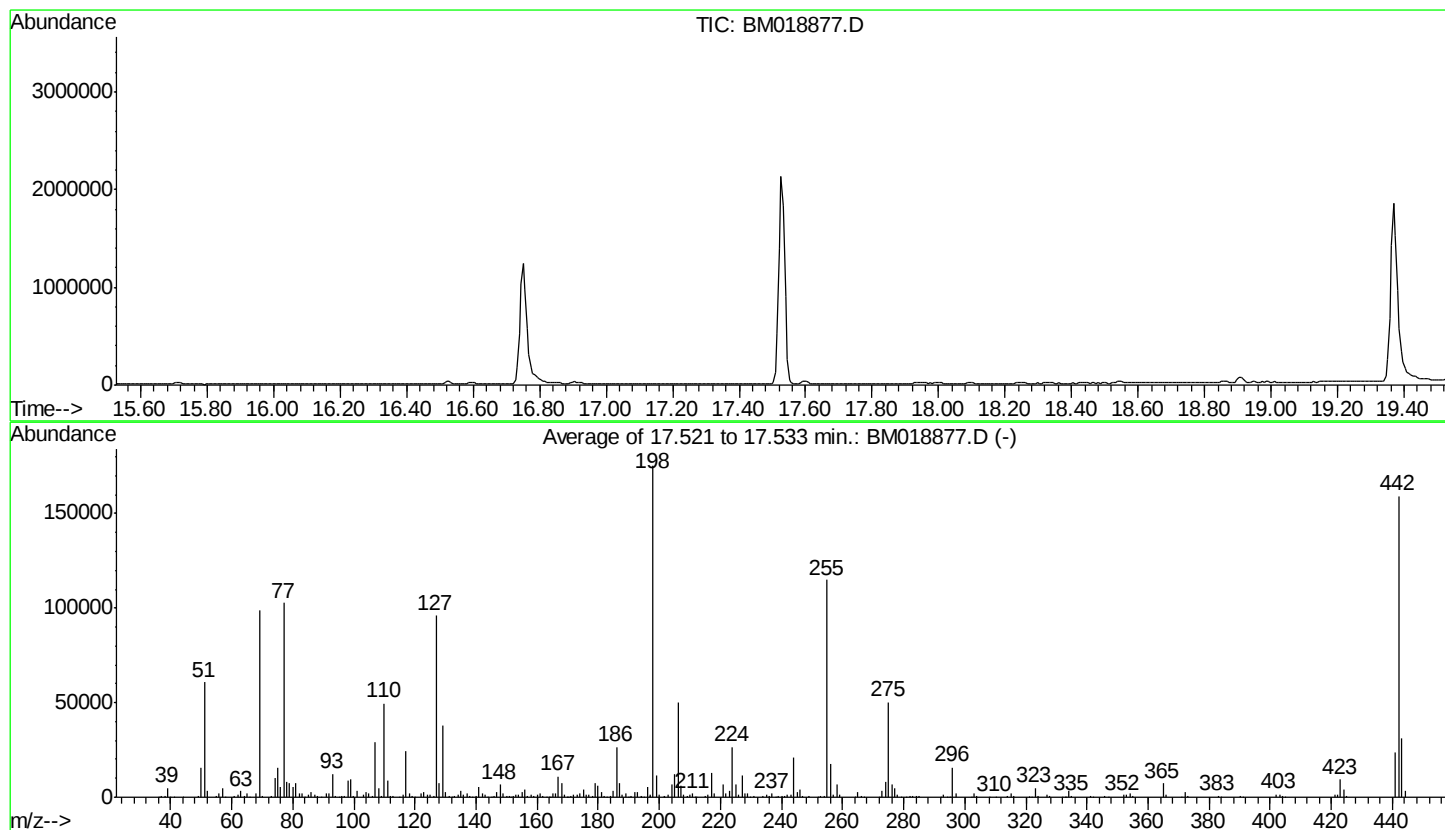

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	60837	PASS
68	69	0.00	2	2.0	1981	PASS
69	198	0.00	100	56.2	98576	PASS
70	69	0.00	2	0.4	441	PASS
127	198	10	80	54.8	96037	PASS
197	198	0.00	2	0.7	1212	PASS
198	198	100	100	100.0	175338	PASS
199	198	5	9	6.8	11841	PASS
275	198	10	60	28.7	50357	PASS
365	198	1	100	4.2	7429	PASS
441	198	0.01	100	13.7	23937	PASS
442	198	50	100	90.9	159381	PASS
443	442	15	24	19.5	31138	PASS