

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022118\
 Data File : BM014319.D
 Acq On : 21 Feb 2018 10:09
 Operator : SJ/JU
 Sample : PB106684BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK84

Quant Time: Feb 22 03:38:53 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 22 03:35:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	75711	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	354177	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.19	164	233191	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.94	188	554986	20.00	ng/ul	0.00
75) Chrysene-d12	21.15	240	558969	20.00	ng/ul	0.00
83) Perylene-d12	23.32	264	476615	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	10526	5.95	ng/uL	0.00
5) Phenol-d5	6.72	99	177628	27.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.88	67	123337	31.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.07	132	151457	30.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	158386	28.29	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	83711	31.98	ng/ul	0.00
22) 2-Nitrophenol-d4	9.40	143	85020	31.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.94	165	146368	26.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	200144	36.21	ng/ul	0.00
43) Dimethylphthalate-d6	13.61	166	617570	32.07	ng/ul	0.00
46) Acenaphthylene-d8	13.87	160	773098	32.56	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	53684	20.19	ng/ul	0.01
57) Fluorene-d10	15.19	176	550936	31.93	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	78019	23.43	ng/ul	0.00
70) Anthracene-d10	17.04	188	893293	33.36	ng/ul	0.00
76) Pyrene-d10	19.34	212	995027	34.51	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.18	264	776490	33.47	ng/ul	0.00

Target Compounds


				Ovalue	
21) Isophorone	9.40	82	14018	1.059	ng/ul# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022118\
Data File : BM014319.D
Acq On : 21 Feb 2018 10:09
Operator : SJ/JU
Sample : PB106684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK84

Quant Time: Feb 22 03:38:53 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 22 03:35:18 2018
Response via : Initial Calibration

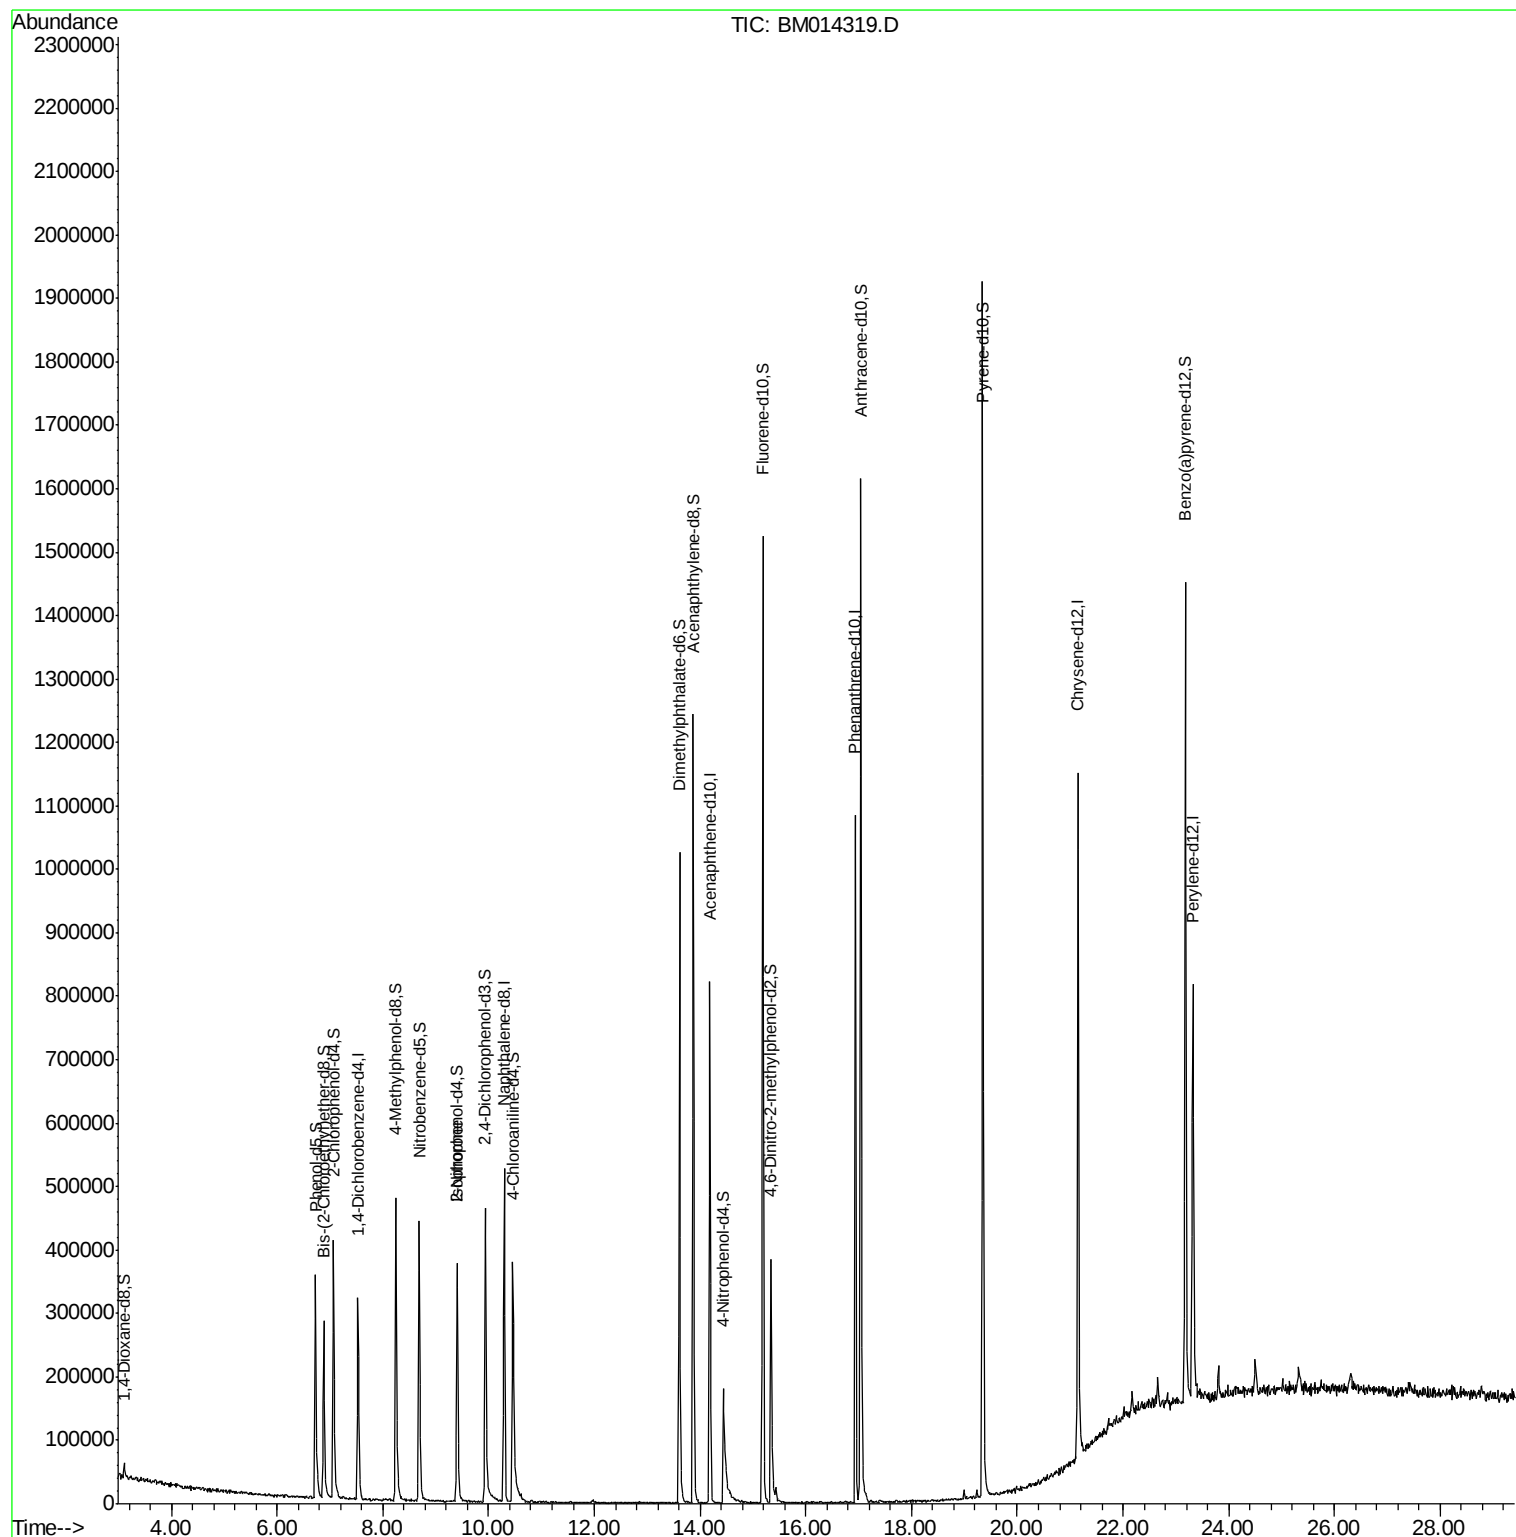

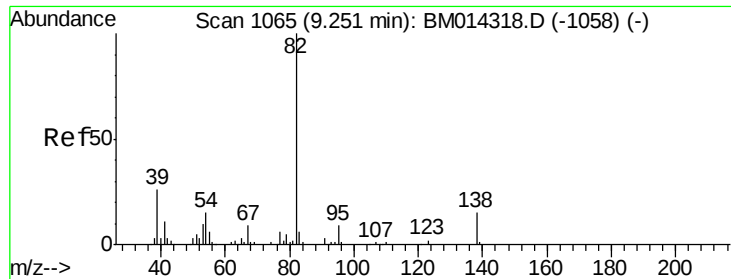

#21

Isophorone

Concen: 1.059 ng/ul

RT: 9.40 min Scan# 1090

Delta R.T. 0.15 min

Lab File: BM014319.D

Acq: 21 Feb 2018 10:09

Instrument :

BNA_M

ClientSampleId :

SBLK84

Tot Ion: 82 Resp: 14018

Ion Ratio Lower Upper

82 100

95 0.0 7.8 11.8#

138 0.0 11.9 17.9#

