
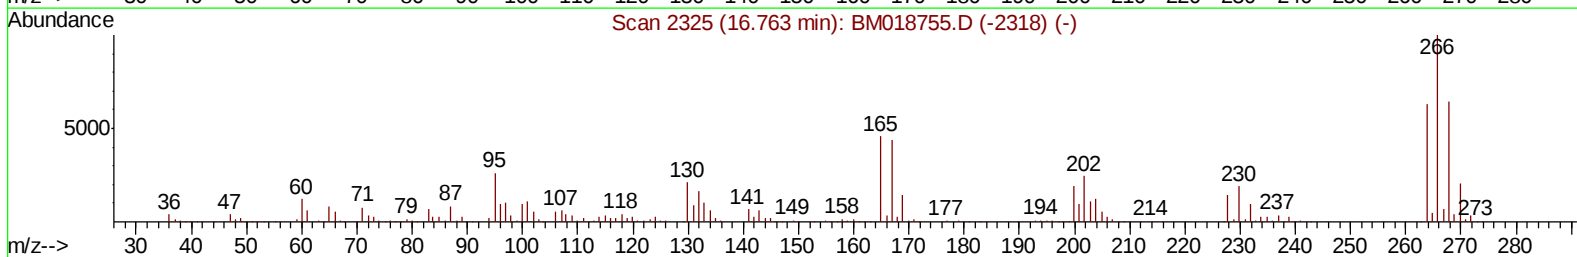
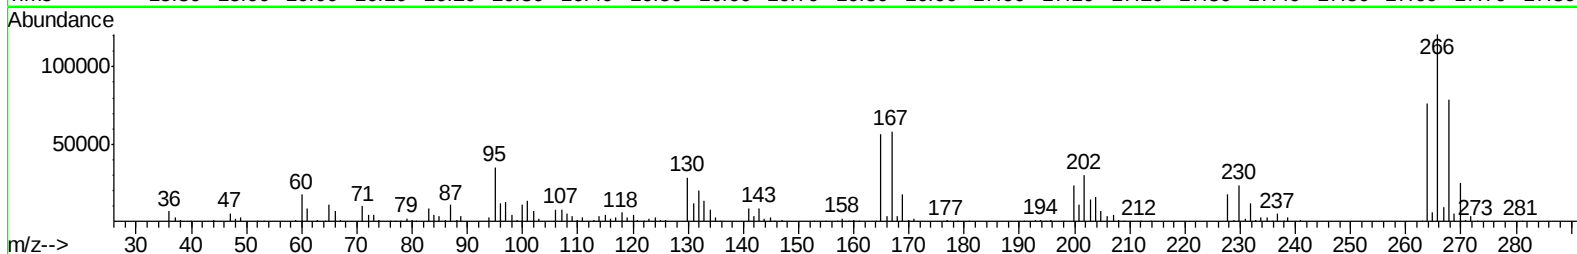


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022119\
Data File : BM018891.D
Acq On : 21 Feb 2019 12:20
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 04:49:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

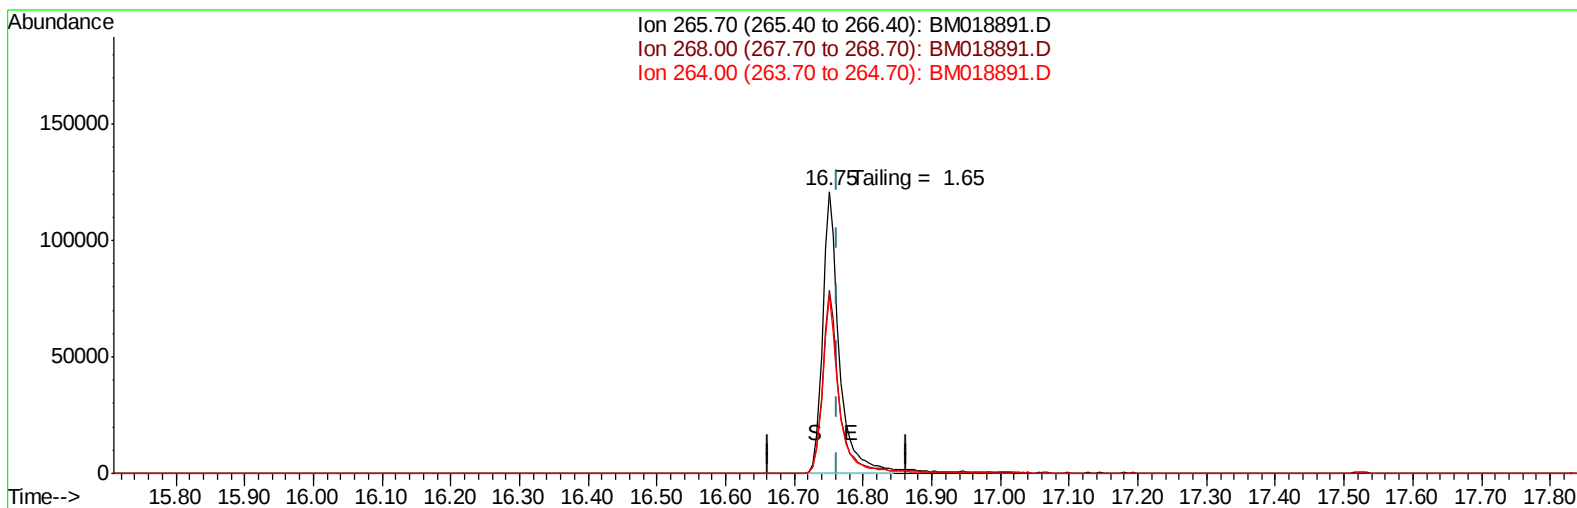

TIC: BM018891.D

(70) Pentachlorophenol (C)




16.751min (-0.012) 0.00ng

response 204456

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	65.14
264.00	63.20	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022119\
 Data File : BM018891.D
 Acq On : 21 Feb 2019 12:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 04:49:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 11 16:02:12 2019
 Response via : Initial Calibration

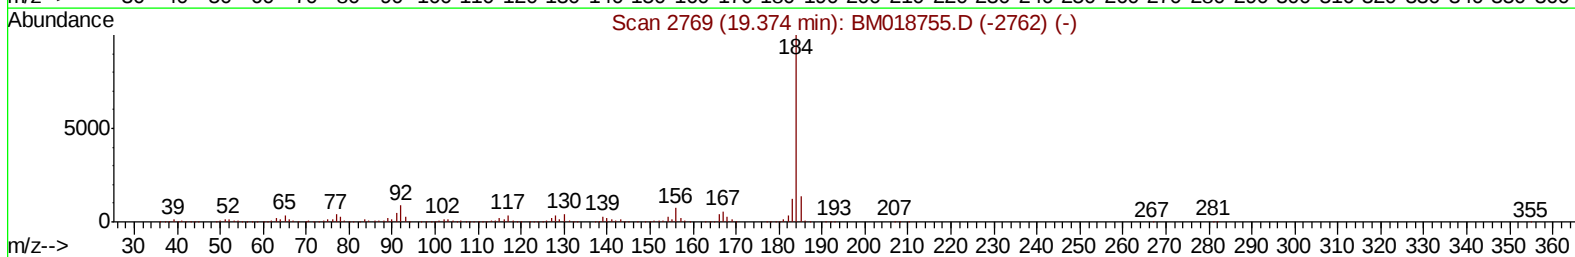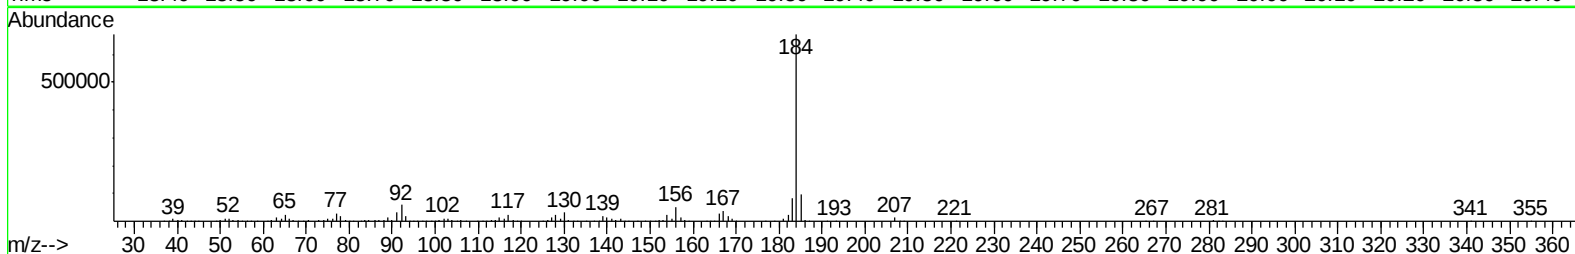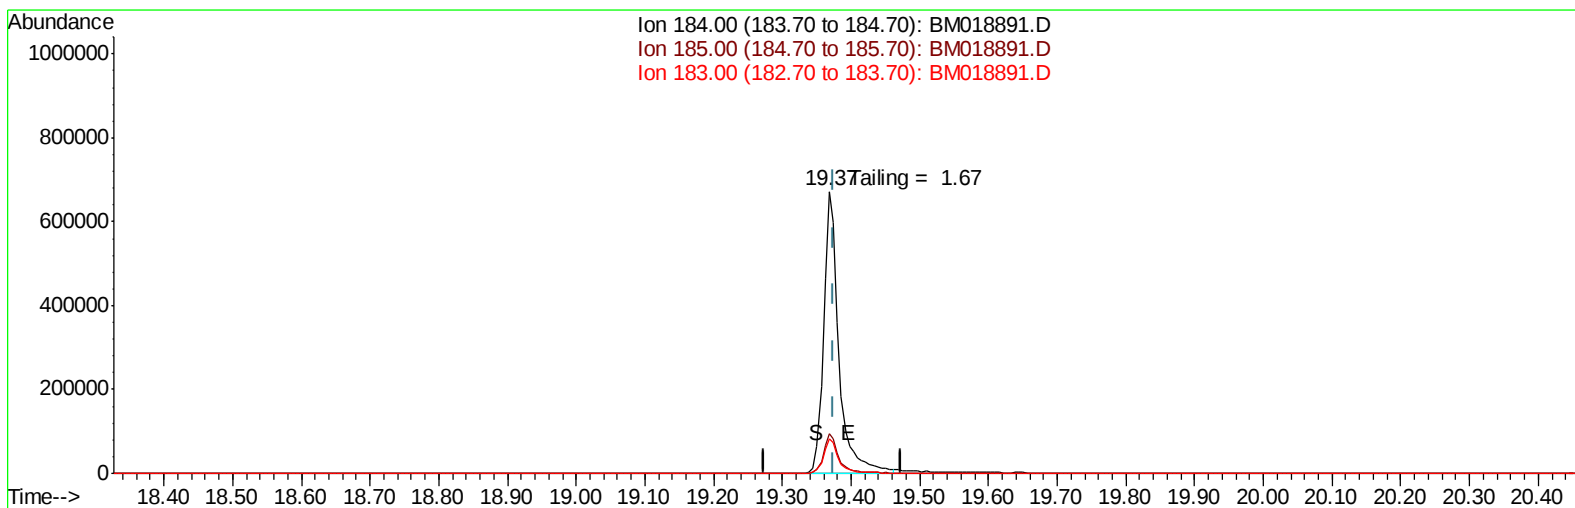

TIC: BM018891.D

(77) Benzidine

19.368min (-0.006) 63332.91ng

response 1044086

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.27
183.00	12.10	12.46
0.00	0.00	0.00