

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022119\
 Data File : BM018901.D
 Acq On : 21 Feb 2019 18:20
 Operator : JU/SJ
 Sample : K1546-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 RT-3422

Quant Time: Feb 22 04:02:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 11 16:02:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	285817	20.00	ng	-0.02
21) Naphthalene-d8	10.49	136	1160934	20.00	ng	-0.02
39) Acenaphthene-d10	14.35	164	661869	20.00	ng	-0.02
64) Phenanthrene-d10	17.10	188	1489705	20.00	ng	-0.02
76) Chrysene-d12	21.30	240	1471133	20.00	ng	-0.01
87) Perylene-d12	23.54	264	1333923	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	2600489	149.08	ng	-0.01
7) Phenol-d6	6.88	99	3616877	147.18	ng	-0.01
23) Nitrobenzene-d5	8.86	82	2323385	92.54	ng	-0.02
42) 2,4,6-Tribromophenol	15.85	330	1340530	140.51	ng	-0.02
45) 2-Fluorobiphenyl	12.96	172	4067182	81.57	ng	-0.02
79) Terphenyl-d14	19.73	244	6149957	86.24	ng	-0.01
Target Compounds						
10) Phenol	6.90	94	55491	2.146	ng	Qvalue # 74
50) Dimethylphthalate	13.81	163	224457	4.069	ng	99
52) Acenaphthene	14.41	154	148989	3.708	ng	94
58) Fluorene	15.40	166	192445	3.809	ng	97
71) Phenanthrene	17.14	178	728509	9.100	ng	99
75) Fluoranthene	19.16	202	1321888	14.294	ng	99
78) Pyrene	19.53	202	921035	10.780	ng	100
81) Benzo(a)anthracene	21.28	228	206059	2.403	ng	98
83) Chrysene	21.33	228	164690	2.004	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022119\
Data File : BM018901.D
Acq On : 21 Feb 2019 18:20
Operator : JU/SJ
Sample : K1546-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RT-3422

Quant Time: Feb 22 04:02:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

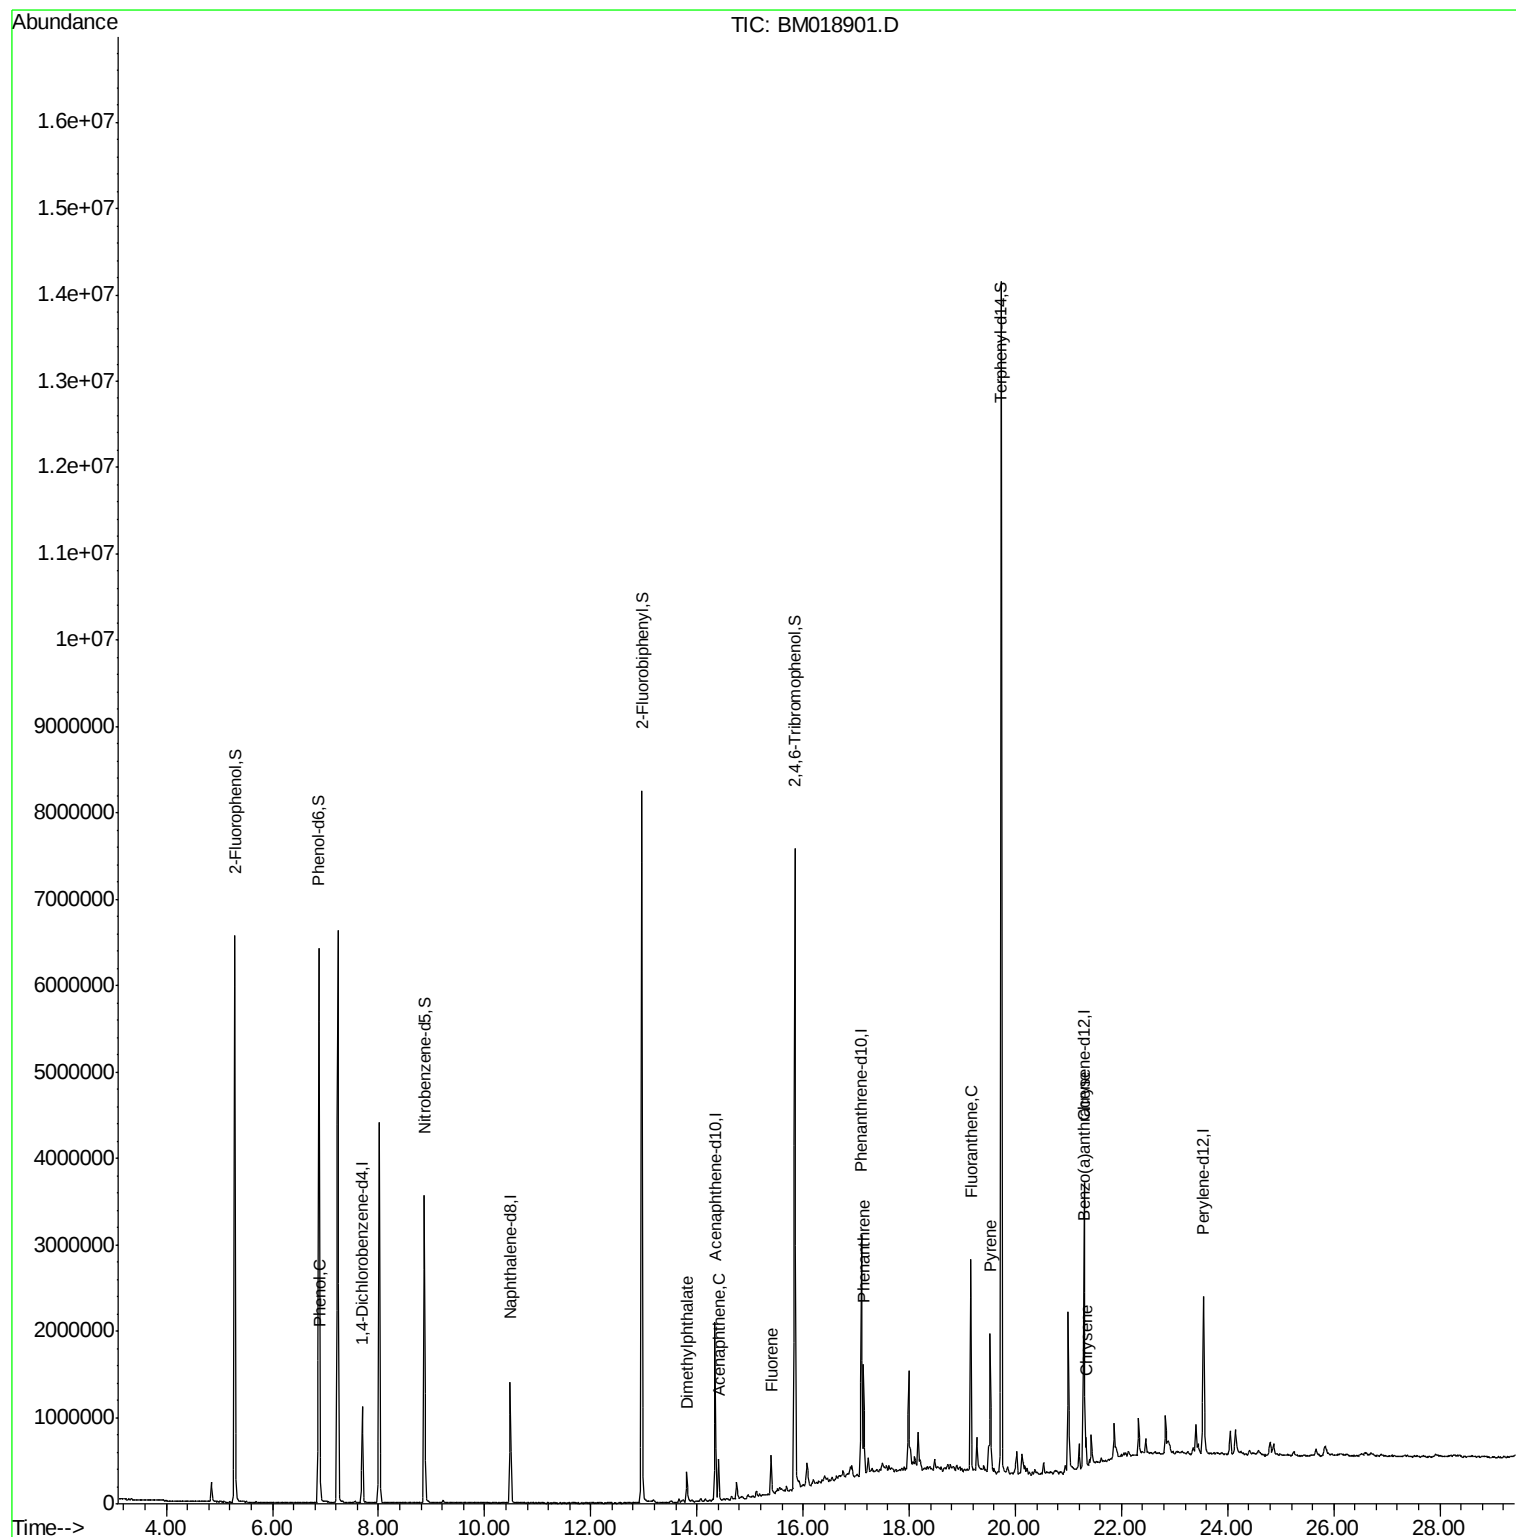

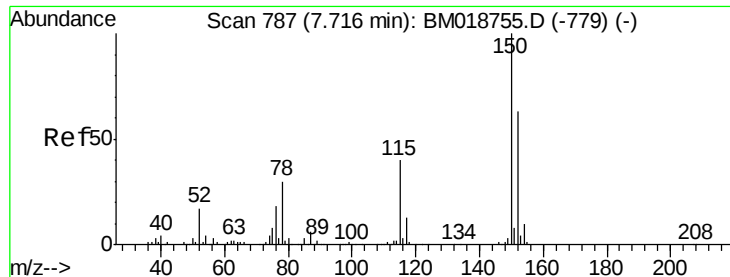


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.70 min Scan# 784
Delta R.T. -0.02 min
Lab File: BM018901.D
Acq: 21 Feb 2019 18:20

Instrument :
BNA_M
ClientSampleId :
RT-3422

Tot Ion:152 Resp: 285817
Ion Ratio Lower Upper
152 100
150 154.1 127.3 190.9
115 62.0 50.8 76.2

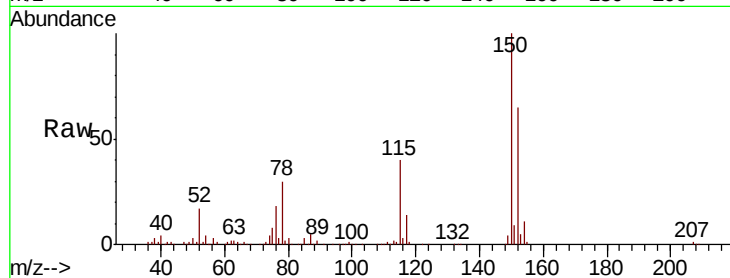


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

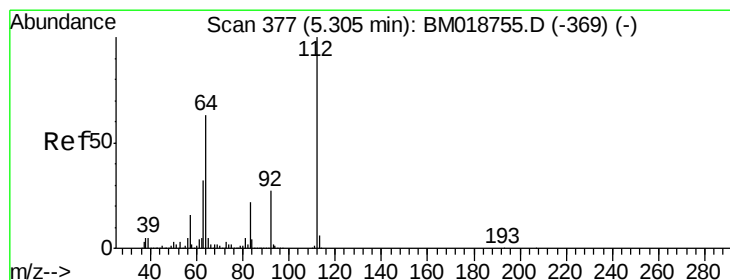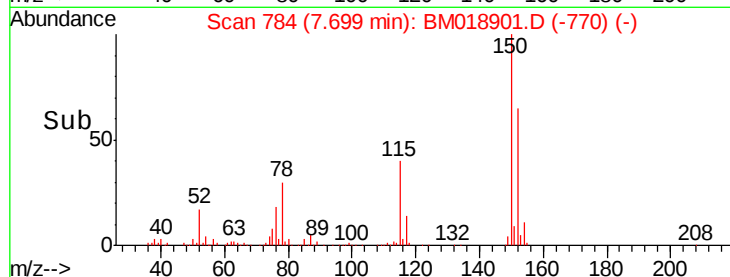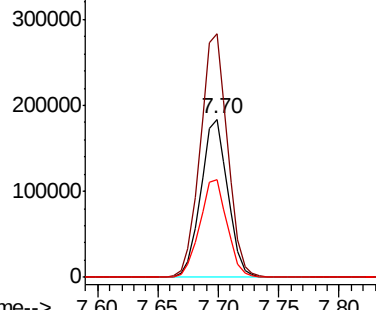



#5


2-Fluorophenol
Concen: 149.076 ng
RT: 5.29 min Scan# 375
Delta R.T. -0.01 min
Lab File: BM018901.D
Acq: 21 Feb 2019 18:20

Tgt Ion:112 Resp: 2600489
Ion Ratio Lower Upper
112 100
64 64.0 50.6 75.8
63 32.6 25.7 38.5

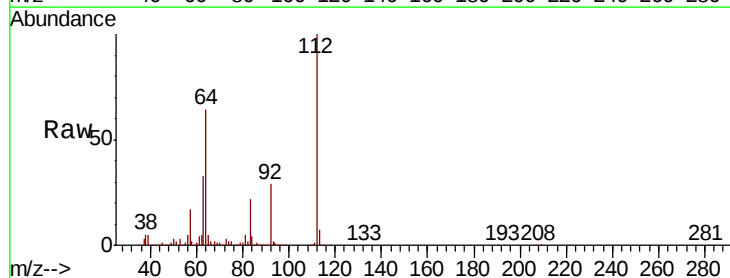

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

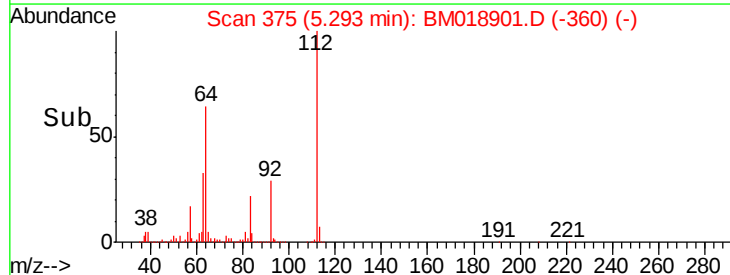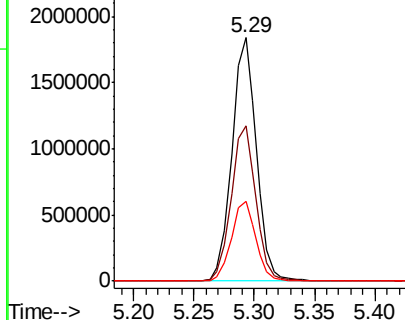



#7

Phenol-d6

Concen: 147.180 ng

RT: 6.88 min Scan# 644

Delta R.T. -0.01 min

Lab File: BM018901.D

Acq: 21 Feb 2019 18:20

Instrument :


BNA_M

ClientSampleId :

RT-3422

Tot Ion: 99 Resp: 3616877

Ion	Ratio	Lower	Upper
99	100		
42	14.0	11.0	16.6
71	39.6	31.3	46.9






Abundance

Ion 99.00 (98.70 to 99.70): BM018755.D (-637) (-)

Ion 42.00 (41.70 to 42.70): BM018755.D (-637) (-)

Ion 71.00 (70.70 to 71.70): BM018755.D (-637) (-)

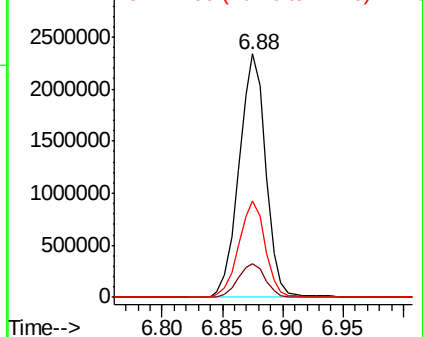

#10

Phenol

Concen: 2.146 ng

RT: 6.90 min Scan# 648


Delta R.T. -0.02 min

Lab File: BM018901.D

Acq: 21 Feb 2019 18:20

Tgt Ion: 94 Resp: 55491

Ion	Ratio	Lower	Upper
94	100		
65	37.7	9.6	49.6
66	62.0	20.4	60.4






Abundance

Ion 94.00 (93.70 to 94.70): BM018755.D (-642) (-)

Ion 65.00 (64.70 to 65.70): BM018755.D (-642) (-)

Ion 66.00 (65.70 to 66.70): BM018755.D (-642) (-)

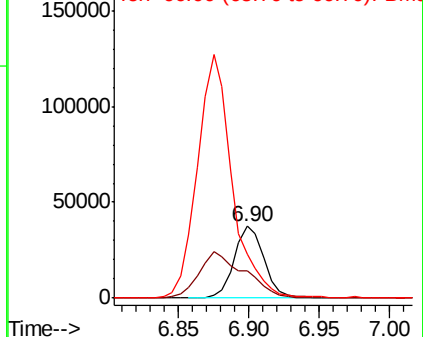



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.49 min Scan# 1258

Delta R.T. -0.02 min

Lab File: BM018901.D

Acq: 21 Feb 2019 18:20

Instrument :

BNA_M

ClientSampleId :

RT-3422

Tot Ion:136 Resp: 1160934


Ion Ratio Lower Upper

136 100

137 10.7 8.8 13.2

54 6.6 5.0 7.6

68 7.2 5.5 8.3



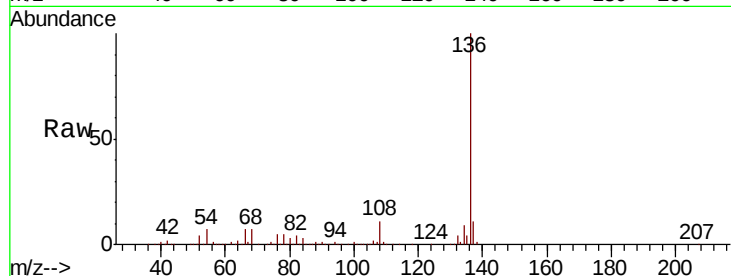


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BM

Ion 68.00 (67.70 to 68.70): BM

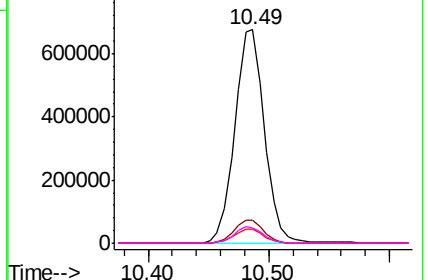

#23

Nitrobenzene-d5

Concen: 92.538 ng

RT: 8.86 min Scan# 982

Delta R.T. -0.02 min

Lab File: BM018901.D

Acq: 21 Feb 2019 18:20


Tgt Ion: 82 Resp: 2323385

Ion Ratio Lower Upper

82 100

128 35.9 29.9 44.9



54 37.3 29.1 43.7




Abundance Ion 82.00 (81.70 to 82.70): BM

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BM



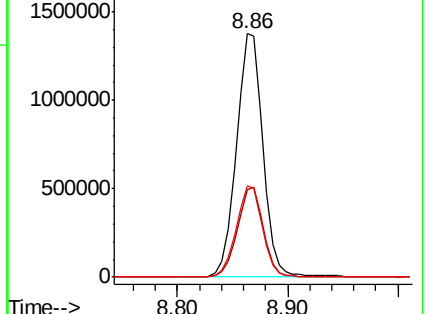



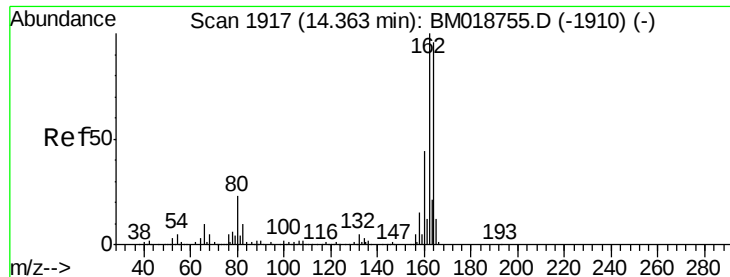

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.35 min Scan# 1914
Delta R.T. -0.02 min
Lab File: BM018901.D
Acq: 21 Feb 2019 18:20




Instrument :
BNA_M
ClientSampleId :
RT-3422


Tot Ion:164 Resp: 661869
Ion Ratio Lower Upper
164 100
162 102.7 83.4 125.0
160 45.5 36.6 55.0

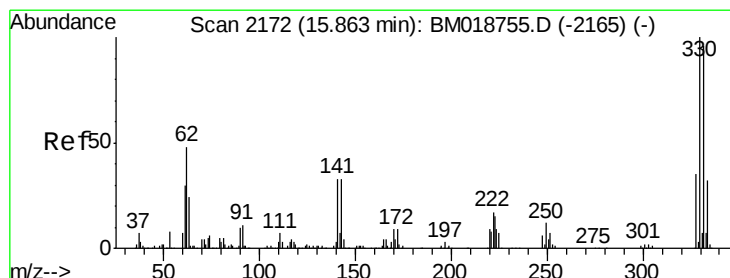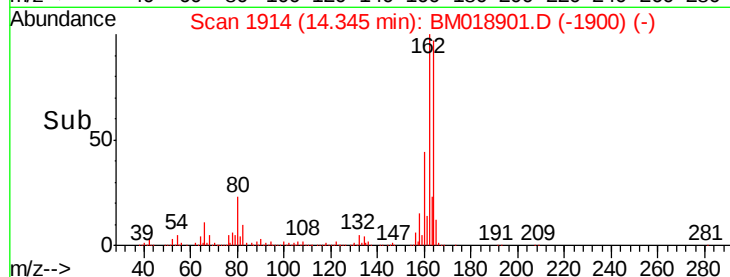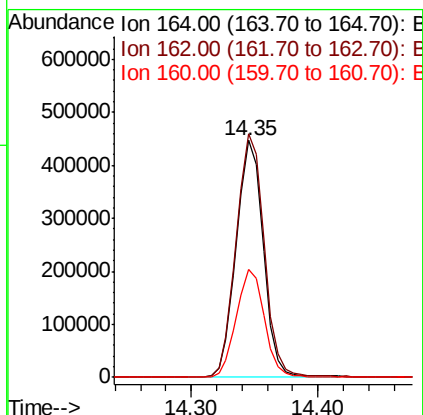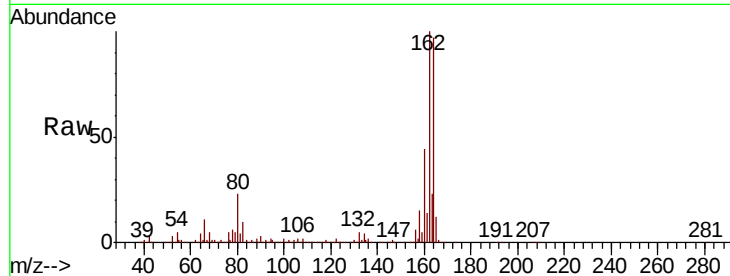

#42
2,4,6-Tribromophenol
Concen: 140.507 ng
RT: 15.85 min Scan# 2169
Delta R.T. -0.02 min
Lab File: BM018901.D
Acq: 21 Feb 2019 18:20

Tgt Ion:330 Resp: 1340530
Ion Ratio Lower Upper
330 100
332 97.3 76.9 115.3
141 35.2 28.7 43.1


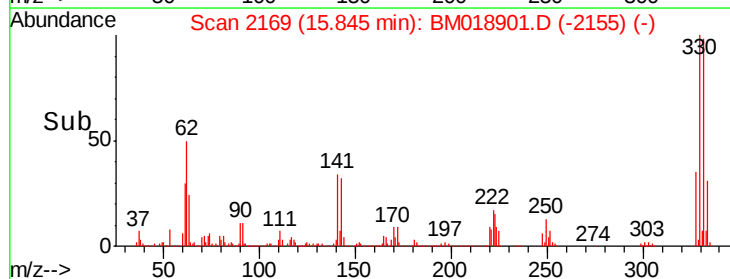
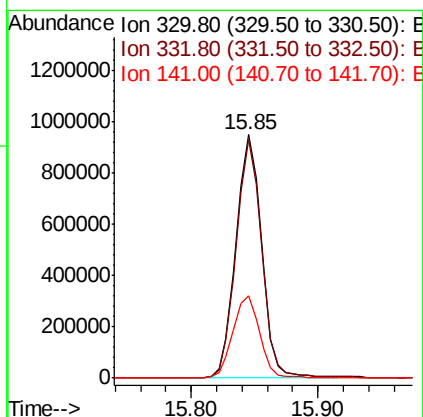
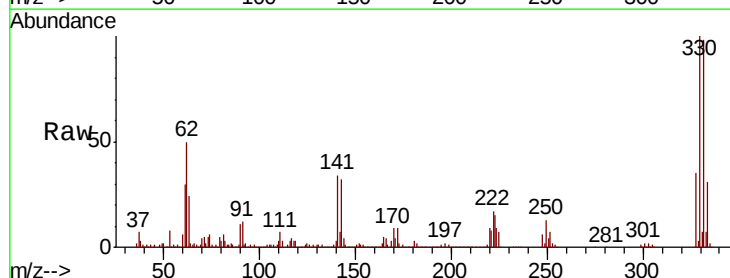


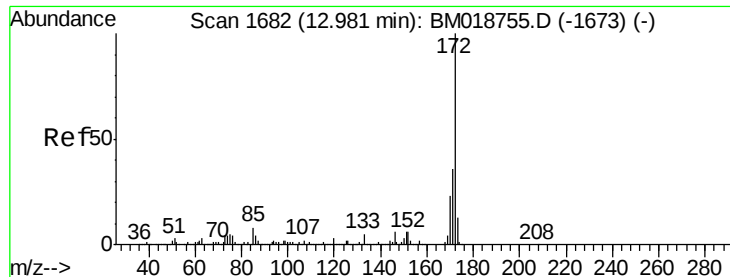

#45
2-Fluorobiphenyl
Concen: 81.573 ng
RT: 12.96 min Scan# 1679
Delta R.T. -0.02 min
Lab File: BM018901.D
Acq: 21 Feb 2019 18:20




Instrument :
BNA_M
ClientSampleId :
RT-3422


Tot Ion:172 Resp: 4067182
Ion Ratio Lower Upper
172 100
171 35.9 29.0 43.6
170 23.7 18.6 28.0

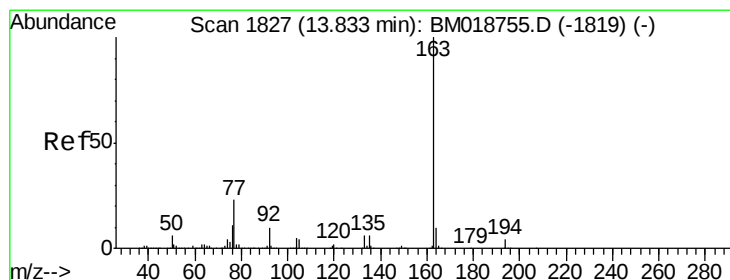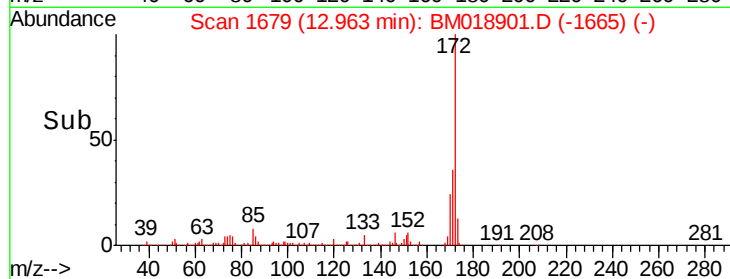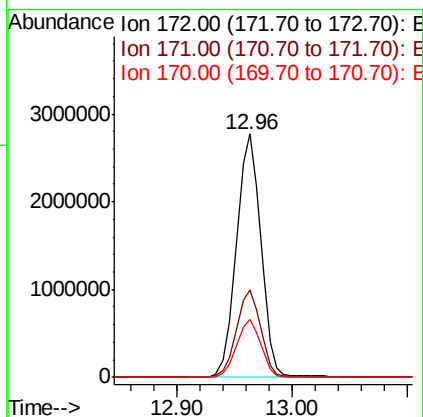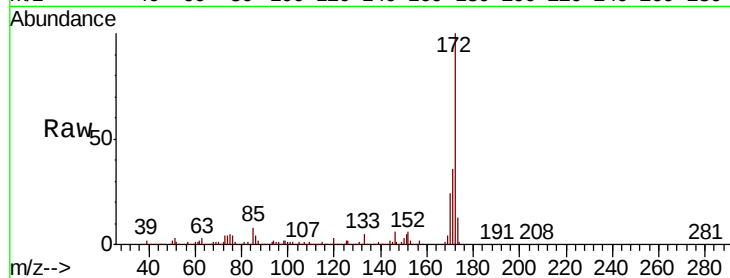

#50
Dimethylphthalate
Concen: 4.069 ng
RT: 13.81 min Scan# 1823
Delta R.T. -0.02 min
Lab File: BM018901.D
Acq: 21 Feb 2019 18:20

Tgt Ion:163 Resp: 224457
Ion Ratio Lower Upper
163 100
194 4.2 3.2 4.8
164 10.1 7.8 11.8

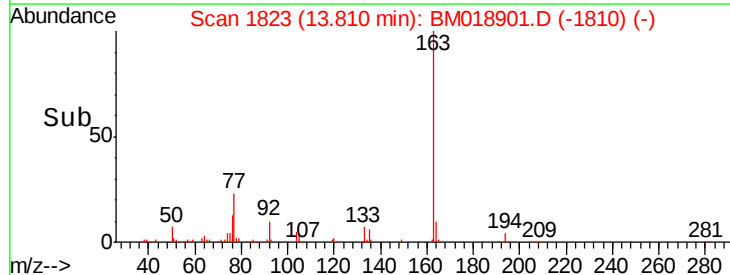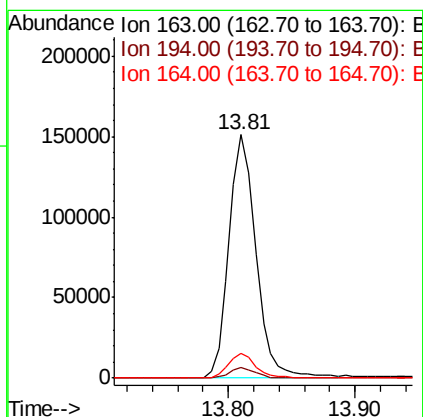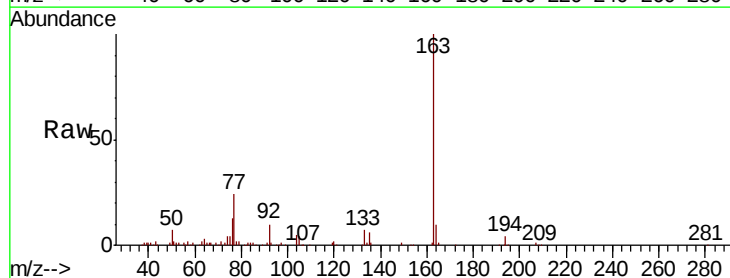

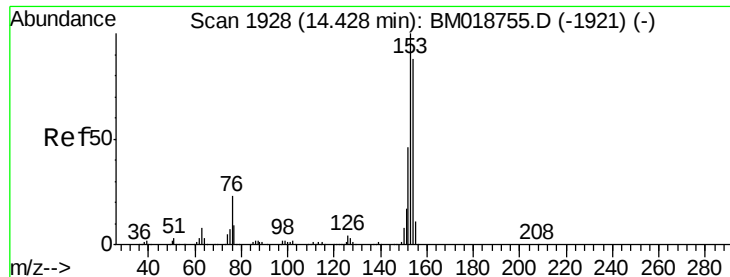

#52

Acenaphthene

Concen: 3.708 ng

RT: 14.41 min Scan# 1925

Delta R.T. -0.02 min

Lab File: BM018901.D

Acq: 21 Feb 2019 18:20

Instrument :

BNA_M

ClientSampleId :

RT-3422


Tot Ion:154 Resp: 148989

Ion Ratio Lower Upper

154 100

153 120.1 91.3 136.9




152 57.0 42.2 63.4

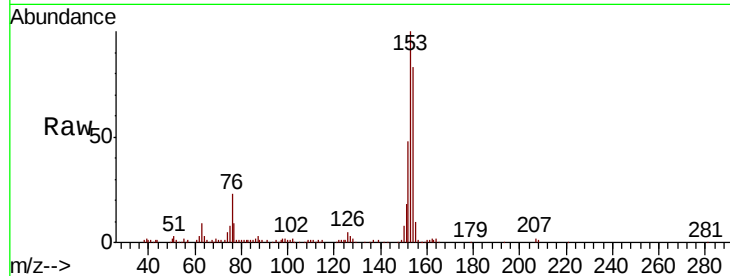

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

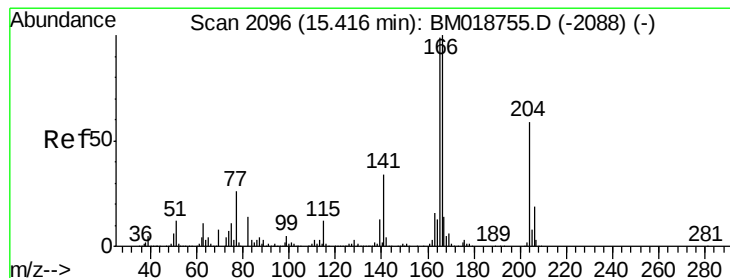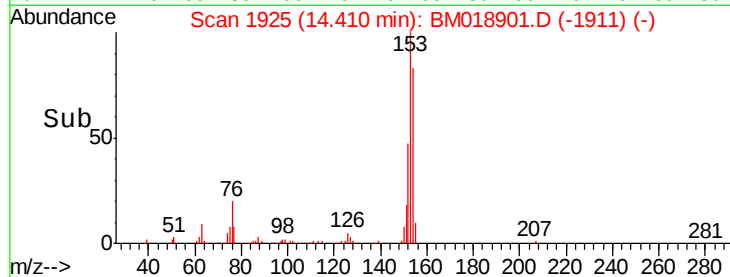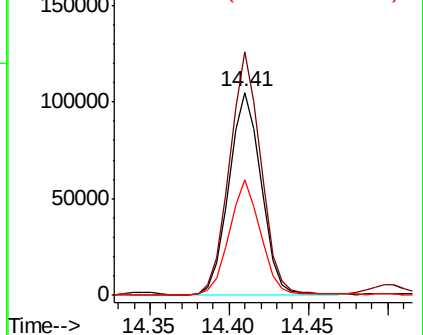

#58

Fluorene

Concen: 3.809 ng

RT: 15.40 min Scan# 2093

Delta R.T. -0.02 min

Lab File: BM018901.D

Acq: 21 Feb 2019 18:20


Tgt Ion:166 Resp: 192445

Ion Ratio Lower Upper

166 100

165 95.8 79.1 118.7



167 14.3 11.0 16.4

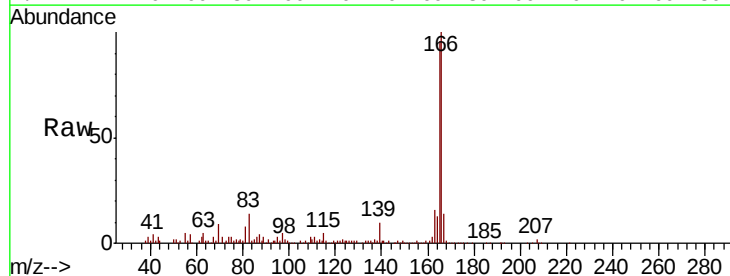


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E



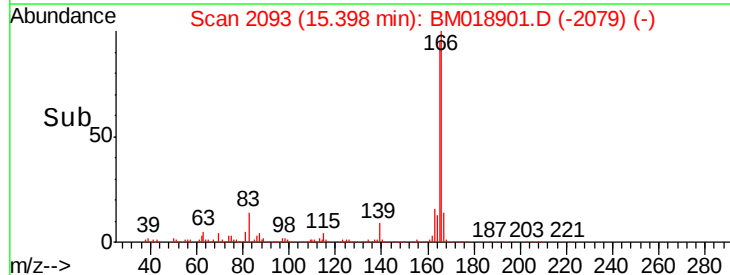
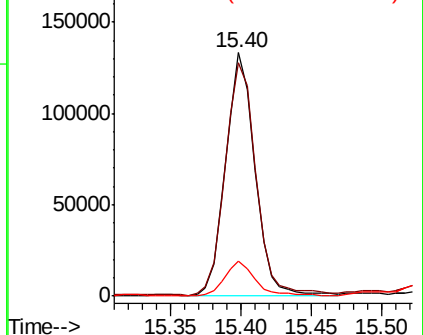




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.10 min Scan# 2382
Delta R.T. -0.02 min
Lab File: BM018901.D
Acq: 21 Feb 2019 18:20




Instrument :
BNA_M
ClientSampleId :
RT-3422


Tot Ion:188 Resp: 1489705
Ion Ratio Lower Upper
188 100
94 10.1 8.2 12.2
80 12.5 9.7 14.5

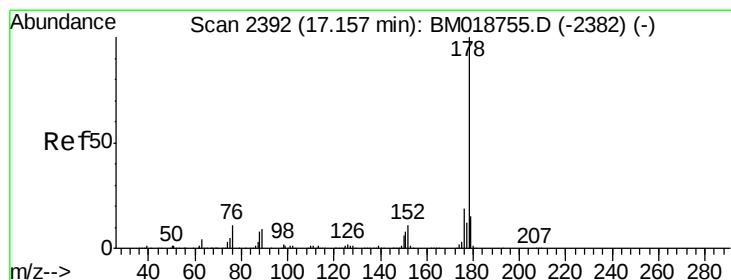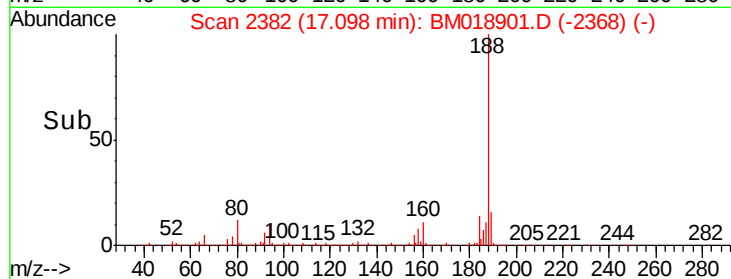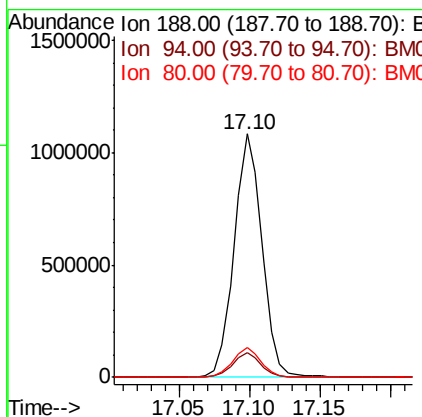

#71
Phenanthrene
Concen: 9.100 ng
RT: 17.14 min Scan# 2389
Delta R.T. -0.02 min
Lab File: BM018901.D
Acq: 21 Feb 2019 18:20

Tgt Ion:178 Resp: 728509
Ion Ratio Lower Upper
178 100
176 19.2 15.4 23.0
179 16.1 12.3 18.5

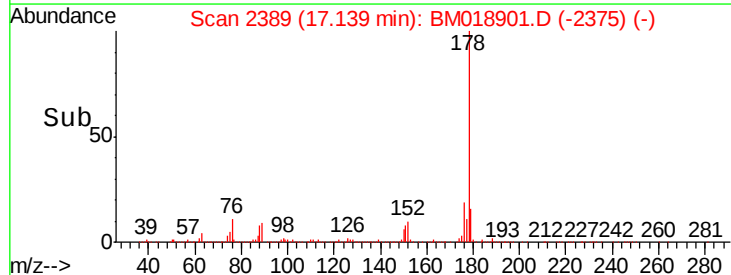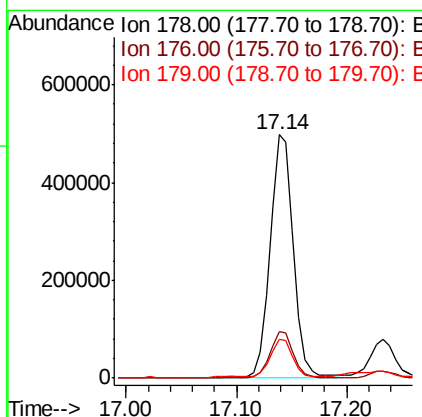

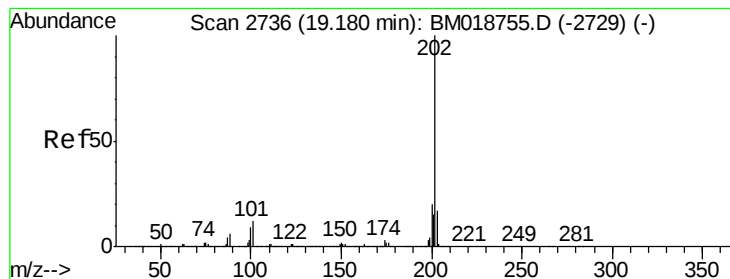

#75

Fluoranthene

Concen: 14.294 ng

RT: 19.16 min Scan# 2733

Delta R.T. -0.02 min

Lab File: BM018901.D

Acq: 21 Feb 2019 18:20

Instrument :

BNA_M

ClientSampleId :

RT-3422


Tot Ion:202 Resp: 1321888

Ion Ratio Lower Upper

202 100

101 11.9 0.0 31.5




203 17.4 0.0 37.3

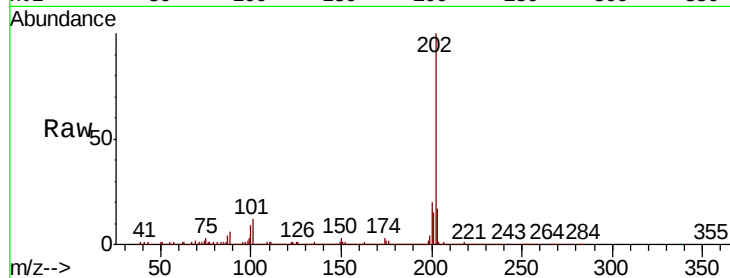

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

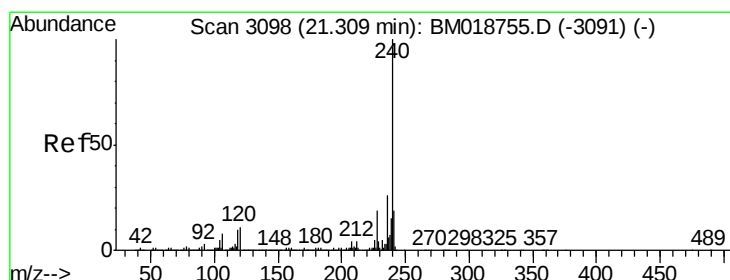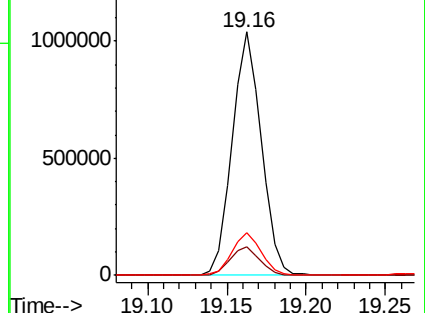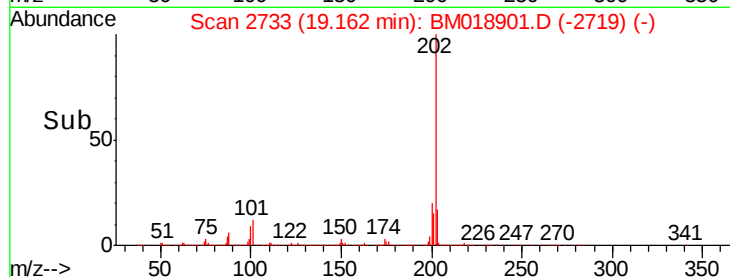

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.30 min Scan# 3096

Delta R.T. -0.01 min

Lab File: BM018901.D

Acq: 21 Feb 2019 18:20


Tgt Ion:240 Resp: 1471133

Ion Ratio Lower Upper

240 100

120 10.9 8.9 13.3



236 26.2 20.9 31.3

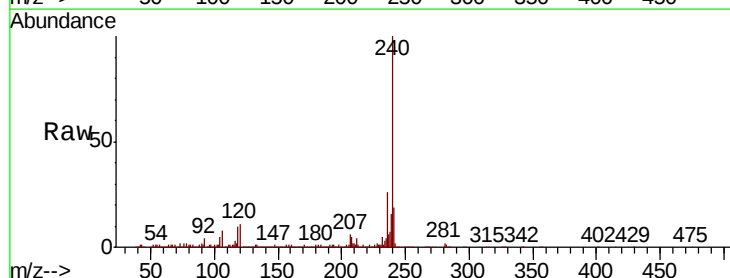


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



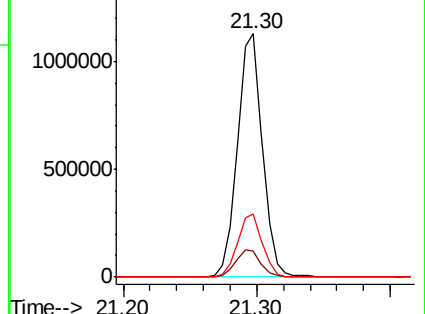
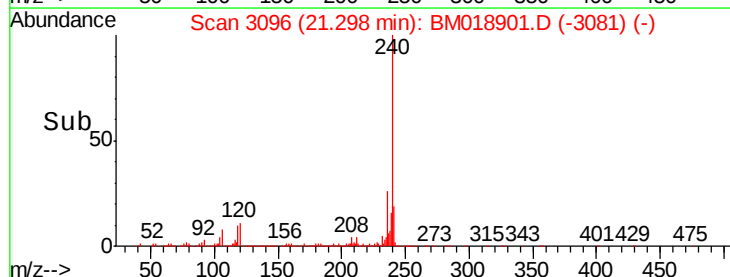




#78
Pvrene
Concen: 10.780 ng
RT: 19.53 min Scan# 2795
Delta R.T. -0.02 min
Lab File: BM018901.D
Acq: 21 Feb 2019 18:20




Instrument :
BNA_M
ClientSampleId :
RT-3422


Tot Ion	Ratio	Lower	Upper
202	100		
200	21.0	16.9	25.3
203	17.5	13.8	20.8

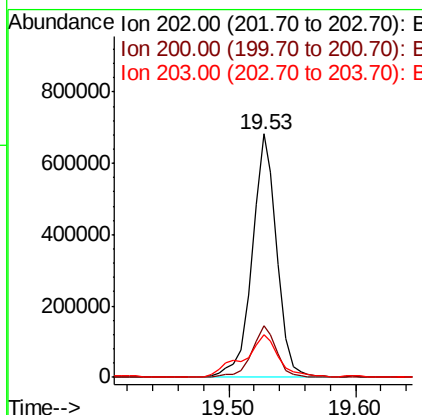

#79
Terphenyl-d14
Concen: 86.238 ng
RT: 19.73 min Scan# 2830
Delta R.T. -0.01 min
Lab File: BM018901.D
Acq: 21 Feb 2019 18:20

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.0	5.6	8.4
122	11.7	9.3	13.9

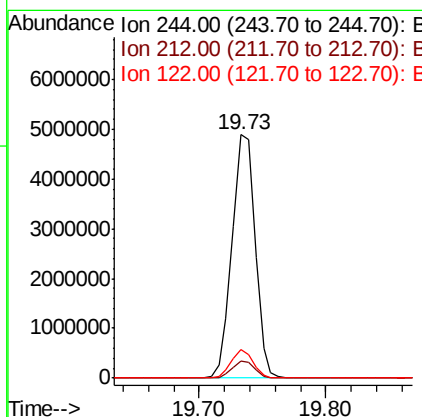

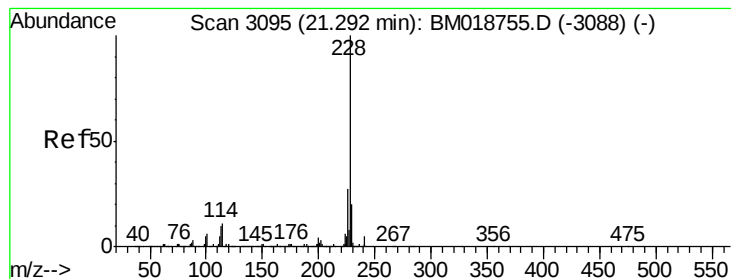

#81

Benzo(a)anthracene

Concen: 2.403 ng

RT: 21.28 min Scan# 3093

Delta R.T. -0.01 min

Lab File: BM018901.D

Acq: 21 Feb 2019 18:20

Instrument :

BNA_M

ClientSampleId :

RT-3422


Tot Ion:228 Resp: 206059

Ion Ratio Lower Upper

228 100

226 26.1 21.9 32.9

229 20.4 15.9 23.9






Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

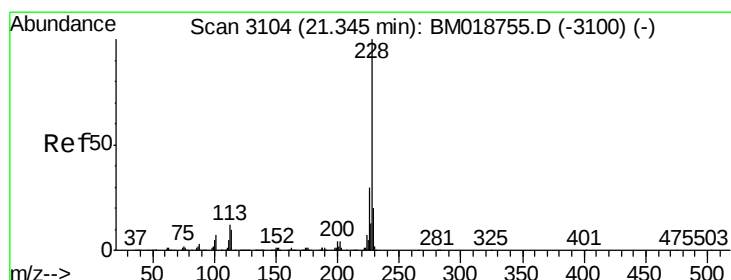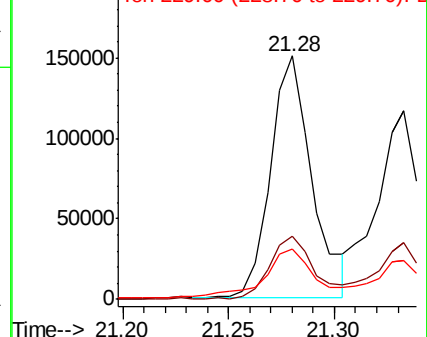

#83

Chrysene

Concen: 2.004 ng

RT: 21.33 min Scan# 3102

Delta R.T. -0.01 min

Lab File: BM018901.D

Acq: 21 Feb 2019 18:20


Tgt Ion:228 Resp: 164690

Ion Ratio Lower Upper

228 100

226 30.0 24.1 36.1

229 20.8 16.0 24.0






Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

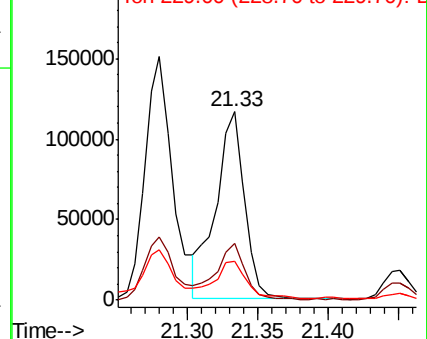



#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 23.54 min Scan# 3478
 Delta R.T. -0.02 min
 Lab File: BM018901.D
 Acq: 21 Feb 2019 18:20

Instrument :
 BNA_M
 ClientSampleId :
 RT-3422

Tot Ion: 264 Resp: 1333923
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.9 28.3
 265 22.0 17.3 25.9

