


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022119\
 Data File : BM018891.D
 Acq On : 21 Feb 2019 12:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 11 16:02:12 2019

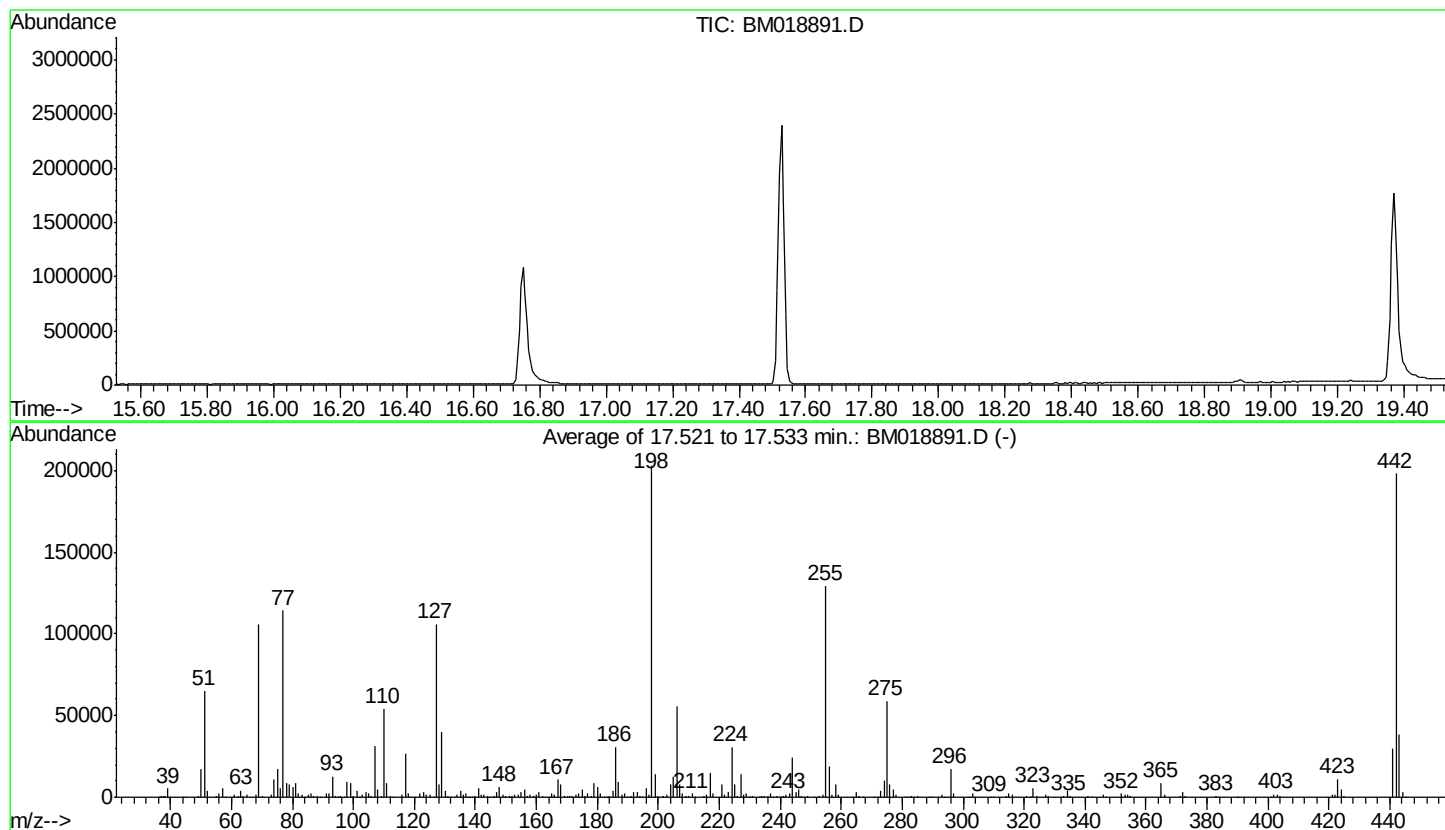

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	65104	PASS
68	69	0.00	2	1.8	1895	PASS
69	198	0.00	100	52.0	105541	PASS
70	69	0.00	2	0.4	452	PASS
127	198	10	80	52.3	106133	PASS
197	198	0.00	2	0.8	1633	PASS
198	198	100	100	100.0	202986	PASS
199	198	5	9	6.8	13871	PASS
275	198	10	60	29.0	58776	PASS
365	198	1	100	4.3	8670	PASS
441	198	0.01	100	14.8	30128	PASS
442	198	50	100	97.8	198421	PASS
443	442	15	24	19.5	38634	PASS