

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
 Data File : BM044224.D
 Acq On : 21 Feb 2024 19:12
 Operator : MA/JU
 Sample : P1493-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3X1

Quant Time: Feb 21 22:43:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.896	152	3948	0.400	ng/ul	0.00
4) Naphthalene-d8	10.694	136	12191	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.538	164	6610	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.389	188	1527875	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.50
23) Perylene-d12	23.885	264	19137	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	23841	4.264	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.288	152	8610	0.504	ng/ul	-0.01
18) Fluoranthene-d10	19.326	212	18236	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.537	166	2903	0.098	ng/ul#	13
26) Benzo(a)pyrene	23.733	252	6119	0.083	ng/ul#	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
Data File : BM044224.D
Acq On : 21 Feb 2024 19:12
Operator : MA/JU
Sample : P1493-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3X1

Quant Time: Feb 21 22:43:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration

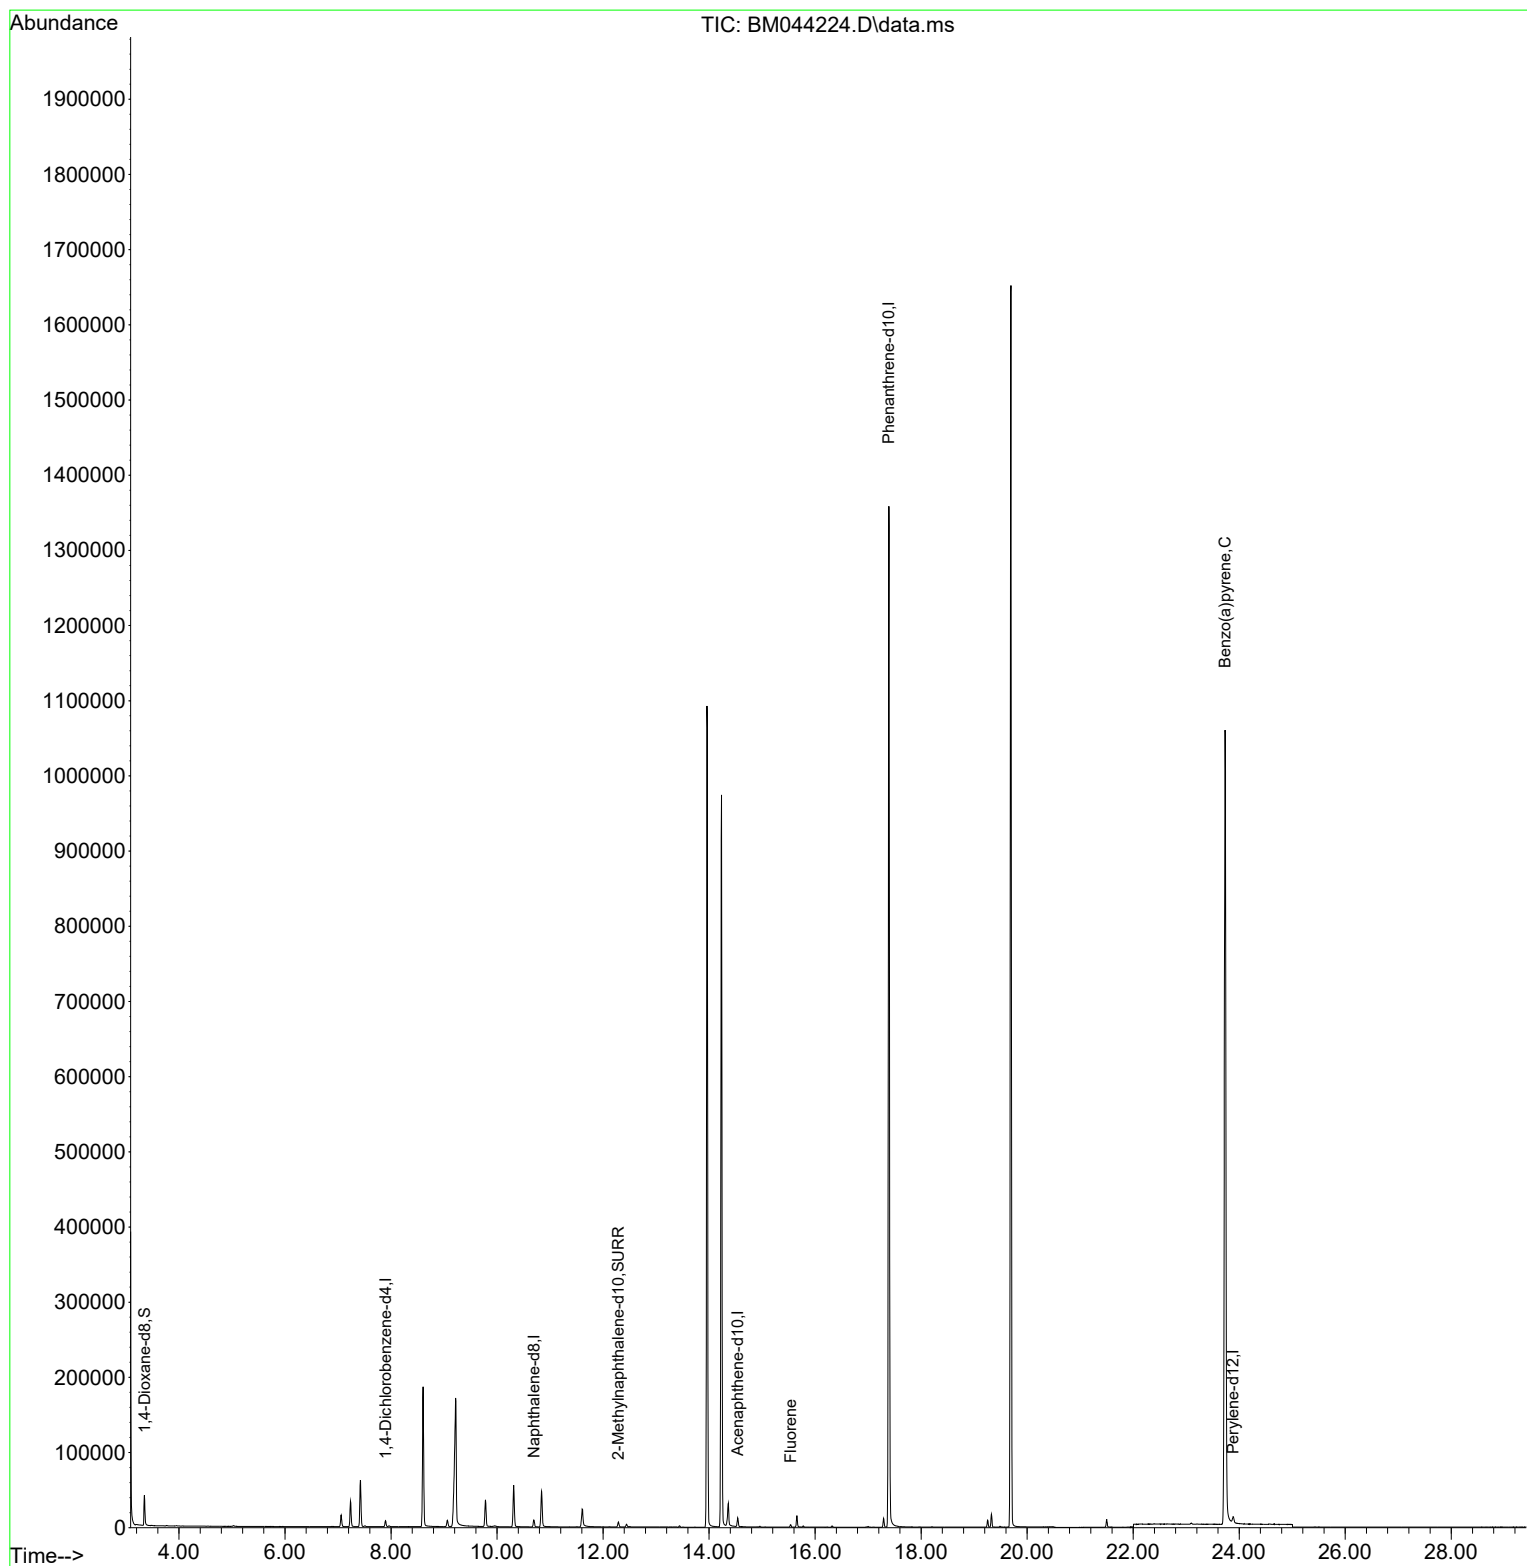

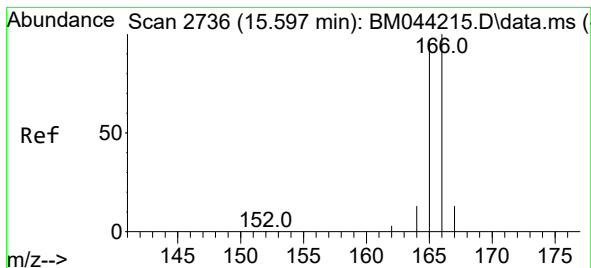

#12

Fluorene

Concen: 0.098 ng/ul

RT: 15.537 min Scan# 21

Delta R.T. -0.060 min

Lab File: BM044224.D

Acq: 21 Feb 2024 19:12

Instrument :

BNA_M

ClientSampleId :

BH3X1





Tgt Ion:166 Resp: 2903

Ion Ratio Lower Upper

166 100

165 7.3 79.8 119.6#

167 34.7 11.1 16.7#

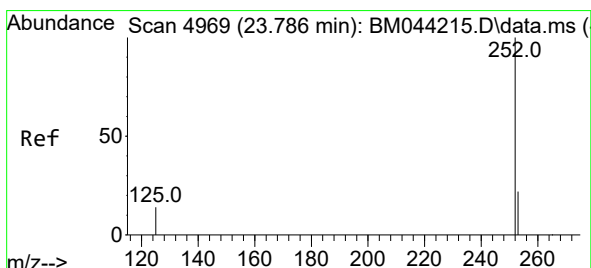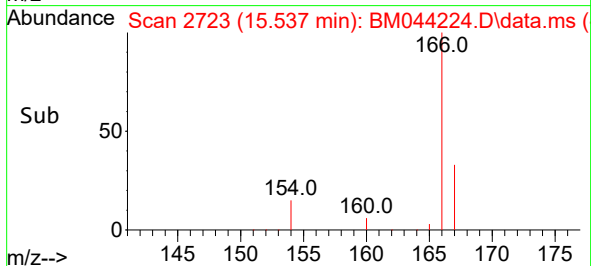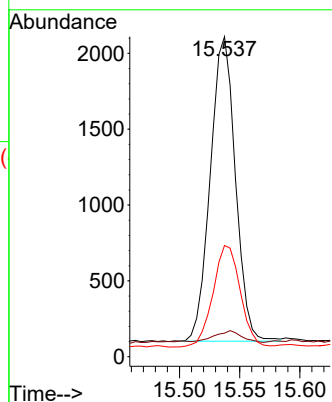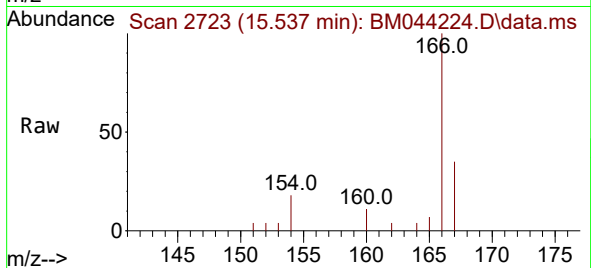

#26

Benzo(a)pyrene

Concen: 0.083 ng/ul

RT: 23.733 min Scan# 4951

Delta R.T. -0.052 min

Lab File: BM044224.D

Acq: 21 Feb 2024 19:12

Tgt Ion:252 Resp: 6119

Ion Ratio Lower Upper

252 100

253 46.4 21.4 32.2#

125 61.0 13.3 19.9#

