

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
 Data File : BM044226.D
 Acq On : 21 Feb 2024 20:25
 Operator : MA/JU
 Sample : P1493-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH407

Quant Time: Feb 21 22:43:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 15 13:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.896	152	4328	0.400	ng/ul	0.00
4) Naphthalene-d8	10.694	136	13175	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.538	164	6545	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.389	188	1401477	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.50
23) Perylene-d12	23.882	264	18073	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	28687	4.680	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.288	152	8287	0.449	ng/ul	-0.01
18) Fluoranthene-d10	19.326	212	15782	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.537	166	2753	0.094	ng/ul#	13
26) Benzo(a)pyrene	23.733	252	5537	0.080	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022124\
Data File : BM044226.D
Acq On : 21 Feb 2024 20:25
Operator : MA/JU
Sample : P1493-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH407

Quant Time: Feb 21 22:43:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM021524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 13:40:24 2024
Response via : Initial Calibration




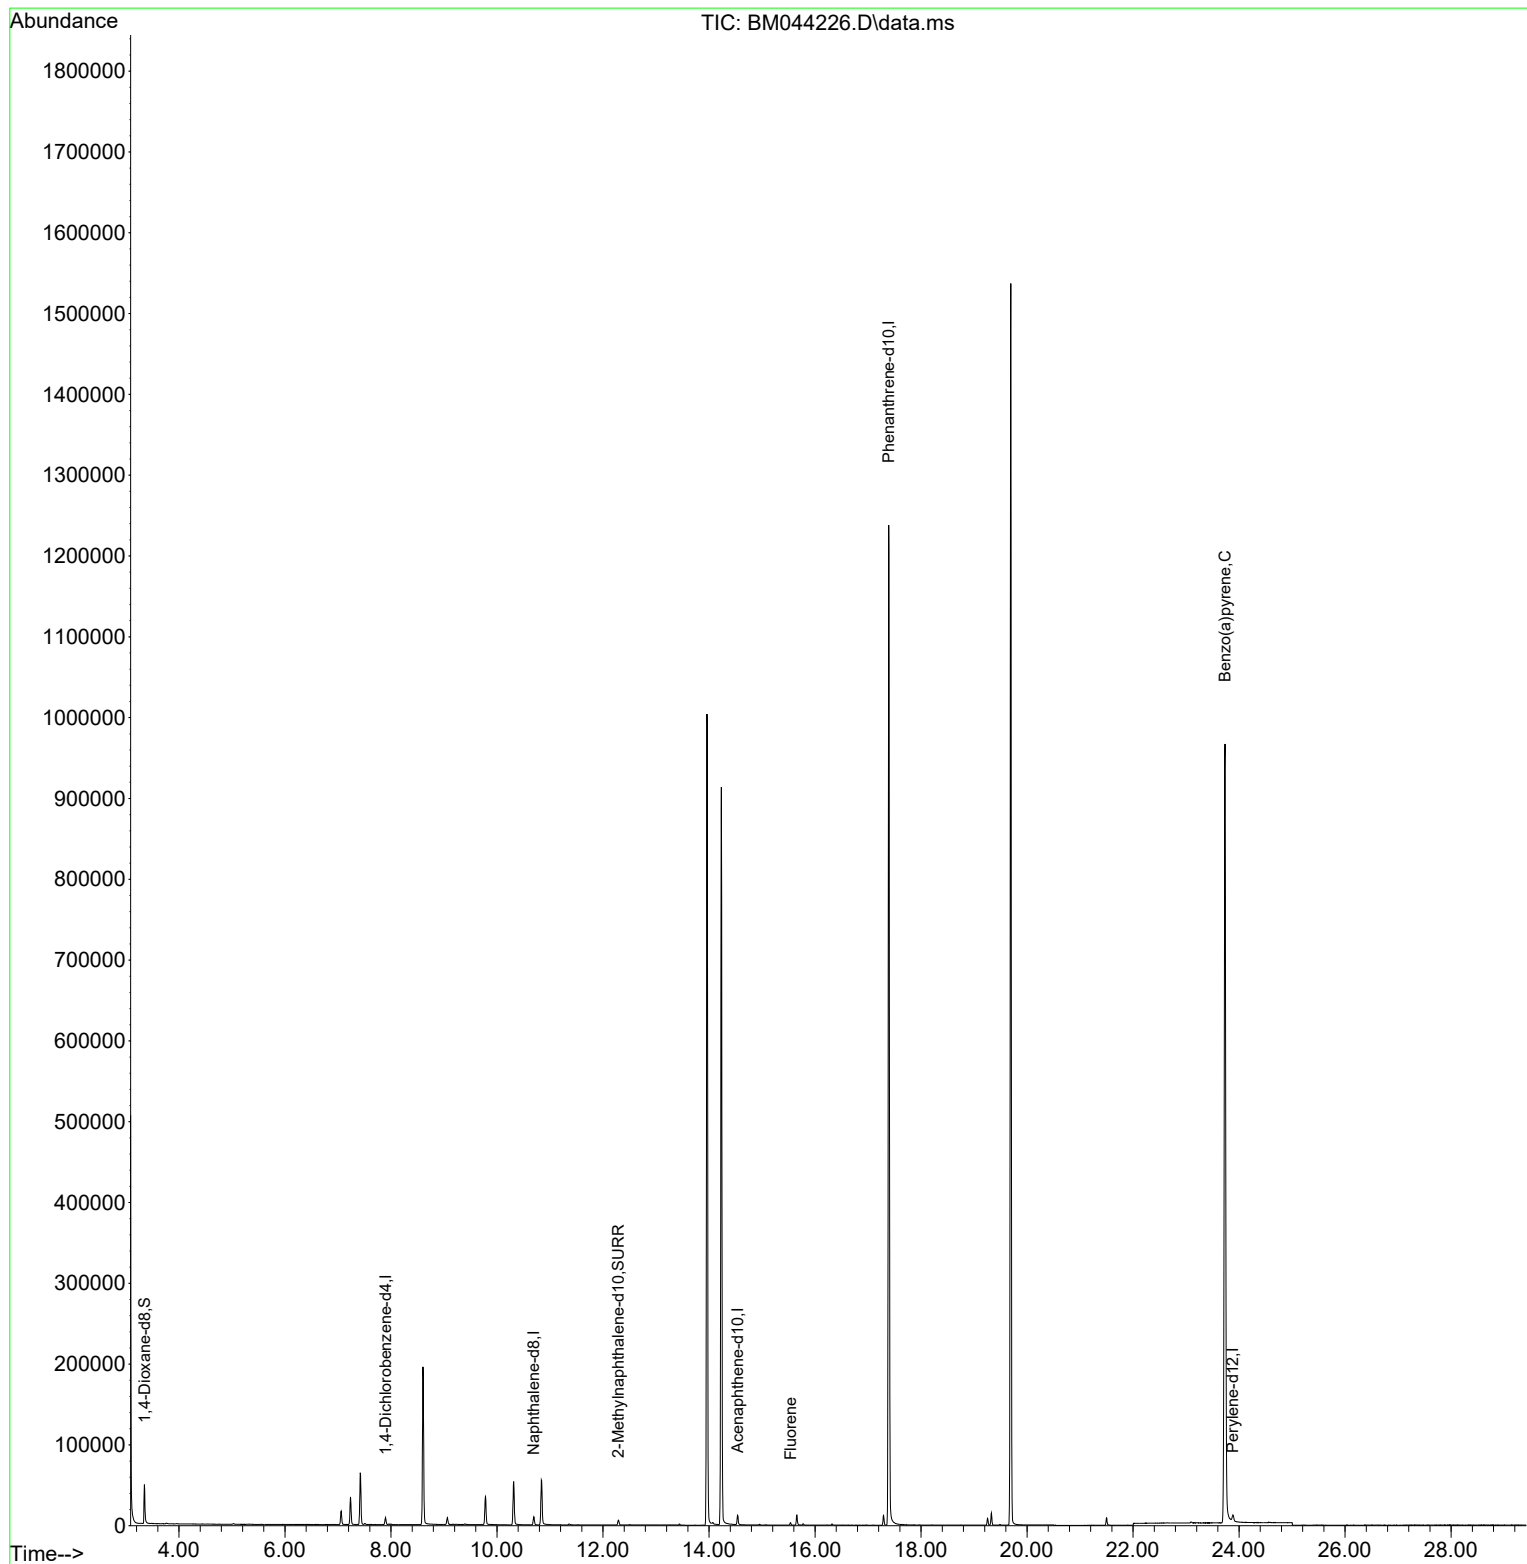


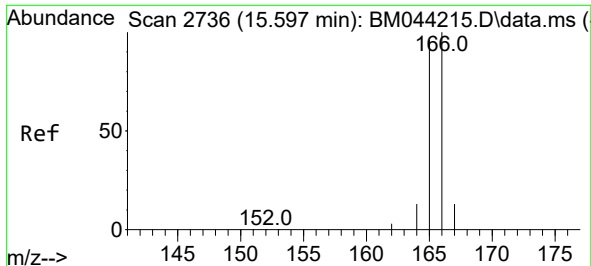

#12
Fluorene
Concen: 0.094 ng/ul
RT: 15.537 min Scan# 21
Delta R.T. -0.060 min
Lab File: BM044226.D
Acq: 21 Feb 2024 20:25

Instrument :
BNA_M
ClientSampleId :
BH407

Tgt Ion:166 Resp: 2753
Ion Ratio Lower Upper
166 100
165 7.7 79.8 119.6#
167 35.8 11.1 16.7#

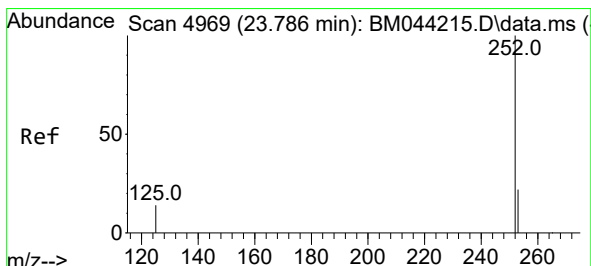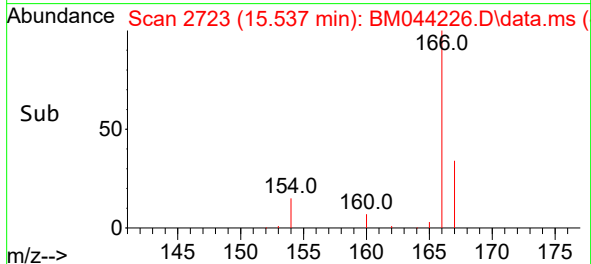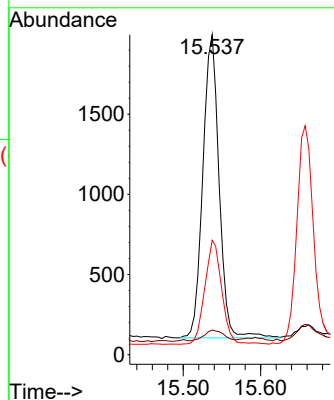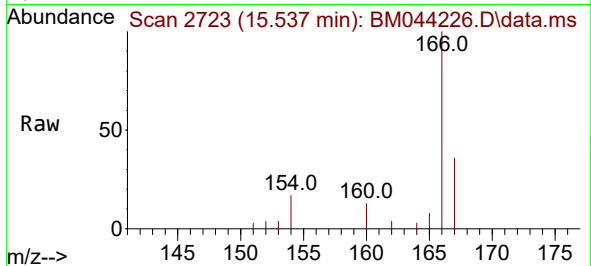

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.733 min Scan# 4951
Delta R.T. -0.053 min
Lab File: BM044226.D
Acq: 21 Feb 2024 20:25

Tgt Ion:252 Resp: 5537
Ion Ratio Lower Upper
252 100
253 46.3 21.4 32.2#
125 37.0 13.3 19.9#

